

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029773.D
 Acq On : 22 Dec 2022 20:59
 Operator : SY/MD
 Sample : N6195-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP2

Quant Time: Dec 23 02:10:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 21 00:15:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	473790	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	457419	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	244295	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	164715	56.773	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	113.540%
7) Chloroethane-d5	1.564	69	136737	61.807	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	123.620%
11) 1,1-Dichloroethene-d2	2.105	63	205692	45.454	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.900%
21) 2-Butanone-d5	3.870	46	181078	102.312	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.310%
24) Chloroform-d	4.339	84	269398	49.343	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.680%
26) 1,2-Dichloroethane-d4	5.021	65	163001	52.274	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.540%
32) Benzene-d6	5.043	84	592137	48.991	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.980%
36) 1,2-Dichloropropane-d6	6.059	67	184638	50.012	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	100.020%
41) Toluene-d8	7.307	98	521978	45.835	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.660%
43) trans-1,3-Dichloroprop...	7.612	79	75868	40.696	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.400%
47) 2-Hexanone-d5	8.082	63	148619	94.270	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.270%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	253474	48.046	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.100%
66) 1,2-Dichlorobenzene-d4	11.612	152	209094	44.962	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.920%
Target Compounds						
					Qvalue	
13) Acetone	2.159	43	8368	7.258	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029773.D
Acq On : 22 Dec 2022 20:59
Operator : SY/MD
Sample : N6195-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP2

Quant Time: Dec 23 02:10:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 21 00:15:13 2022
Response via : Initial Calibration

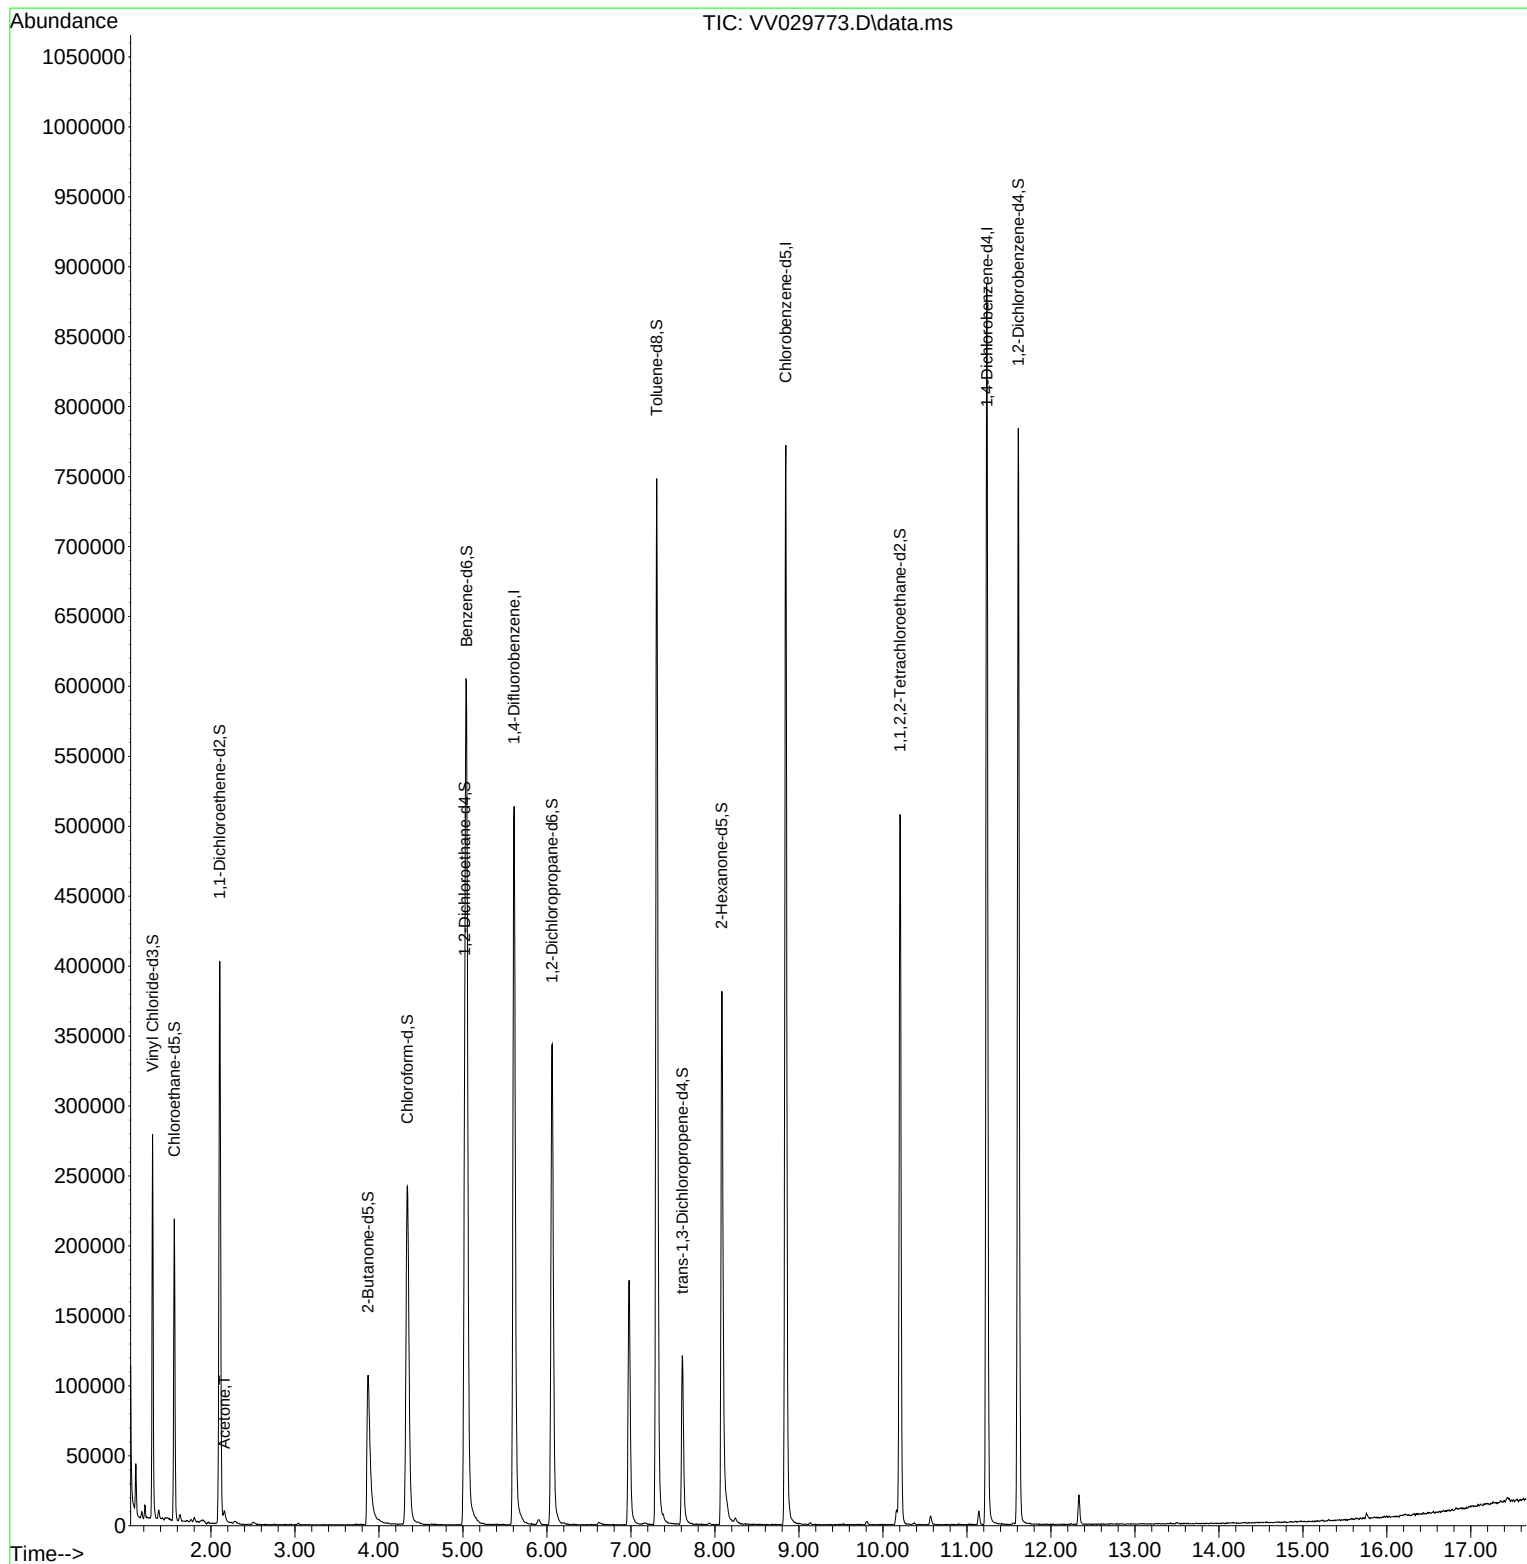

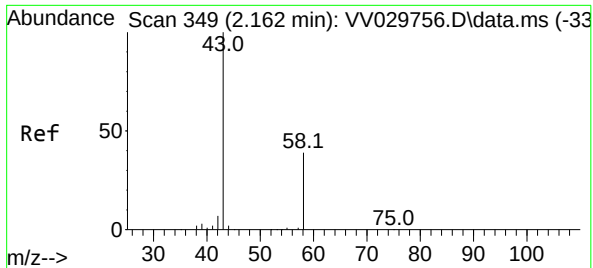

#13
 Acetone
 Concen: 7.258 ug/L
 RT: 2.159 min Scan# 34
 Delta R.T. -0.003 min
 Lab File: VV029773.D
 Acq: 22 Dec 2022 20:59

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP2

Tgt Ion: 43 Resp: 8368
 Ion Ratio Lower Upper
 43 100
 58 35.7 0.0 74.8

