

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029757.D
 Acq On : 22 Dec 2022 11:42
 Operator : SY/MD
 Sample : VV1222WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK313

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029757.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	193721	197686	13.26%	1.639%
2	1.564	155	163	176	rVB	185092	203905	13.67%	1.691%
3	2.050	312	314	316	rBV	492	245	0.02%	0.002%
4	2.105	320	331	348	rBV	331081	480057	32.19%	3.981%
5	2.394	417	421	422	rBV	416	291	0.02%	0.002%
6	2.471	438	445	447	rBV4	408	474	0.03%	0.004%
7	2.500	447	454	465	rVB	4223	6529	0.44%	0.054%
8	3.326	709	711	720	rVB3	331	286	0.02%	0.002%
9	3.796	852	857	861	rBV3	286	329	0.02%	0.003%
10	3.876	871	882	926	rBV	114821	353893	23.73%	2.934%
11	4.339	1008	1026	1058	rBV	231009	592138	39.71%	4.910%
12	4.706	1137	1140	1145	rVV3	239	253	0.02%	0.002%
13	4.773	1157	1161	1165	rBV2	268	254	0.02%	0.002%
14	4.957	1216	1218	1222	rVB2	369	238	0.02%	0.002%
15	5.037	1222	1243	1284	rBV2	565681	1491166	100.00%	12.364%
16	5.391	1349	1353	1357	rBV2	312	303	0.02%	0.003%
17	5.433	1362	1366	1369	rBV	327	332	0.02%	0.003%
18	5.523	1389	1394	1398	rVB3	463	446	0.03%	0.004%
19	5.609	1408	1421	1457	rBV	512065	1052701	70.60%	8.729%
20	5.899	1501	1511	1523	rBV6	4447	10064	0.67%	0.083%
21	6.063	1547	1562	1582	rBV	329401	677575	45.44%	5.618%
22	6.236	1614	1616	1619	rVB2	744	430	0.03%	0.004%
23	6.423	1670	1674	1678	rVV2	300	229	0.02%	0.002%
24	6.545	1708	1712	1716	rVB2	338	324	0.02%	0.003%
25	6.616	1728	1734	1736	rBV5	349	319	0.02%	0.003%
26	6.638	1738	1741	1745	rVB3	428	249	0.02%	0.002%
27	6.828	1794	1800	1801	rBV	275	261	0.02%	0.002%
28	6.879	1812	1816	1818	rBV	301	245	0.02%	0.002%
29	6.979	1835	1847	1885	rVV	164533	303199	20.33%	2.514%
30	7.307	1936	1949	1986	rBV	678712	1207035	80.95%	10.008%
31	7.513	2009	2013	2014	rBV3	563	379	0.03%	0.003%
32	7.612	2032	2044	2074	rBV	116163	205787	13.80%	1.706%
33	7.767	2090	2092	2097	rBV4	551	380	0.03%	0.003%
34	7.886	2124	2129	2130	rBV2	306	244	0.02%	0.002%
35	7.969	2153	2155	2161	rVB3	381	316	0.02%	0.003%
36	8.085	2180	2191	2222	rBV	389437	727288	48.77%	6.030%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029757.D
 Acq On : 22 Dec 2022 11:42
 Operator : SY/MD
 Sample : VV1222WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK313

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	8.410	2284	2292	2299	rBV4	1593	2290	0.15%	0.019%
38	8.484	2310	2315	2316	rVV2	406	242	0.02%	0.002%
39	8.567	2337	2341	2343	rBV3	326	267	0.02%	0.002%
40	8.680	2370	2376	2380	rVB4	326	315	0.02%	0.003%
41	8.738	2390	2394	2395	rBV	468	282	0.02%	0.002%
42	8.764	2399	2402	2405	rBV	473	346	0.02%	0.003%
43	8.844	2410	2427	2457	rBV	742805	1242949	83.35%	10.306%
44	9.008	2474	2478	2489	rVB7	1325	1752	0.12%	0.015%
45	9.137	2512	2518	2524	rVV3	1163	1496	0.10%	0.012%
46	9.165	2525	2527	2531	rVB2	491	267	0.02%	0.002%
47	9.220	2540	2544	2547	rBV2	590	425	0.03%	0.004%
48	9.246	2547	2552	2555	rVV3	289	299	0.02%	0.002%
49	9.384	2589	2595	2600	rBV3	547	417	0.03%	0.003%
50	9.448	2612	2615	2621	rBV2	306	270	0.02%	0.002%
51	9.551	2638	2647	2650	rBV5	1006	1445	0.10%	0.012%
52	9.632	2667	2672	2675	rBV	282	288	0.02%	0.002%
53	9.648	2675	2677	2682	rVV2	341	288	0.02%	0.002%
54	9.670	2682	2684	2689	rVV4	326	275	0.02%	0.002%
55	9.719	2695	2699	2707	rBV2	302	362	0.02%	0.003%
56	9.815	2725	2729	2732	rVV	418	379	0.03%	0.003%
57	9.844	2734	2738	2742	rVV3	459	415	0.03%	0.003%
58	9.921	2755	2762	2770	rBV4	770	1187	0.08%	0.010%
59	9.979	2776	2780	2781	rBV2	366	268	0.02%	0.002%
60	10.001	2784	2787	2790	rBV3	319	257	0.02%	0.002%
61	10.162	2828	2837	2840	rBV2	11192	14701	0.99%	0.122%
62	10.204	2840	2850	2871	rVB	510133	805913	54.05%	6.682%
63	10.374	2894	2903	2909	rBV3	1237	1945	0.13%	0.016%
64	10.477	2932	2935	2939	rBV3	313	227	0.02%	0.002%
65	10.567	2956	2963	2973	rVB2	5949	8716	0.58%	0.072%
66	10.738	3012	3016	3017	rBV2	433	295	0.02%	0.002%
67	10.773	3022	3027	3031	rBV2	322	429	0.03%	0.004%
68	10.905	3061	3068	3076	rBV4	1032	1949	0.13%	0.016%
69	10.963	3081	3086	3091	rBV2	338	434	0.03%	0.004%
70	11.014	3100	3102	3106	rVB2	330	229	0.02%	0.002%
71	11.153	3141	3145	3146	rBV	410	309	0.02%	0.003%
72	11.169	3146	3150	3151	rBV2	1511	955	0.06%	0.008%
73	11.236	3159	3171	3199	rBV	792797	1240719	83.20%	10.288%
74	11.503	3251	3254	3257	rBV2	352	247	0.02%	0.002%
75	11.522	3257	3260	3266	rVB3	256	241	0.02%	0.002%
76	11.612	3276	3288	3308	rBV	727867	1144153	76.73%	9.487%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029757.D
 Acq On : 22 Dec 2022 11:42
 Operator : SY/MD
 Sample : VV1222WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK313

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.934	3387	3388	3393	rVV3	480	351	0.02%	0.003%
78	11.960	3393	3396	3403	rVB2	411	444	0.03%	0.004%
79	11.995	3403	3407	3413	rBV2	470	538	0.04%	0.004%
80	12.027	3413	3417	3425	rVB3	507	638	0.04%	0.005%
81	12.066	3425	3429	3435	rBV3	293	451	0.03%	0.004%
82	12.194	3466	3469	3473	rBV	276	236	0.02%	0.002%
83	12.236	3473	3482	3491	rBV3	1136	2187	0.15%	0.018%
84	12.490	3555	3561	3563	rBV2	470	435	0.03%	0.004%
85	12.551	3578	3580	3583	rBV	323	227	0.02%	0.002%
86	12.635	3595	3606	3614	rBV5	2409	3881	0.26%	0.032%
87	12.783	3649	3652	3653	rBV	412	230	0.02%	0.002%
88	12.831	3664	3667	3673	rBV4	1146	1136	0.08%	0.009%
89	12.911	3689	3692	3694	rVB2	472	305	0.02%	0.003%
90	12.969	3707	3710	3712	rBV2	424	286	0.02%	0.002%
91	13.040	3727	3732	3734	rBV4	493	352	0.02%	0.003%
92	13.175	3771	3774	3776	rBV	466	319	0.02%	0.003%
93	13.252	3790	3798	3811	rVB6	4465	7626	0.51%	0.063%
94	13.413	3846	3848	3852	rVB3	783	458	0.03%	0.004%
95	13.493	3858	3873	3889	rBV	21014	36215	2.43%	0.300%
96	13.615	3909	3911	3914	rBV2	643	364	0.02%	0.003%
97	13.731	3939	3947	3960	rVB6	4673	8160	0.55%	0.068%
98	13.779	3960	3962	3967	rVB2	472	242	0.02%	0.002%
99	14.152	4076	4078	4080	rBV2	459	304	0.02%	0.003%
100	14.484	4178	4181	4187	rBV4	649	716	0.05%	0.006%




Sum of corrected areas: 12060194

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029757.D
Acq On : 22 Dec 2022 11:42
Operator : SY/MD
Sample : VV1222WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK313

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

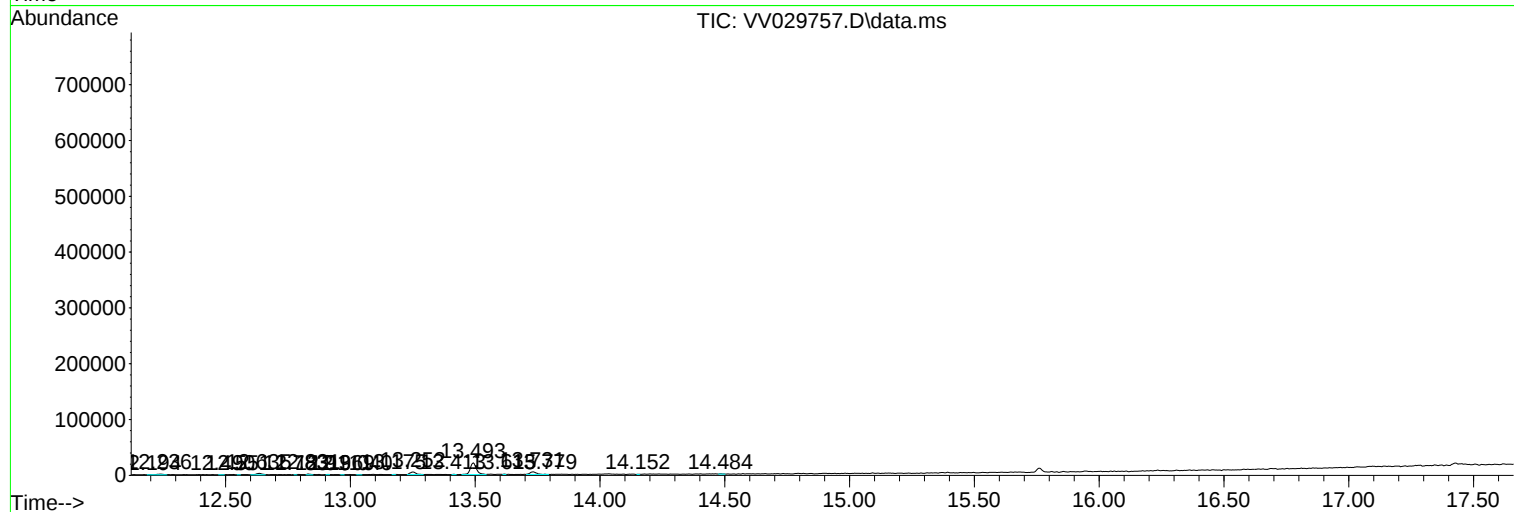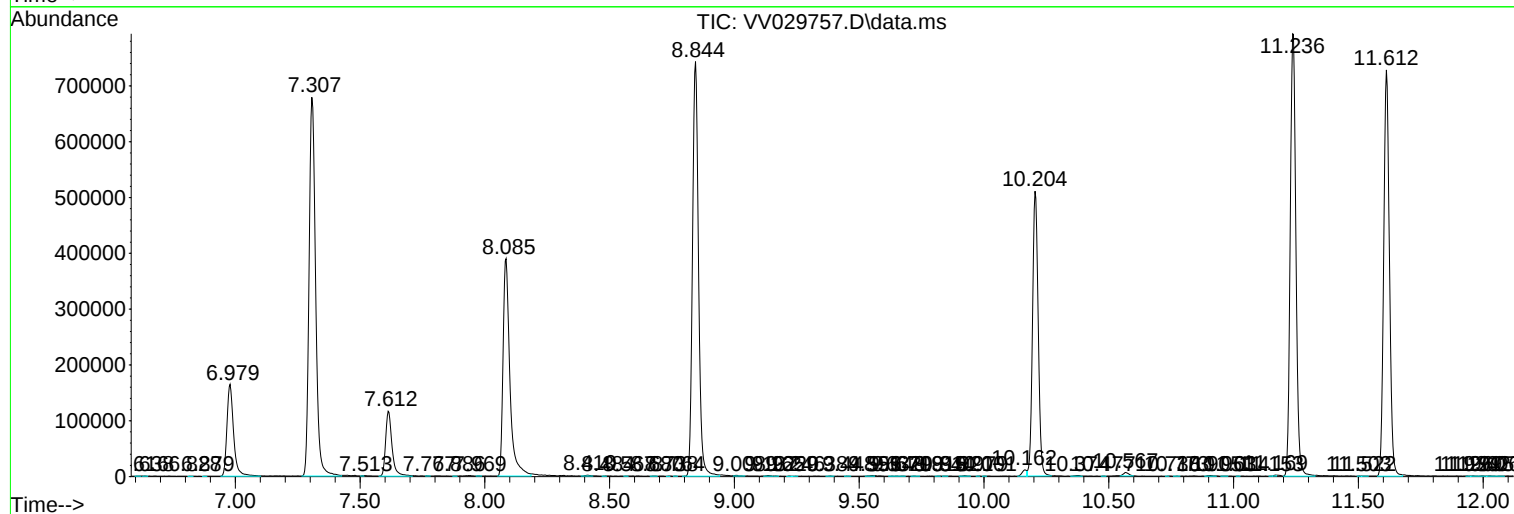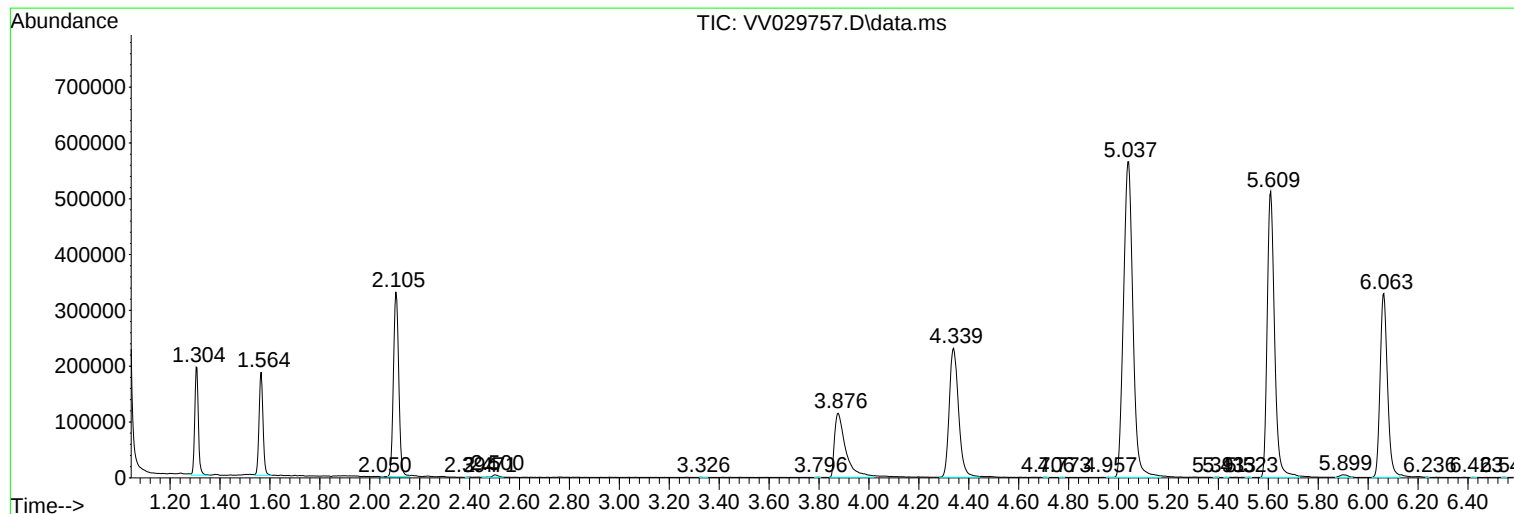

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029757.D
Acq On : 22 Dec 2022 11:42
Operator : SY/MD
Sample : VV1222WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK313

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029757.D
Acq On : 22 Dec 2022 11:42
Operator : SY/MD
Sample : VV1222WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK313

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc