

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029758.D
 Acq On : 22 Dec 2022 15:07
 Operator : SY/MD
 Sample : N6193-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	300901	304345	15.96%	2.094%
2	1.565	155	163	179	rVB	260136	293556	15.39%	2.019%
3	2.102	319	330	346	rBV	487441	700030	36.71%	4.815%
4	3.558	779	783	785	rBV	578	469	0.02%	0.003%
5	3.867	869	879	917	rBV	122742	352816	18.50%	2.427%
6	4.333	1007	1024	1052	rBV	285778	743275	38.97%	5.113%
7	4.635	1115	1118	1121	rBV3	506	389	0.02%	0.003%
8	5.034	1224	1242	1293	rBV2	718145	1907120	100.00%	13.119%
9	5.519	1390	1393	1395	rBV2	781	487	0.03%	0.003%
10	5.603	1406	1419	1447	rBV	540069	1095595	57.45%	7.536%
11	5.896	1499	1510	1523	rBV4	4206	9032	0.47%	0.062%
12	6.056	1545	1560	1597	rBV	404161	843587	44.23%	5.803%
13	6.503	1696	1699	1704	rBV2	575	542	0.03%	0.004%
14	6.609	1725	1732	1738	rBV5	2457	3824	0.20%	0.026%
15	6.973	1833	1845	1868	rBV	214588	390720	20.49%	2.688%
16	7.304	1934	1948	1981	rBV	900553	1574226	82.54%	10.829%
17	7.609	2032	2043	2068	rVV	148205	260374	13.65%	1.791%
18	7.851	2112	2118	2124	rBV4	682	1056	0.06%	0.007%
19	7.931	2134	2143	2152	rBV2	3820	6445	0.34%	0.044%
20	7.995	2159	2163	2165	rBV2	552	432	0.02%	0.003%
21	8.079	2179	2189	2231	rBV	441224	820336	43.01%	5.643%
22	8.368	2275	2279	2284	rBV3	541	590	0.03%	0.004%
23	8.523	2324	2327	2330	rBV	454	399	0.02%	0.003%
24	8.677	2369	2375	2380	rBV2	569	703	0.04%	0.005%
25	8.841	2413	2426	2451	rBV	808774	1334918	70.00%	9.183%
26	9.005	2475	2477	2485	rVB3	739	827	0.04%	0.006%
27	9.320	2571	2575	2577	rBV3	518	376	0.02%	0.003%
28	9.487	2616	2627	2633	rBV3	613	1084	0.06%	0.007%
29	9.838	2734	2736	2738	rBV2	577	380	0.02%	0.003%
30	10.092	2809	2815	2822	rBV2	615	923	0.05%	0.006%
31	10.162	2827	2837	2839	rBV3	13524	17555	0.92%	0.121%
32	10.204	2840	2850	2873	rVB	583505	920816	48.28%	6.334%
33	10.349	2890	2895	2896	rBV3	632	549	0.03%	0.004%
34	10.371	2896	2902	2910	rVB4	4146	6162	0.32%	0.042%
35	10.413	2911	2915	2918	rVB2	442	398	0.02%	0.003%
36	10.448	2923	2926	2935	rVB3	550	612	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029758.D
 Acq On : 22 Dec 2022 15:07
 Operator : SY/MD
 Sample : N6193-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	10.567	2953	2963	2978	rVB2	8415	13887	0.73%	0.096%
38	10.648	2983	2988	2994	rVB3	583	687	0.04%	0.005%
39	10.686	2994	3000	3006	rVB2	442	365	0.02%	0.003%
40	10.799	3029	3035	3039	rVV2	634	722	0.04%	0.005%
41	10.841	3044	3048	3051	rVB2	767	685	0.04%	0.005%
42	10.911	3067	3070	3080	rVB5	820	1055	0.06%	0.007%
43	10.953	3080	3083	3090	rVB3	709	809	0.04%	0.006%
44	10.985	3090	3093	3096	rBV	410	354	0.02%	0.002%
45	11.040	3103	3110	3113	rBV2	495	551	0.03%	0.004%
46	11.172	3148	3151	3157	rVB2	977	860	0.05%	0.006%
47	11.236	3158	3171	3192	rBV	941716	1449566	76.01%	9.971%
48	11.429	3227	3231	3238	rVB3	676	752	0.04%	0.005%
49	11.612	3275	3288	3315	rBV	901107	1421927	74.56%	9.781%
50	11.757	3330	3333	3337	rVB4	903	705	0.04%	0.005%
51	11.789	3337	3343	3346	rBV2	353	379	0.02%	0.003%
52	11.828	3351	3355	3360	rBV3	612	635	0.03%	0.004%
53	11.895	3369	3376	3379	rBV3	608	685	0.04%	0.005%
54	12.001	3406	3409	3412	rBV3	397	363	0.02%	0.002%
55	12.120	3444	3446	3452	rVV2	379	378	0.02%	0.003%
56	12.149	3452	3455	3462	rVB3	683	804	0.04%	0.006%
57	12.178	3462	3464	3466	rBV	673	398	0.02%	0.003%
58	12.272	3489	3493	3496	rVB2	642	474	0.02%	0.003%
59	12.339	3509	3514	3518	rVB2	763	589	0.03%	0.004%
60	12.374	3520	3525	3528	rBV3	390	372	0.02%	0.003%
61	12.442	3532	3546	3559	rBV5	7202	13702	0.72%	0.094%
62	12.500	3562	3564	3569	rVB2	694	463	0.02%	0.003%
63	12.538	3574	3576	3581	rVB2	559	361	0.02%	0.002%
64	12.622	3598	3602	3604	rBV3	786	651	0.03%	0.004%
65	12.673	3615	3618	3622	rVV	473	396	0.02%	0.003%
66	12.712	3627	3630	3633	rBV3	417	409	0.02%	0.003%
67	12.786	3646	3653	3654	rBV3	401	452	0.02%	0.003%
68	12.821	3658	3664	3665	rBV3	652	477	0.03%	0.003%
69	12.834	3665	3668	3671	rVV3	788	565	0.03%	0.004%
70	12.937	3693	3700	3703	rBV3	497	548	0.03%	0.004%
71	12.976	3709	3712	3715	rBV2	586	459	0.02%	0.003%
72	13.024	3725	3727	3732	rVB2	664	365	0.02%	0.003%
73	13.053	3732	3736	3740	rVB2	483	348	0.02%	0.002%
74	13.088	3743	3747	3752	rVB2	652	467	0.02%	0.003%
75	13.297	3807	3812	3815	rVB4	624	524	0.03%	0.004%
76	13.317	3815	3818	3822	rBV3	495	488	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029758.D
 Acq On : 22 Dec 2022 15:07
 Operator : SY/MD
 Sample : N6193-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	13.374	3832	3836	3839	rVB2	708	411	0.02%	0.003%
78	13.429	3851	3853	3855	rBV	651	350	0.02%	0.002%
79	13.497	3865	3874	3887	rBV2	4829	7532	0.39%	0.052%
80	13.599	3901	3906	3907	rBV2	551	442	0.02%	0.003%
81	13.632	3913	3916	3919	rBV	732	610	0.03%	0.004%
82	13.702	3932	3938	3939	rBV3	394	396	0.02%	0.003%
83	13.731	3940	3947	3955	rVB6	1588	1950	0.10%	0.013%
84	13.873	3988	3991	3998	rVB4	719	609	0.03%	0.004%
85	13.915	3998	4004	4009	rBV5	866	1213	0.06%	0.008%
86	13.956	4014	4017	4022	rBV4	1193	1276	0.07%	0.009%
87	14.027	4034	4039	4042	rBV4	945	887	0.05%	0.006%
88	14.124	4065	4069	4070	rBV3	541	406	0.02%	0.003%
89	14.201	4090	4093	4096	rBV2	710	435	0.02%	0.003%
90	14.316	4126	4129	4133	rVB3	601	417	0.02%	0.003%
91	14.339	4133	4136	4139	rBV	646	355	0.02%	0.002%
92	14.419	4156	4161	4166	rBV4	766	1009	0.05%	0.007%
93	14.471	4175	4177	4180	rBV4	582	347	0.02%	0.002%
94	14.490	4180	4183	4185	rBV3	821	654	0.03%	0.004%
95	14.551	4198	4202	4204	rBV3	684	615	0.03%	0.004%
96	14.651	4230	4233	4237	rVB3	901	601	0.03%	0.004%
97	14.799	4274	4279	4280	rBV3	1205	960	0.05%	0.007%
98	14.847	4291	4294	4296	rBV3	869	644	0.03%	0.004%
99	14.947	4323	4325	4327	rBV3	931	557	0.03%	0.004%
100	15.220	4406	4410	4412	rBV4	1035	909	0.05%	0.006%




Sum of corrected areas: 14537210

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029758.D
Acq On : 22 Dec 2022 15:07
Operator : SY/MD
Sample : N6193-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

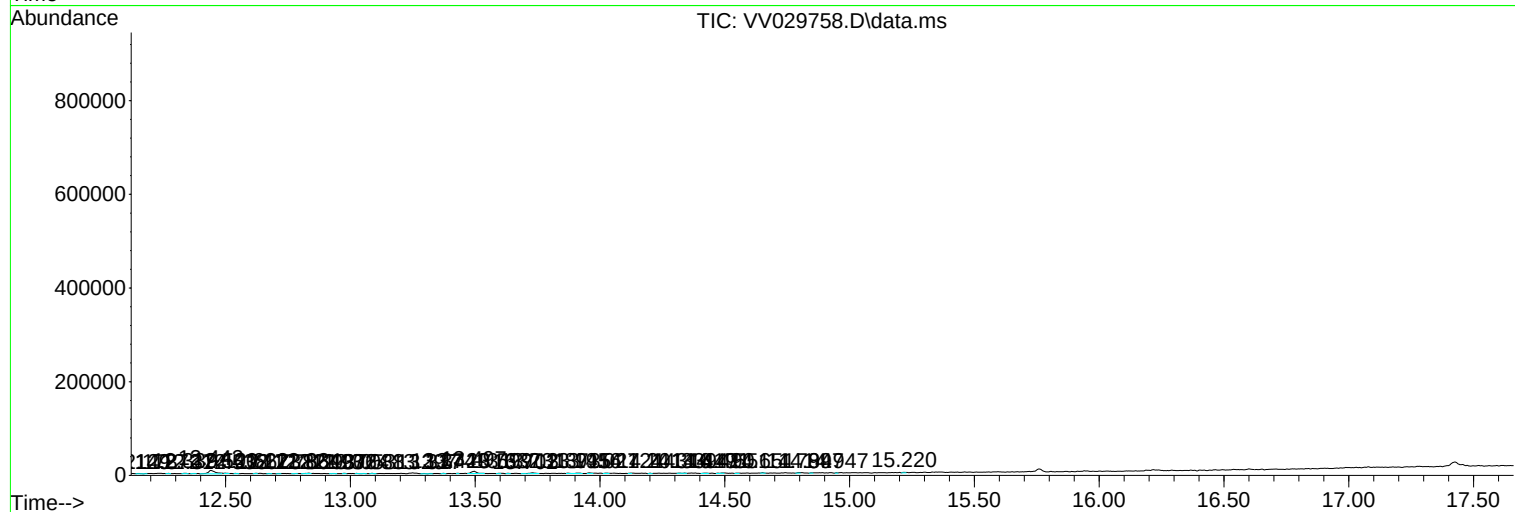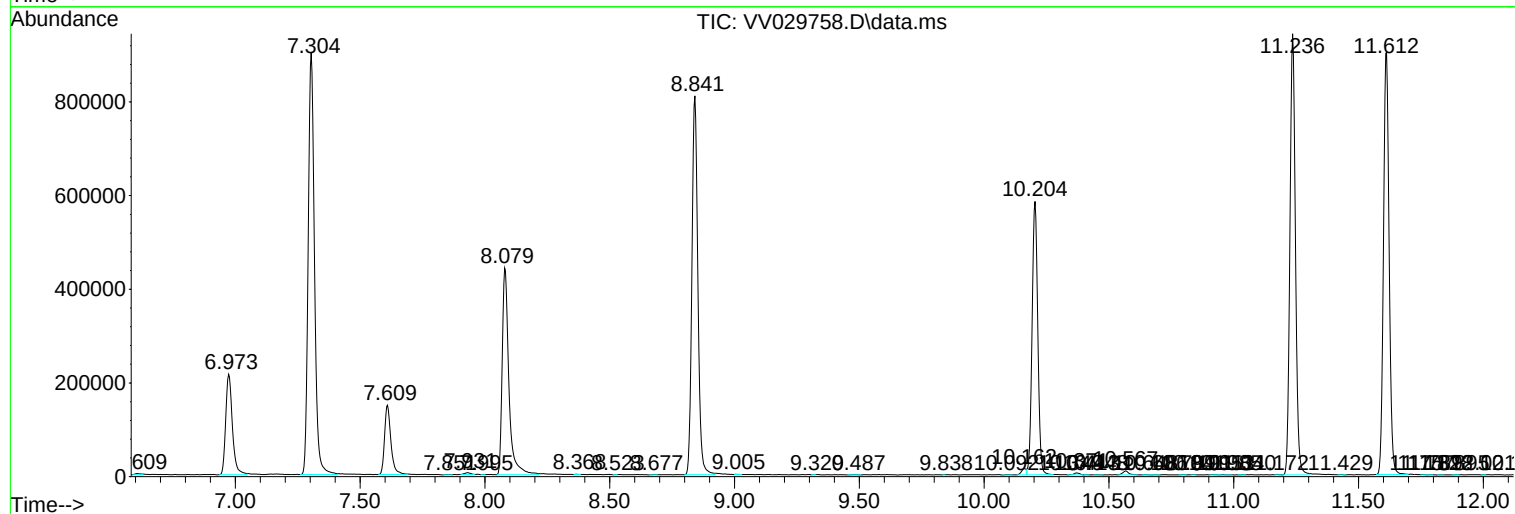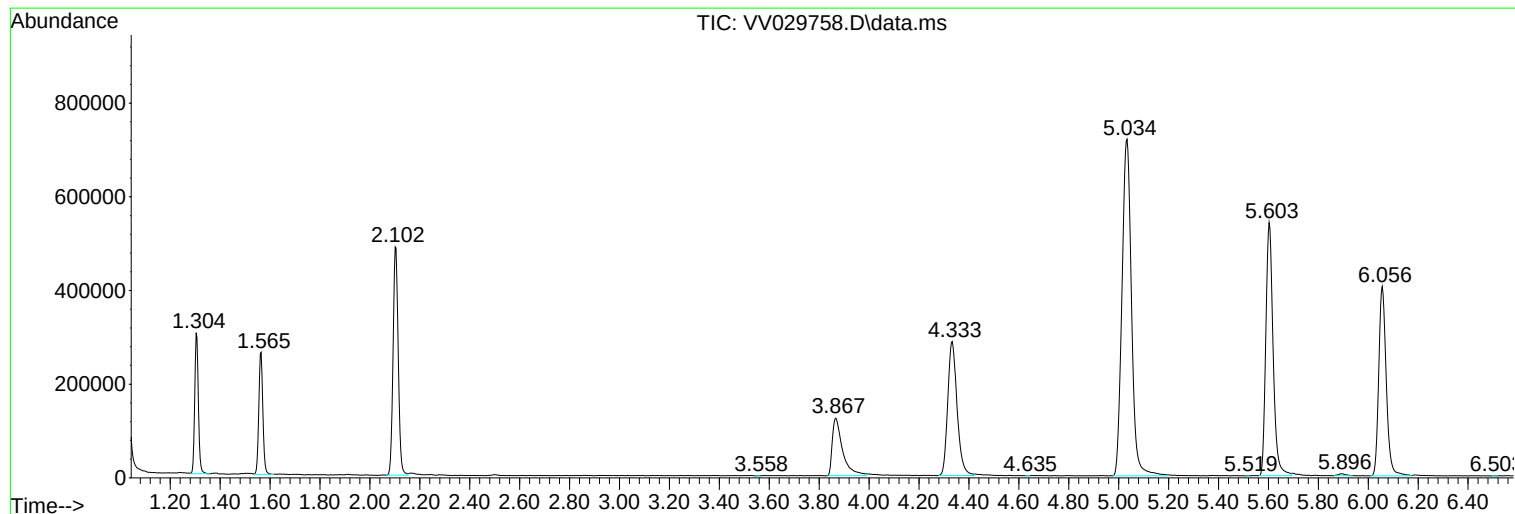

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029758.D
Acq On : 22 Dec 2022 15:07
Operator : SY/MD
Sample : N6193-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029758.D
Acq On : 22 Dec 2022 15:07
Operator : SY/MD
Sample : N6193-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc