

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029759.D
 Acq On : 22 Dec 2022 15:30
 Operator : SY/MD
 Sample : N6195-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	272387	274561	15.51%	2.011%
2	1.564	155	163	178	rVB	243508	267519	15.11%	1.960%
3	2.105	320	331	347	rBV	440719	633238	35.78%	4.638%
4	2.506	451	456	460	rVB2	1375	1325	0.07%	0.010%
5	2.613	486	489	492	rBV2	433	335	0.02%	0.002%
6	2.629	492	494	499	rVB3	320	273	0.02%	0.002%
7	2.687	507	512	515	rBV2	360	317	0.02%	0.002%
8	3.056	624	627	632	rBV3	408	297	0.02%	0.002%
9	3.117	640	646	649	rBV2	450	461	0.03%	0.003%
10	3.191	666	669	672	rBV	330	245	0.01%	0.002%
11	3.873	871	881	933	rBV	118295	355855	20.10%	2.607%
12	4.339	1009	1026	1062	rBV	263650	692006	39.10%	5.069%
13	4.616	1108	1112	1116	rBV4	432	478	0.03%	0.004%
14	4.844	1177	1183	1184	rBV	460	381	0.02%	0.003%
15	5.037	1225	1243	1278	rBV2	671486	1770029	100.00%	12.965%
16	5.394	1347	1354	1357	rBV3	605	714	0.04%	0.005%
17	5.407	1357	1358	1368	rVB3	638	570	0.03%	0.004%
18	5.532	1394	1397	1403	rBV3	286	334	0.02%	0.002%
19	5.609	1408	1421	1464	rBV	507624	1044774	59.03%	7.653%
20	5.902	1503	1512	1527	rVB5	4370	8992	0.51%	0.066%
21	6.059	1546	1561	1599	rBV	380710	793196	44.81%	5.810%
22	6.198	1601	1604	1610	rVB5	1299	1264	0.07%	0.009%
23	6.310	1635	1639	1643	rBV3	501	472	0.03%	0.003%
24	6.532	1706	1708	1714	rVB2	428	297	0.02%	0.002%
25	6.619	1725	1735	1741	rBV4	2034	3635	0.21%	0.027%
26	6.760	1775	1779	1782	rBV2	315	313	0.02%	0.002%
27	6.850	1801	1807	1808	rBV2	338	244	0.01%	0.002%
28	6.979	1834	1847	1881	rVV	197108	368546	20.82%	2.700%
29	7.104	1884	1886	1890	rVB3	447	331	0.02%	0.002%
30	7.146	1895	1899	1900	rBV3	812	485	0.03%	0.004%
31	7.249	1928	1931	1935	rVB3	693	444	0.03%	0.003%
32	7.307	1936	1949	1982	rBV	841593	1472122	83.17%	10.783%
33	7.612	2033	2044	2070	rBV	137388	242202	13.68%	1.774%
34	7.937	2137	2145	2153	rVB6	3037	4913	0.28%	0.036%
35	8.085	2180	2191	2228	rBV	440278	822279	46.46%	6.023%
36	8.403	2287	2290	2294	rBV2	592	576	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029759.D
 Acq On : 22 Dec 2022 15:30
 Operator : SY/MD
 Sample : N6195-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	8.587	2344	2347	2350	rVB3	480	328	0.02%	0.002%
38	8.648	2363	2366	2368	rBV2	405	291	0.02%	0.002%
39	8.699	2377	2382	2387	rBV4	614	552	0.03%	0.004%
40	8.735	2391	2393	2396	rVB3	416	246	0.01%	0.002%
41	8.844	2414	2427	2454	rBV	763436	1267348	71.60%	9.283%
42	9.143	2515	2520	2524	rVB2	536	531	0.03%	0.004%
43	9.172	2524	2529	2533	rBV3	435	388	0.02%	0.003%
44	9.342	2580	2582	2586	rVB	591	419	0.02%	0.003%
45	9.368	2586	2590	2593	rBV2	552	363	0.02%	0.003%
46	9.426	2606	2608	2612	rVB2	404	261	0.01%	0.002%
47	9.458	2612	2618	2622	rBV2	411	406	0.02%	0.003%
48	9.625	2668	2670	2673	rVV2	384	241	0.01%	0.002%
49	9.686	2686	2689	2691	rBV2	325	242	0.01%	0.002%
50	9.754	2706	2710	2713	rVB2	317	294	0.02%	0.002%
51	9.911	2754	2759	2760	rBV	275	245	0.01%	0.002%
52	9.953	2770	2772	2778	rVB2	441	381	0.02%	0.003%
53	9.982	2778	2781	2786	rBV	435	364	0.02%	0.003%
54	10.165	2828	2838	2840	rVV2	11544	15549	0.88%	0.114%
55	10.204	2840	2850	2876	rVB	556102	877134	49.55%	6.425%
56	10.374	2896	2903	2912	rVB2	3660	5242	0.30%	0.038%
57	10.487	2933	2938	2941	rBV2	325	297	0.02%	0.002%
58	10.532	2948	2952	2954	rBV	413	303	0.02%	0.002%
59	10.567	2954	2963	2974	rVV2	7110	11356	0.64%	0.083%
60	10.693	3000	3002	3006	rVB2	479	305	0.02%	0.002%
61	10.728	3009	3013	3015	rBV	351	271	0.02%	0.002%
62	10.908	3065	3069	3078	rVB4	529	715	0.04%	0.005%
63	11.017	3097	3103	3104	rBV2	359	298	0.02%	0.002%
64	11.056	3114	3115	3120	rVB2	425	282	0.02%	0.002%
65	11.149	3140	3144	3146	rBV2	369	306	0.02%	0.002%
66	11.236	3158	3171	3194	rBV	848168	1343737	75.92%	9.843%
67	11.374	3212	3214	3218	rVB2	713	466	0.03%	0.003%
68	11.419	3223	3228	3236	rVB4	620	918	0.05%	0.007%
69	11.451	3236	3238	3241	rBV	372	250	0.01%	0.002%
70	11.612	3276	3288	3307	rBV	851881	1324080	74.81%	9.699%
71	12.066	3427	3429	3433	rVB2	411	250	0.01%	0.002%
72	12.088	3433	3436	3441	rBV2	373	435	0.02%	0.003%
73	12.117	3441	3445	3446	rBV2	373	283	0.02%	0.002%
74	12.207	3469	3473	3476	rVB2	423	366	0.02%	0.003%
75	12.233	3476	3481	3493	rBV5	795	1527	0.09%	0.011%
76	12.445	3538	3547	3559	rBV3	7336	14486	0.82%	0.106%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029759.D
 Acq On : 22 Dec 2022 15:30
 Operator : SY/MD
 Sample : N6195-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	12.522	3568	3571	3575	rBV5	444	346	0.02%	0.003%
78	12.541	3575	3577	3580	rBV	380	271	0.02%	0.002%
79	12.580	3585	3589	3592	rBV3	385	280	0.02%	0.002%
80	12.599	3592	3595	3600	rVB3	270	250	0.01%	0.002%
81	12.628	3600	3604	3607	rBV4	736	710	0.04%	0.005%
82	12.702	3624	3627	3630	rBV2	427	402	0.02%	0.003%
83	12.767	3644	3647	3649	rBV2	603	359	0.02%	0.003%
84	12.834	3664	3668	3675	rBV4	1051	908	0.05%	0.007%
85	12.866	3675	3678	3681	rVB3	494	289	0.02%	0.002%
86	12.902	3686	3689	3693	rBV3	384	289	0.02%	0.002%
87	12.969	3708	3710	3714	rBV2	304	246	0.01%	0.002%
88	13.014	3721	3724	3726	rBV2	403	246	0.01%	0.002%
89	13.242	3793	3795	3799	rBV4	572	520	0.03%	0.004%
90	13.332	3819	3823	3826	rBV4	434	382	0.02%	0.003%
91	13.442	3853	3857	3862	rVB4	540	611	0.03%	0.004%
92	13.496	3867	3874	3882	rVV4	2837	4233	0.24%	0.031%
93	13.606	3905	3908	3911	rVB2	546	366	0.02%	0.003%
94	13.731	3942	3947	3954	rBV5	1423	1920	0.11%	0.014%
95	13.860	3983	3987	3988	rBV3	446	304	0.02%	0.002%
96	13.959	4014	4018	4024	rVV7	1174	1608	0.09%	0.012%
97	14.014	4032	4035	4037	rBV2	665	396	0.02%	0.003%
98	14.082	4053	4056	4059	rBV3	451	332	0.02%	0.002%
99	14.120	4064	4068	4071	rBV4	629	568	0.03%	0.004%
100	14.165	4080	4082	4085	rBV2	371	274	0.02%	0.002%




Sum of corrected areas: 13651889

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029759.D
Acq On : 22 Dec 2022 15:30
Operator : SY/MD
Sample : N6195-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

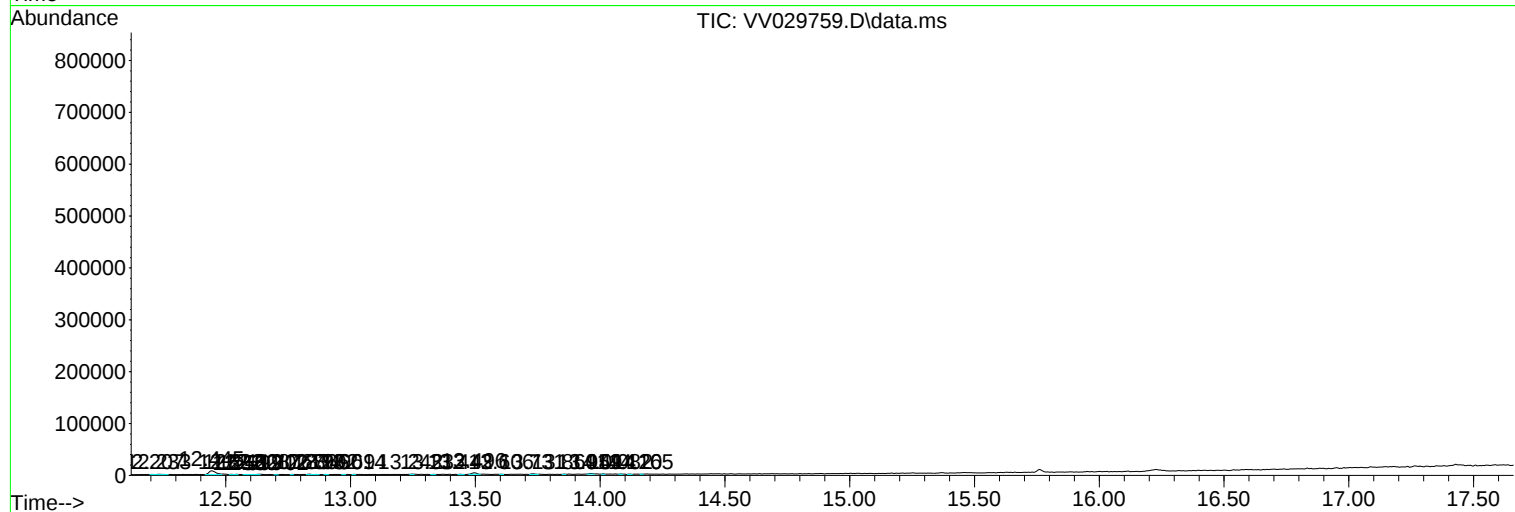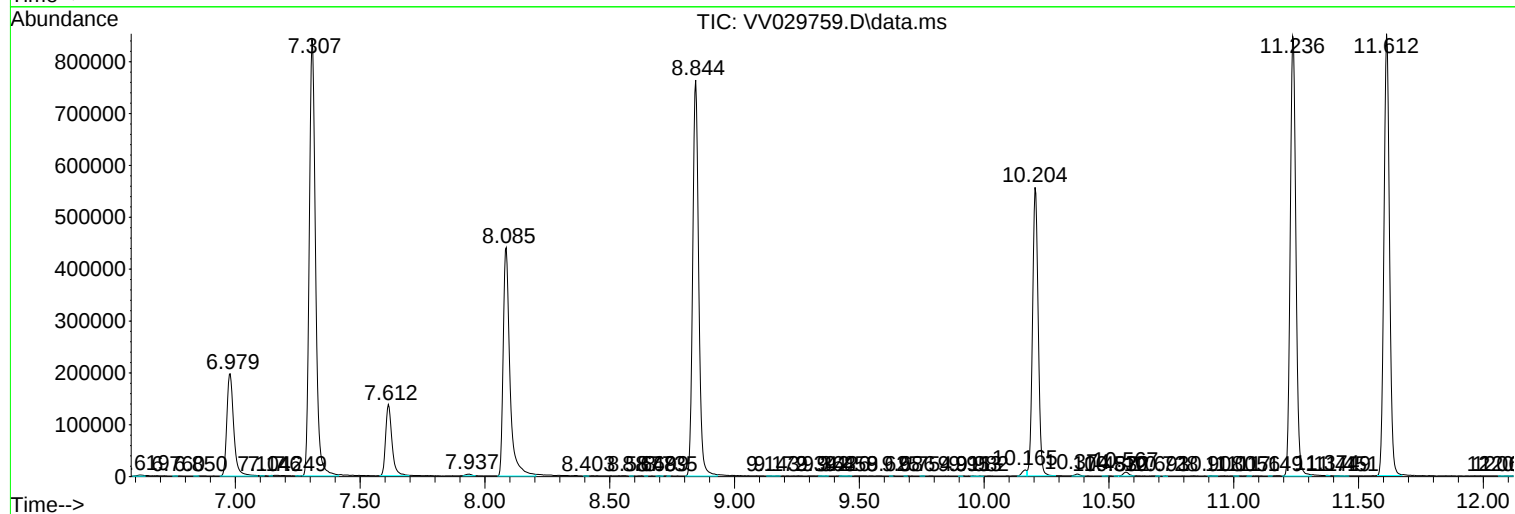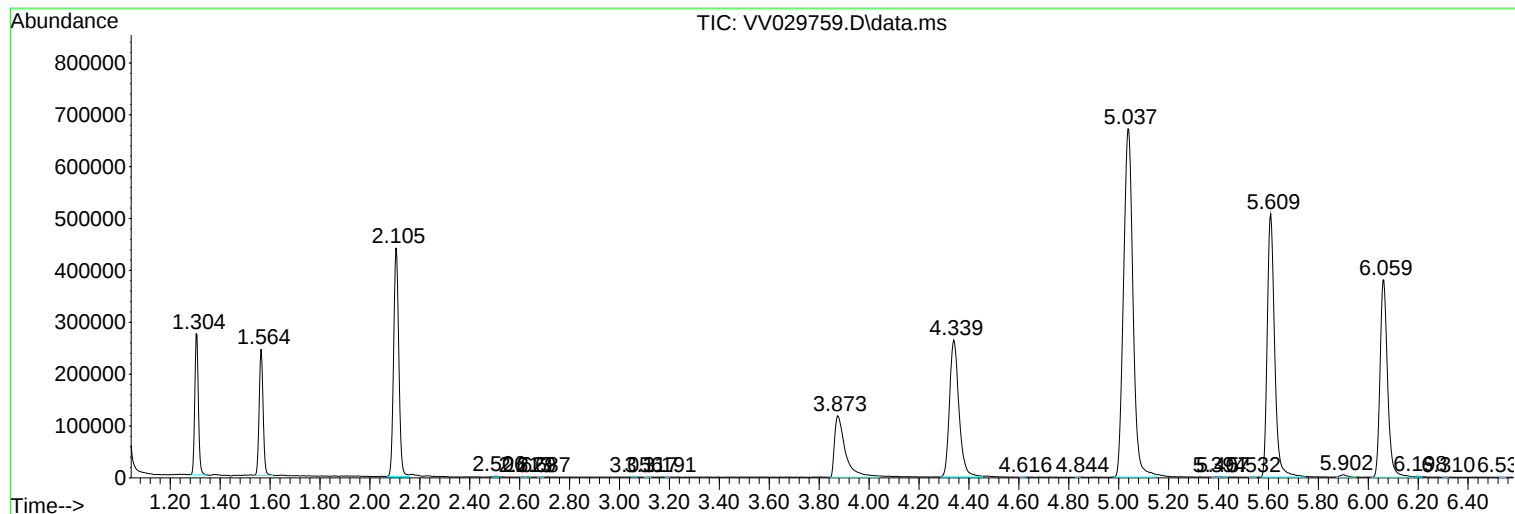

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029759.D
Acq On : 22 Dec 2022 15:30
Operator : SY/MD
Sample : N6195-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029759.D
Acq On : 22 Dec 2022 15:30
Operator : SY/MD
Sample : N6195-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc