

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029760.D
 Acq On : 22 Dec 2022 15:54
 Operator : SY/MD
 Sample : N6193-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSNO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029760.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.104	17	20	33	rVB	20112	20240	1.21%	0.155%
2	1.175	38	42	49	rVB	9010	7648	0.46%	0.059%
3	1.304	75	82	96	rVB	268575	269583	16.07%	2.068%
4	1.378	101	105	116	rVB3	5815	7590	0.45%	0.058%
5	1.564	155	163	177	rVB	224807	246413	14.69%	1.890%
6	2.104	320	331	344	rBV	425908	604000	36.01%	4.633%
7	2.500	447	454	464	rBV4	2322	3579	0.21%	0.027%
8	2.561	470	473	477	rBV	292	241	0.01%	0.002%
9	2.638	493	497	500	rBV	333	242	0.01%	0.002%
10	2.722	520	523	528	rBV3	392	365	0.02%	0.003%
11	2.764	528	536	544	rVV5	1330	1791	0.11%	0.014%
12	2.847	559	562	567	rVB2	442	312	0.02%	0.002%
13	2.892	567	576	577	rBV2	451	472	0.03%	0.004%
14	3.050	623	625	632	rVB3	354	382	0.02%	0.003%
15	3.114	641	645	649	rBV2	293	312	0.02%	0.002%
16	3.342	712	716	720	rBV2	516	422	0.03%	0.003%
17	3.362	720	722	727	rVB	414	256	0.02%	0.002%
18	3.751	839	843	847	rBV2	382	284	0.02%	0.002%
19	3.789	853	855	865	rVB3	381	404	0.02%	0.003%
20	3.876	871	882	923	rBV	109140	326550	19.47%	2.505%
21	4.339	1009	1026	1058	rBV	261573	653234	38.94%	5.011%
22	4.561	1092	1095	1099	rVB4	475	363	0.02%	0.003%
23	4.590	1099	1104	1107	rBV4	275	260	0.02%	0.002%
24	4.673	1123	1130	1140	rVB5	852	1726	0.10%	0.013%
25	4.805	1169	1171	1174	rBV2	400	277	0.02%	0.002%
26	5.040	1225	1244	1293	rBV2	631482	1677353	100.00%	12.867%
27	5.387	1348	1352	1354	rBV2	573	414	0.02%	0.003%
28	5.400	1354	1356	1361	rVB2	451	338	0.02%	0.003%
29	5.548	1399	1402	1405	rBV2	337	290	0.02%	0.002%
30	5.609	1408	1421	1467	rBV	501498	1028559	61.32%	7.890%
31	5.905	1500	1513	1526	rVB8	4002	8377	0.50%	0.064%
32	6.062	1544	1562	1595	rBV	356896	747116	44.54%	5.731%
33	6.191	1600	1602	1607	rVB3	663	431	0.03%	0.003%
34	6.271	1625	1627	1631	rBV	460	244	0.01%	0.002%
35	6.307	1635	1638	1641	rVV2	670	377	0.02%	0.003%
36	6.419	1668	1673	1676	rVV2	375	313	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029760.D
 Acq On : 22 Dec 2022 15:54
 Operator : SY/MD
 Sample : N6193-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.574	1713	1721	1728	rBV5	1711	3546	0.21%	0.027%
38	6.616	1730	1734	1749	rVB4	1888	3547	0.21%	0.027%
39	6.979	1835	1847	1878	rBV	184233	343763	20.49%	2.637%
40	7.140	1893	1897	1898	rBV	663	445	0.03%	0.003%
41	7.249	1929	1931	1935	rVB2	521	304	0.02%	0.002%
42	7.307	1936	1949	1971	rBV	767471	1362117	81.21%	10.449%
43	7.558	2024	2027	2030	rBV3	374	328	0.02%	0.003%
44	7.612	2033	2044	2079	rVB	126887	229571	13.69%	1.761%
45	7.905	2131	2135	2136	rBV2	474	324	0.02%	0.002%
46	7.934	2136	2144	2155	rVV4	3814	7200	0.43%	0.055%
47	8.014	2165	2169	2171	rBV2	404	345	0.02%	0.003%
48	8.085	2180	2191	2223	rBV	395594	735099	43.82%	5.639%
49	8.249	2235	2242	2254	rVB8	2839	5694	0.34%	0.044%
50	8.410	2290	2292	2298	rVB3	355	295	0.02%	0.002%
51	8.442	2298	2302	2305	rBV2	372	282	0.02%	0.002%
52	8.551	2335	2336	2341	rVB2	518	277	0.02%	0.002%
53	8.587	2341	2347	2350	rBV3	369	445	0.03%	0.003%
54	8.606	2350	2353	2357	rVB2	407	363	0.02%	0.003%
55	8.644	2357	2365	2369	rBV4	404	468	0.03%	0.004%
56	8.734	2390	2393	2397	rVB2	422	343	0.02%	0.003%
57	8.763	2397	2402	2404	rBV	325	263	0.02%	0.002%
58	8.844	2414	2427	2467	rBV	751200	1245587	74.26%	9.555%
59	9.133	2509	2517	2526	rVV5	2479	3827	0.23%	0.029%
60	9.313	2569	2573	2576	rVV2	269	275	0.02%	0.002%
61	9.429	2605	2609	2613	rBV	273	274	0.02%	0.002%
62	9.532	2638	2641	2643	rBV3	1041	755	0.05%	0.006%
63	9.609	2660	2665	2666	rBV2	352	257	0.02%	0.002%
64	9.815	2719	2729	2733	rBV6	1537	2336	0.14%	0.018%
65	9.921	2758	2762	2771	rVB3	1323	1596	0.10%	0.012%
66	10.033	2793	2797	2802	rVB2	552	606	0.04%	0.005%
67	10.059	2802	2805	2809	rBV2	532	472	0.03%	0.004%
68	10.098	2812	2817	2819	rBV2	291	298	0.02%	0.002%
69	10.162	2827	2837	2840	rBV	11932	15721	0.94%	0.121%
70	10.207	2840	2851	2875	rVB	509877	824083	49.13%	6.322%
71	10.371	2892	2902	2913	rVB2	6287	10215	0.61%	0.078%
72	10.439	2918	2923	2926	rBV3	361	326	0.02%	0.003%
73	10.532	2947	2952	2956	rBV3	1025	1103	0.07%	0.008%
74	10.567	2956	2963	2979	rVB2	7336	11603	0.69%	0.089%
75	10.792	3030	3033	3037	rVB2	379	286	0.02%	0.002%
76	10.847	3047	3050	3053	rVB3	384	258	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029760.D
 Acq On : 22 Dec 2022 15:54
 Operator : SY/MD
 Sample : N6193-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.908	3062	3069	3078	rVB2	988	1601	0.10%	0.012%
78	11.046	3107	3112	3113	rBV2	429	308	0.02%	0.002%
79	11.143	3135	3142	3151	rBV7	4613	7675	0.46%	0.059%
80	11.239	3159	3172	3192	rBV	843324	1320094	78.70%	10.127%
81	11.474	3242	3245	3251	rVB3	495	390	0.02%	0.003%
82	11.551	3262	3269	3275	rBV5	1418	2055	0.12%	0.016%
83	11.612	3275	3288	3311	rBV	791039	1241075	73.99%	9.520%
84	11.805	3345	3348	3353	rBV3	429	492	0.03%	0.004%
85	12.239	3474	3483	3493	rBV6	1480	2801	0.17%	0.021%
86	12.336	3504	3513	3523	rBV3	10998	16471	0.98%	0.126%
87	12.419	3534	3539	3542	rBV6	634	690	0.04%	0.005%
88	12.635	3597	3606	3613	rBV9	1442	2207	0.13%	0.017%
89	12.712	3626	3630	3636	rBV3	374	353	0.02%	0.003%
90	12.737	3636	3638	3645	rVB3	419	371	0.02%	0.003%
91	12.837	3665	3669	3674	rBV4	1012	744	0.04%	0.006%
92	12.889	3683	3685	3689	rVB2	412	278	0.02%	0.002%
93	12.921	3689	3695	3699	rBV3	766	954	0.06%	0.007%
94	12.963	3704	3708	3710	rBV3	279	252	0.02%	0.002%
95	13.081	3744	3745	3749	rVV3	488	280	0.02%	0.002%
96	13.155	3762	3768	3772	rBV3	392	504	0.03%	0.004%
97	13.249	3792	3797	3807	rVB8	2180	2991	0.18%	0.023%
98	13.496	3870	3874	3888	rVB	3153	4568	0.27%	0.035%
99	13.731	3940	3947	3954	rBV5	1840	2369	0.14%	0.018%
100	14.168	4080	4083	4088	rBV4	695	655	0.04%	0.005%




Sum of corrected areas: 13035833

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029760.D
Acq On : 22 Dec 2022 15:54
Operator : SY/MD
Sample : N6193-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

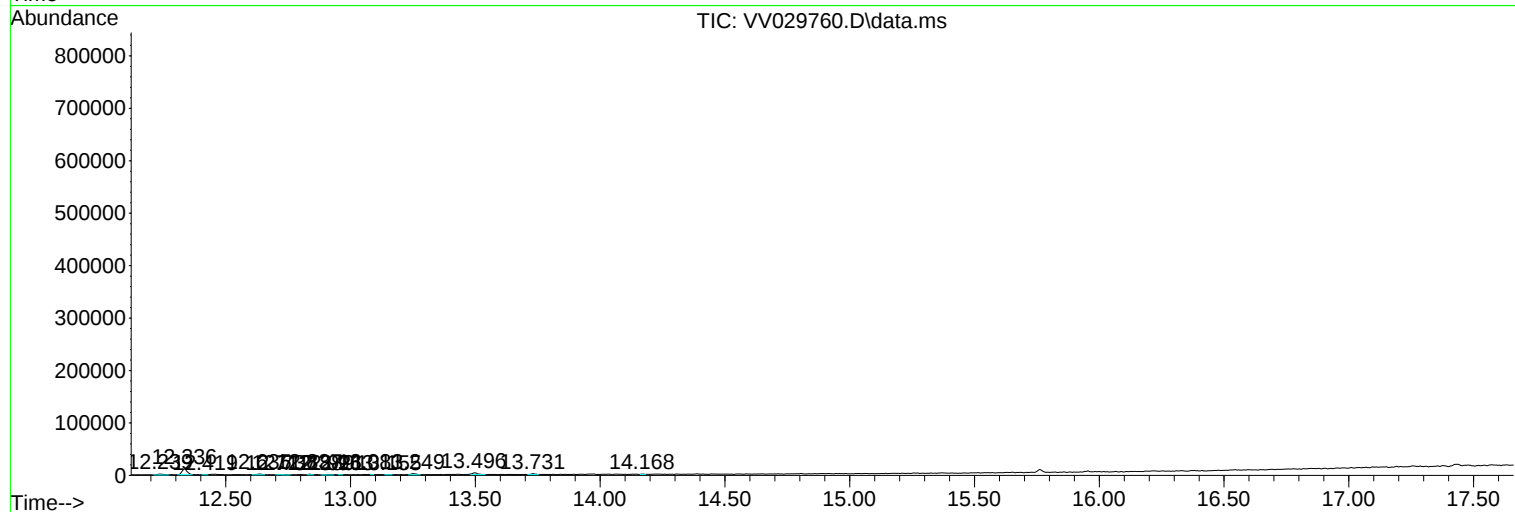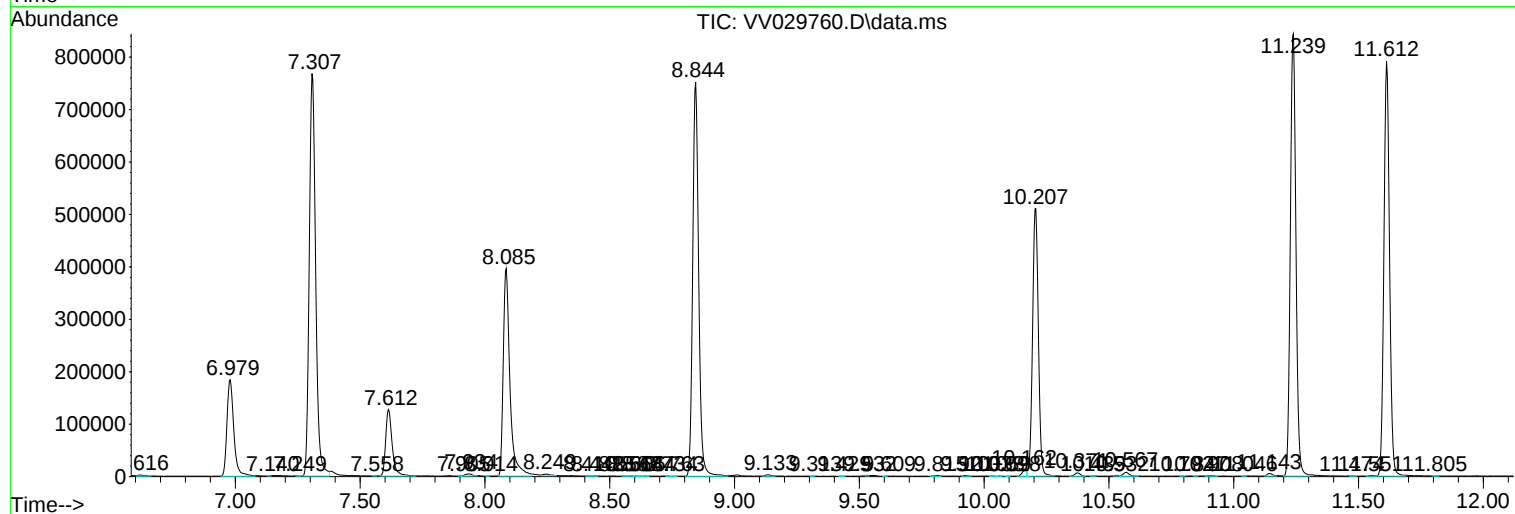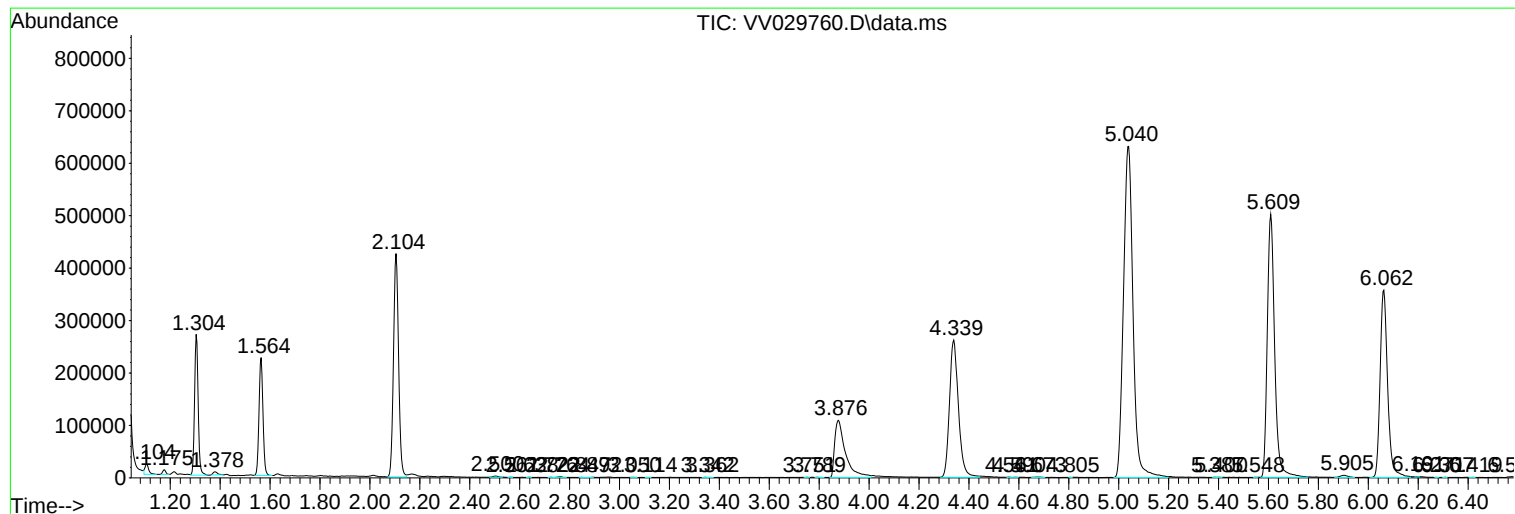

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029760.D
Acq On : 22 Dec 2022 15:54
Operator : SY/MD
Sample : N6193-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029760.D
Acq On : 22 Dec 2022 15:54
Operator : SY/MD
Sample : N6193-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------