

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029762.D
 Acq On : 22 Dec 2022 16:41
 Operator : SY/MD
 Sample : N6193-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	36	rVB	29146	30837	1.87%	0.237%
2	1.175	39	42	47	rVB2	6302	5115	0.31%	0.039%
3	1.304	75	82	99	rVB	268971	273031	16.57%	2.102%
4	1.378	101	105	112	rVB2	7530	8032	0.49%	0.062%
5	1.564	155	163	178	rVB	218933	246664	14.97%	1.899%
6	1.629	178	183	189	rBV8	3128	4400	0.27%	0.034%
7	2.040	309	311	312	rBV	809	373	0.02%	0.003%
8	2.105	319	331	343	rBV	407235	582559	35.36%	4.486%
9	2.343	400	405	411	rVB5	1595	2086	0.13%	0.016%
10	2.503	447	455	469	rVB8	1710	3630	0.22%	0.028%
11	2.603	481	486	488	rBV2	583	484	0.03%	0.004%
12	2.764	529	536	541	rVB3	532	722	0.04%	0.006%
13	2.860	561	566	570	rVB2	431	334	0.02%	0.003%
14	2.947	586	593	594	rBV	461	344	0.02%	0.003%
15	3.092	633	638	640	rBV2	354	328	0.02%	0.003%
16	3.207	670	674	677	rBV	372	277	0.02%	0.002%
17	3.265	690	692	697	rVB2	450	359	0.02%	0.003%
18	3.301	697	703	709	rBV2	381	473	0.03%	0.004%
19	3.362	720	722	727	rVV2	255	257	0.02%	0.002%
20	3.407	732	736	740	rVB2	402	292	0.02%	0.002%
21	3.442	740	747	752	rVB2	438	556	0.03%	0.004%
22	3.474	752	757	759	rBV	352	321	0.02%	0.002%
23	3.551	778	781	789	rVB2	375	453	0.03%	0.003%
24	3.619	794	802	804	rBV	289	350	0.02%	0.003%
25	3.719	829	833	835	rBV2	549	398	0.02%	0.003%
26	3.873	871	881	925	rBV	105976	309745	18.80%	2.385%
27	4.233	989	993	997	rBV3	380	375	0.02%	0.003%
28	4.339	1007	1026	1052	rBV	251157	633082	38.42%	4.875%
29	4.558	1091	1094	1099	rBV3	438	419	0.03%	0.003%
30	4.831	1176	1179	1181	rBV2	455	262	0.02%	0.002%
31	5.040	1225	1244	1290	rBV2	623197	1647632	100.00%	12.687%
32	5.432	1364	1366	1369	rVB3	522	282	0.02%	0.002%
33	5.481	1378	1381	1385	rVB	435	294	0.02%	0.002%
34	5.516	1389	1392	1398	rBV2	470	531	0.03%	0.004%
35	5.609	1408	1421	1453	rBV	523652	1072608	65.10%	8.259%
36	5.854	1494	1497	1502	rBV2	528	392	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029762.D
 Acq On : 22 Dec 2022 16:41
 Operator : SY/MD
 Sample : N6193-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.899	1502	1511	1527	rVB6	3488	7334	0.45%	0.056%
38	6.063	1547	1562	1599	rBV	352991	732772	44.47%	5.642%
39	6.272	1625	1627	1631	rVB3	536	289	0.02%	0.002%
40	6.301	1631	1636	1637	rBV3	804	542	0.03%	0.004%
41	6.317	1638	1641	1644	rVB3	421	266	0.02%	0.002%
42	6.542	1709	1711	1716	rVB	459	297	0.02%	0.002%
43	6.616	1727	1734	1744	rBV3	1889	3479	0.21%	0.027%
44	6.731	1766	1770	1773	rBV3	384	393	0.02%	0.003%
45	6.773	1780	1783	1786	rVV2	350	272	0.02%	0.002%
46	6.793	1786	1789	1793	rVV3	332	329	0.02%	0.003%
47	6.979	1835	1847	1880	rBV	182646	338928	20.57%	2.610%
48	7.156	1894	1902	1908	rBV6	1271	2678	0.16%	0.021%
49	7.220	1918	1922	1928	rBV6	553	497	0.03%	0.004%
50	7.307	1933	1949	1971	rBV	765995	1337943	81.20%	10.302%
51	7.574	2027	2032	2034	rBV3	609	523	0.03%	0.004%
52	7.612	2034	2044	2064	rBV	126617	222958	13.53%	1.717%
53	7.786	2094	2098	2100	rBV	411	277	0.02%	0.002%
54	7.899	2127	2133	2136	rBV3	423	476	0.03%	0.004%
55	7.931	2136	2143	2153	rVB4	1881	2974	0.18%	0.023%
56	8.085	2180	2191	2229	rBV	392287	731341	44.39%	5.631%
57	8.464	2307	2309	2313	rVB2	418	261	0.02%	0.002%
58	8.580	2341	2345	2347	rBV3	403	328	0.02%	0.003%
59	8.657	2366	2369	2372	rBV2	463	288	0.02%	0.002%
60	8.731	2389	2392	2395	rVB2	494	338	0.02%	0.003%
61	8.844	2414	2427	2453	rBV	787812	1300485	78.93%	10.014%
62	9.091	2499	2504	2508	rVB4	511	490	0.03%	0.004%
63	9.124	2508	2514	2517	rBV4	999	1386	0.08%	0.011%
64	9.236	2544	2549	2553	rBV2	527	466	0.03%	0.004%
65	9.284	2558	2564	2570	rBV	721	1036	0.06%	0.008%
66	9.387	2592	2596	2600	rBV3	342	420	0.03%	0.003%
67	9.542	2641	2644	2650	rBV3	596	414	0.03%	0.003%
68	9.661	2673	2681	2686	rBV3	559	703	0.04%	0.005%
69	9.805	2720	2726	2735	rBV5	2118	3196	0.19%	0.025%
70	10.075	2808	2810	2815	rVB3	336	275	0.02%	0.002%
71	10.162	2824	2837	2840	rBV2	10863	15320	0.93%	0.118%
72	10.204	2840	2850	2871	rVB	517456	810313	49.18%	6.239%
73	10.374	2894	2903	2910	rVB5	2627	3472	0.21%	0.027%
74	10.567	2955	2963	2973	rVB3	6738	10377	0.63%	0.080%
75	10.786	3028	3031	3033	rBV3	551	345	0.02%	0.003%
76	10.902	3064	3067	3070	rBV3	385	272	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029762.D
 Acq On : 22 Dec 2022 16:41
 Operator : SY/MD
 Sample : N6193-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.937	3075	3078	3082	rVB3	409	281	0.02%	0.002%
78	10.960	3082	3085	3091	rVB2	509	513	0.03%	0.004%
79	10.985	3091	3093	3095	rBV2	528	304	0.02%	0.002%
80	11.140	3134	3141	3156	rVB7	9947	15346	0.93%	0.118%
81	11.236	3159	3171	3193	rBV	894744	1388775	84.29%	10.694%
82	11.554	3260	3270	3276	rBV6	1467	2440	0.15%	0.019%
83	11.612	3276	3288	3317	rVV	760565	1178635	71.54%	9.076%
84	11.866	3363	3367	3368	rVB2	481	258	0.02%	0.002%
85	11.934	3384	3388	3392	rVB2	451	406	0.02%	0.003%
86	11.972	3396	3400	3405	rVB4	827	758	0.05%	0.006%
87	12.098	3437	3439	3444	rVB3	625	451	0.03%	0.003%
88	12.336	3505	3513	3531	rVB3	17822	27677	1.68%	0.213%
89	12.516	3566	3569	3574	rVB2	579	507	0.03%	0.004%
90	12.599	3592	3595	3599	rBV2	377	331	0.02%	0.003%
91	12.693	3619	3624	3630	rBV3	442	613	0.04%	0.005%
92	12.763	3641	3646	3651	rBV3	557	561	0.03%	0.004%
93	12.869	3675	3679	3683	rBV2	500	444	0.03%	0.003%
94	12.934	3697	3699	3702	rVB2	584	310	0.02%	0.002%
95	12.979	3709	3713	3716	rBV3	471	442	0.03%	0.003%
96	13.258	3793	3800	3803	rBV6	735	943	0.06%	0.007%
97	13.480	3865	3869	3870	rBV2	755	608	0.04%	0.005%
98	13.496	3870	3874	3883	rVB6	2031	2456	0.15%	0.019%
99	14.181	4085	4087	4089	rBV2	545	298	0.02%	0.002%
100	14.297	4121	4123	4127	rBV2	639	434	0.03%	0.003%




Sum of corrected areas: 12986841

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029762.D
Acq On : 22 Dec 2022 16:41
Operator : SY/MD
Sample : N6193-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

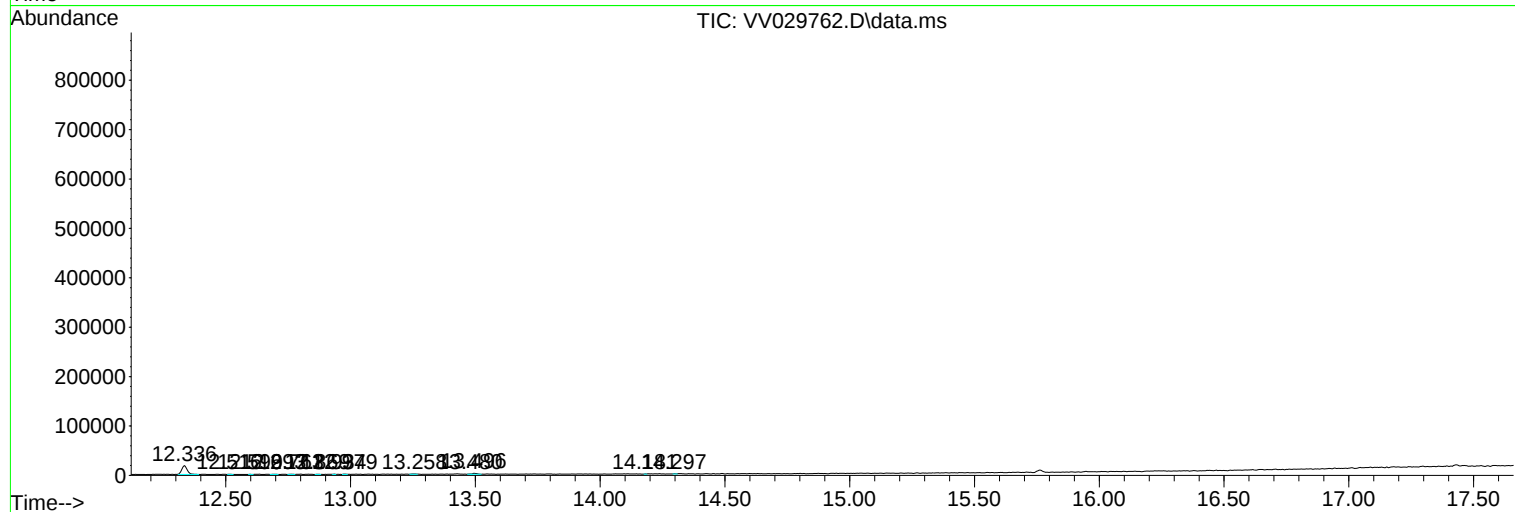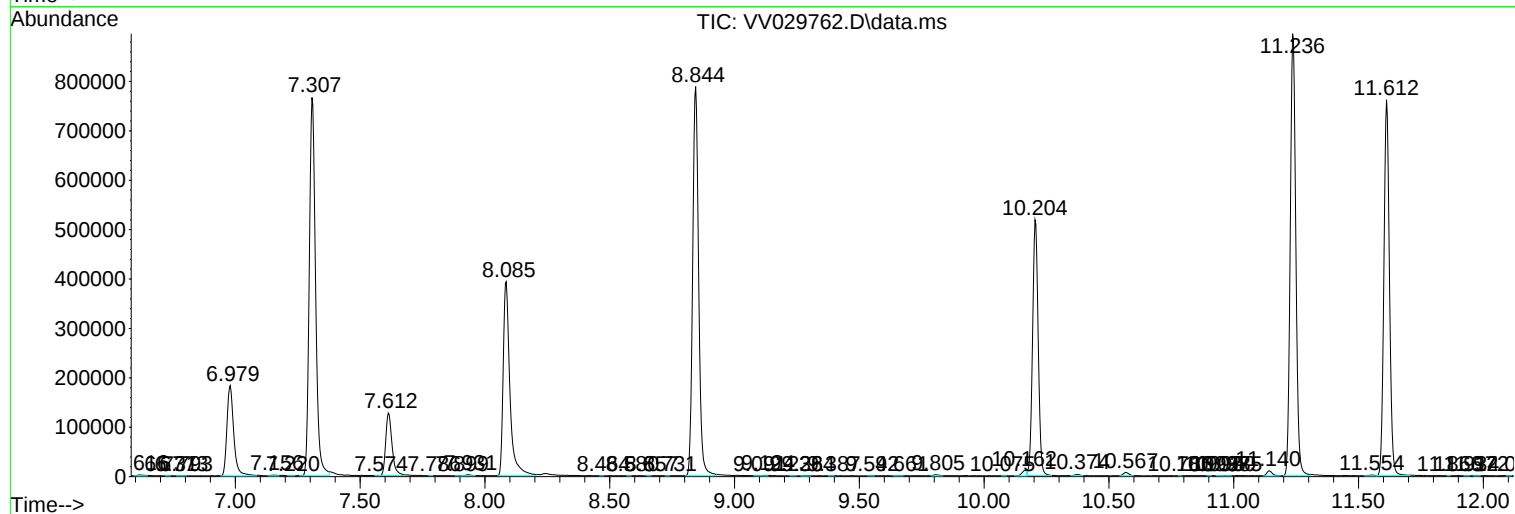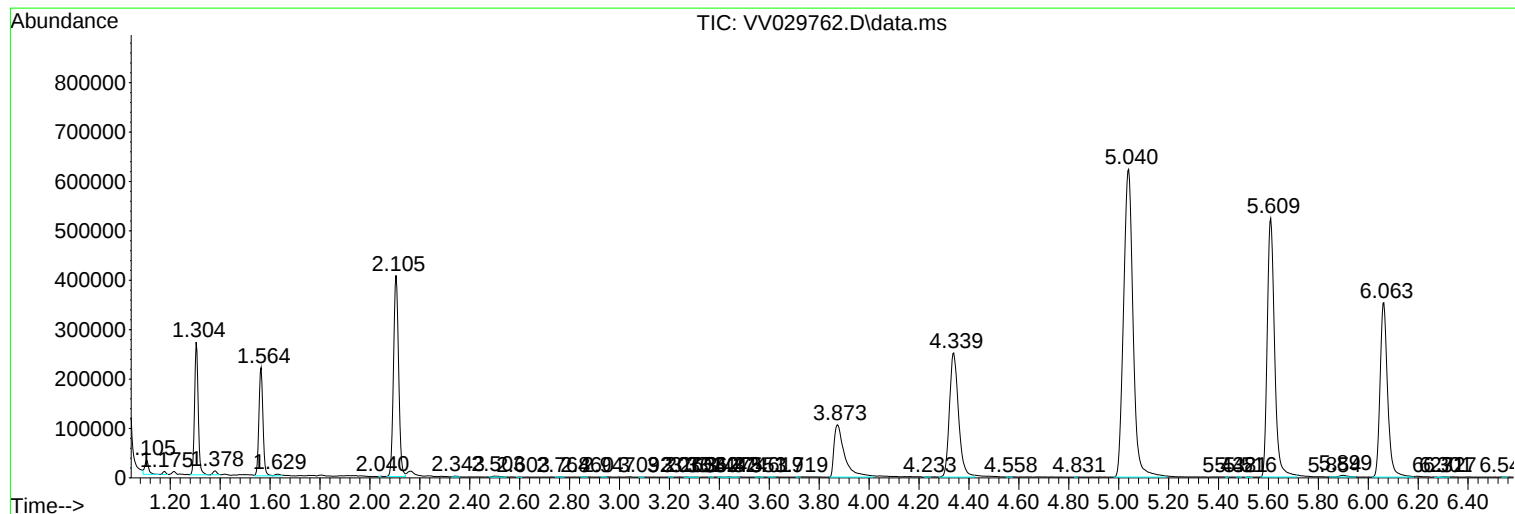

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029762.D
Acq On : 22 Dec 2022 16:41
Operator : SY/MD
Sample : N6193-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029762.D
Acq On : 22 Dec 2022 16:41
Operator : SY/MD
Sample : N6193-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc