

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029763.D
 Acq On : 22 Dec 2022 17:04
 Operator : SY/MD
 Sample : N6193-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	17	20	34	rVB	22349	23624	1.48%	0.190%
2	1.304	75	82	95	rVB	260215	254387	15.91%	2.047%
3	1.378	101	105	111	rBV2	4894	4642	0.29%	0.037%
4	1.565	155	163	176	rVB	211421	236655	14.80%	1.905%
5	2.105	319	331	345	rBV	395433	570758	35.69%	4.593%
6	2.285	384	387	388	rBV3	1126	710	0.04%	0.006%
7	2.503	445	455	466	rBV6	2045	3655	0.23%	0.029%
8	2.745	527	530	531	rBV	483	322	0.02%	0.003%
9	2.819	549	553	554	rBV	354	254	0.02%	0.002%
10	2.828	554	556	559	rVB	482	261	0.02%	0.002%
11	2.954	589	595	598	rBV2	457	401	0.03%	0.003%
12	3.034	616	620	628	rVB4	622	786	0.05%	0.006%
13	3.124	642	648	651	rBV	336	410	0.03%	0.003%
14	3.246	683	686	692	rVB2	405	339	0.02%	0.003%
15	3.632	803	806	809	rVV	390	270	0.02%	0.002%
16	3.661	810	815	819	rVB2	280	300	0.02%	0.002%
17	3.790	849	855	858	rBV3	433	558	0.03%	0.004%
18	3.873	871	881	918	rBV	107345	308034	19.26%	2.479%
19	4.339	1009	1026	1053	rBV2	248047	616771	38.56%	4.964%
20	4.667	1124	1128	1132	rBV3	296	256	0.02%	0.002%
21	4.790	1162	1166	1170	rVB3	359	290	0.02%	0.002%
22	4.818	1170	1175	1181	rBV	451	488	0.03%	0.004%
23	5.040	1226	1244	1295	rBV2	603166	1599338	100.00%	12.871%
24	5.391	1348	1353	1358	rBV3	423	477	0.03%	0.004%
25	5.462	1372	1375	1377	rBV2	290	197	0.01%	0.002%
26	5.609	1408	1421	1462	rBV	469636	966321	60.42%	7.777%
27	5.902	1503	1512	1523	rVV5	3366	7022	0.44%	0.057%
28	5.960	1527	1530	1535	rVB3	222	225	0.01%	0.002%
29	6.063	1547	1562	1597	rBV	345688	710456	44.42%	5.717%
30	6.240	1614	1617	1624	rVB4	773	774	0.05%	0.006%
31	6.281	1627	1630	1635	rVB3	468	393	0.02%	0.003%
32	6.323	1639	1643	1650	rVB2	557	507	0.03%	0.004%
33	6.365	1650	1656	1659	rBV2	413	371	0.02%	0.003%
34	6.471	1686	1689	1697	rBV2	298	372	0.02%	0.003%
35	6.526	1700	1706	1708	rBV2	240	206	0.01%	0.002%
36	6.571	1718	1720	1723	rBV2	348	201	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029763.D
 Acq On : 22 Dec 2022 17:04
 Operator : SY/MD
 Sample : N6193-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.625	1726	1737	1741	rBV5	1897	3616	0.23%	0.029%
38	6.773	1780	1783	1787	rVB2	339	242	0.02%	0.002%
39	6.818	1794	1797	1802	rBV2	468	317	0.02%	0.003%
40	6.902	1820	1823	1827	rVB	382	304	0.02%	0.002%
41	6.979	1836	1847	1883	rBV	177185	329074	20.58%	2.648%
42	7.191	1910	1913	1917	rVB4	722	631	0.04%	0.005%
43	7.211	1917	1919	1924	rVB4	444	254	0.02%	0.002%
44	7.307	1935	1949	1983	rBV	736500	1323133	82.73%	10.648%
45	7.613	2033	2044	2071	rVV	124081	217742	13.61%	1.752%
46	7.770	2088	2093	2094	rBV2	524	296	0.02%	0.002%
47	7.831	2110	2112	2115	rVB2	657	400	0.03%	0.003%
48	7.867	2119	2123	2125	rVV2	337	265	0.02%	0.002%
49	7.941	2138	2146	2152	rVB5	1454	2177	0.14%	0.018%
50	8.018	2164	2170	2173	rBV4	237	253	0.02%	0.002%
51	8.085	2180	2191	2234	rBV	396145	739913	46.26%	5.955%
52	8.551	2330	2336	2340	rBV3	773	842	0.05%	0.007%
53	8.574	2340	2343	2347	rVB3	327	230	0.01%	0.002%
54	8.596	2347	2350	2353	rBV3	385	269	0.02%	0.002%
55	8.613	2353	2355	2359	rBV2	288	221	0.01%	0.002%
56	8.632	2359	2361	2365	rVB3	265	213	0.01%	0.002%
57	8.664	2370	2371	2374	rVB2	534	253	0.02%	0.002%
58	8.715	2374	2387	2394	rBV5	2373	4353	0.27%	0.035%
59	8.844	2413	2427	2453	rBV	718620	1179402	73.74%	9.491%
60	8.998	2473	2475	2478	rBV3	475	374	0.02%	0.003%
61	9.056	2490	2493	2497	rVB3	700	490	0.03%	0.004%
62	9.130	2511	2516	2518	rBV3	1195	1030	0.06%	0.008%
63	9.214	2538	2542	2545	rVB	427	256	0.02%	0.002%
64	9.387	2593	2596	2599	rVV2	471	343	0.02%	0.003%
65	9.420	2599	2606	2613	rVB4	827	1133	0.07%	0.009%
66	9.513	2626	2635	2647	rBV4	3513	6169	0.39%	0.050%
67	9.580	2653	2656	2660	rVB3	443	321	0.02%	0.003%
68	9.603	2660	2663	2668	rBV2	346	260	0.02%	0.002%
69	9.731	2699	2703	2706	rBV2	331	254	0.02%	0.002%
70	9.812	2722	2728	2729	rBV3	386	359	0.02%	0.003%
71	9.857	2739	2742	2745	rVB3	292	222	0.01%	0.002%
72	9.899	2750	2755	2758	rVB3	342	319	0.02%	0.003%
73	9.921	2758	2762	2765	rBV2	408	346	0.02%	0.003%
74	9.995	2779	2785	2787	rBV2	228	235	0.01%	0.002%
75	10.040	2795	2799	2802	rBV	364	321	0.02%	0.003%
76	10.101	2811	2818	2822	rVB2	392	405	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029763.D
 Acq On : 22 Dec 2022 17:04
 Operator : SY/MD
 Sample : N6193-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.162	2826	2837	2840	rBV2	11663	15494	0.97%	0.125%
78	10.204	2840	2850	2873	rVB	499235	794018	49.65%	6.390%
79	10.371	2894	2902	2903	rBV3	1709	1809	0.11%	0.015%
80	10.448	2922	2926	2929	rBV2	431	391	0.02%	0.003%
81	10.571	2954	2964	2976	rVV	6616	10972	0.69%	0.088%
82	10.616	2976	2978	2983	rVB3	458	268	0.02%	0.002%
83	10.783	3024	3030	3038	rVB2	393	483	0.03%	0.004%
84	10.821	3039	3042	3044	rBV2	297	228	0.01%	0.002%
85	10.921	3071	3073	3076	rVB2	382	217	0.01%	0.002%
86	10.947	3076	3081	3084	rBV3	715	651	0.04%	0.005%
87	10.995	3093	3096	3100	rBV2	333	301	0.02%	0.002%
88	11.024	3100	3105	3108	rVV3	390	339	0.02%	0.003%
89	11.043	3109	3111	3116	rVV	384	325	0.02%	0.003%
90	11.146	3134	3143	3149	rBV5	3469	5510	0.34%	0.044%
91	11.236	3159	3171	3195	rBV	804431	1255493	78.50%	10.104%
92	11.548	3263	3268	3269	rBV2	1542	1206	0.08%	0.010%
93	11.612	3276	3288	3320	rBV	755982	1192220	74.54%	9.595%
94	11.908	3378	3380	3386	rVB4	306	305	0.02%	0.002%
95	12.233	3479	3481	3483	rBV2	645	341	0.02%	0.003%
96	12.294	3497	3500	3501	rBV2	350	231	0.01%	0.002%
97	12.333	3504	3512	3527	rVV4	9634	15205	0.95%	0.122%
98	12.519	3567	3570	3575	rVB2	593	524	0.03%	0.004%
99	12.770	3644	3648	3653	rBV3	677	646	0.04%	0.005%
100	13.021	3722	3726	3729	rBV3	531	552	0.03%	0.004%




Sum of corrected areas: 12425997

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029763.D
Acq On : 22 Dec 2022 17:04
Operator : SY/MD
Sample : N6193-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

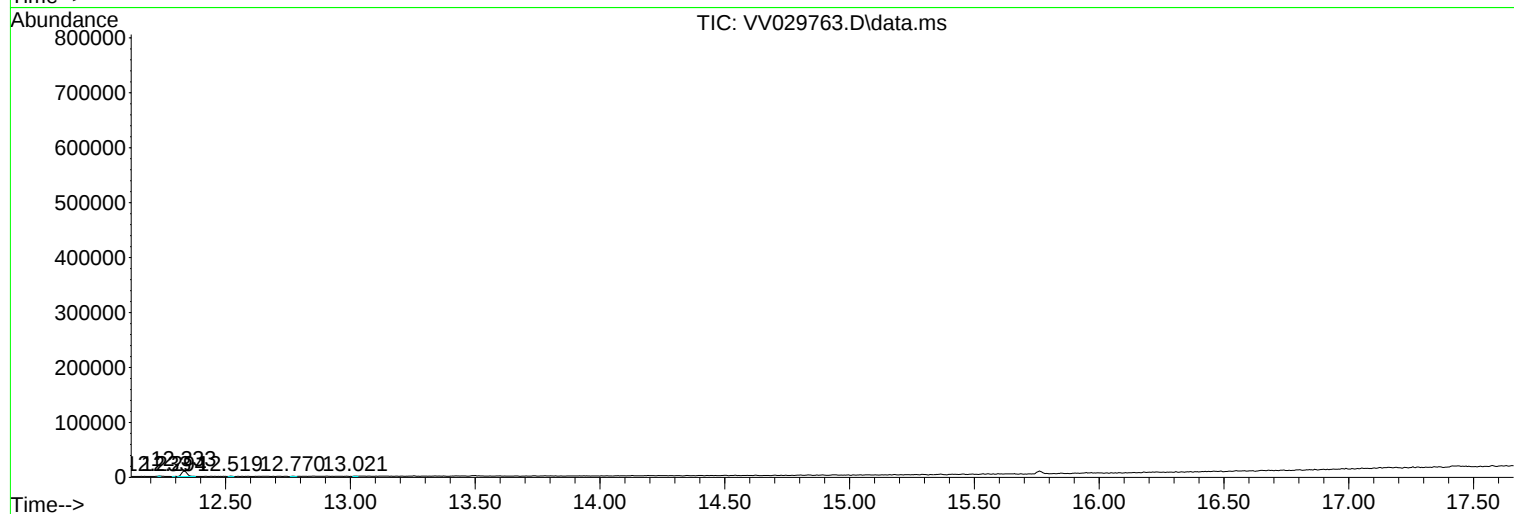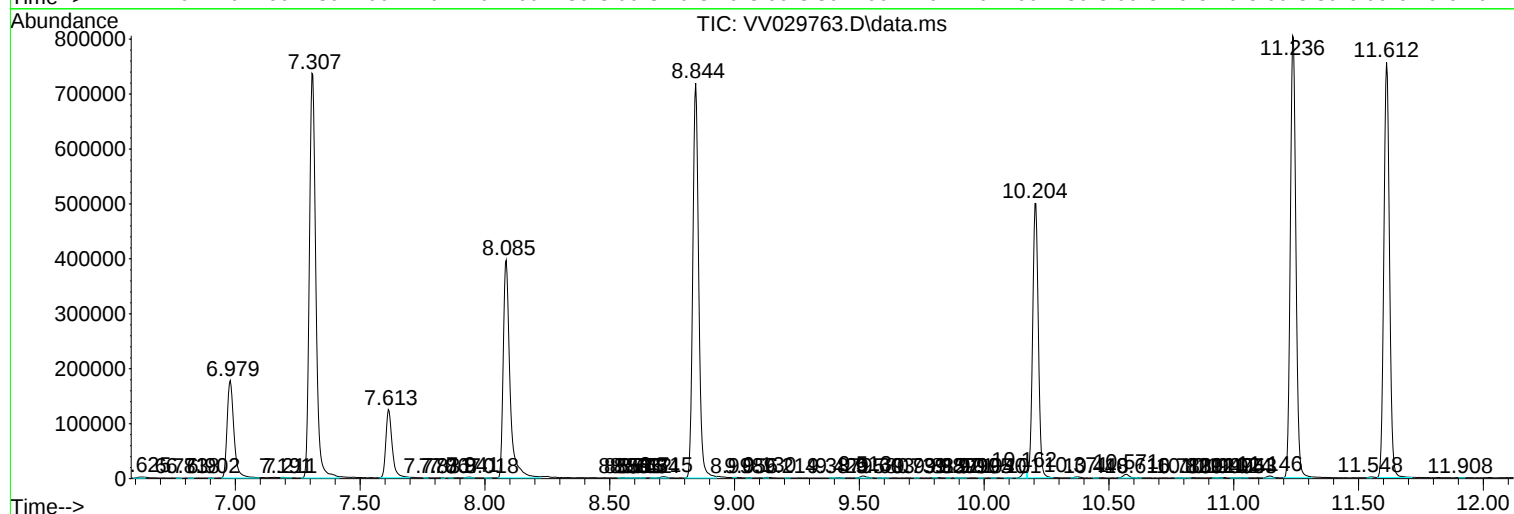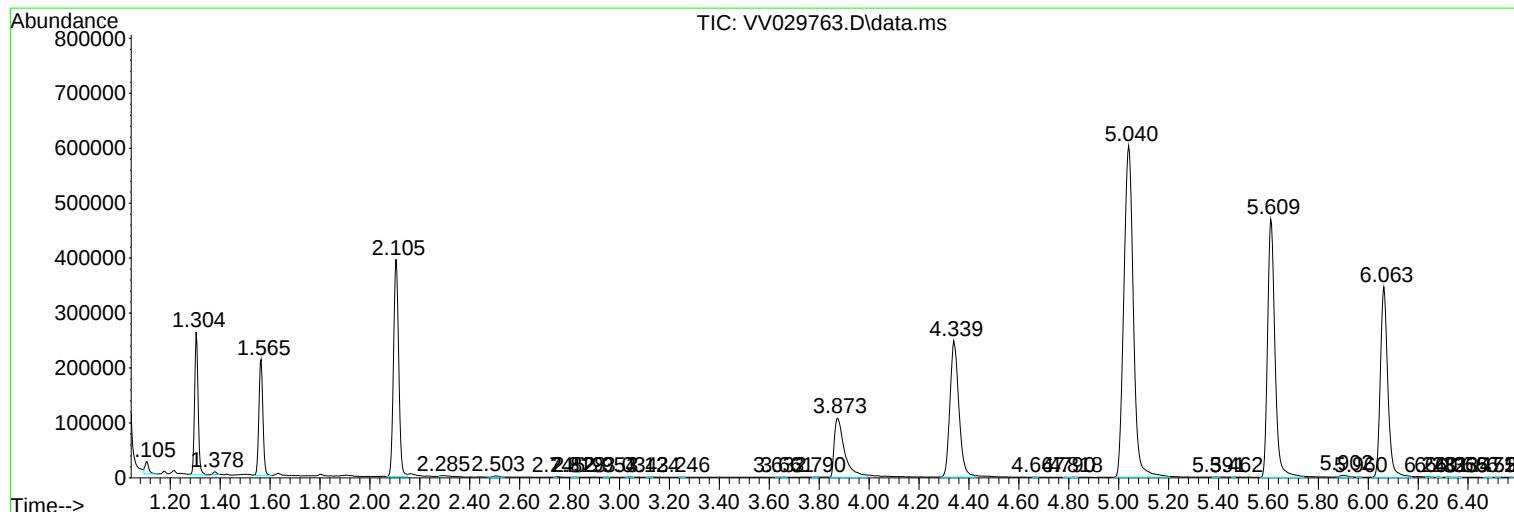

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029763.D
Acq On : 22 Dec 2022 17:04
Operator : SY/MD
Sample : N6193-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029763.D
Acq On : 22 Dec 2022 17:04
Operator : SY/MD
Sample : N6193-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------