

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029764.D
 Acq On : 22 Dec 2022 17:27
 Operator : SY/MD
 Sample : N6193-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029764.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	17	20	31	rVB	26428	27018	1.66%	0.219%
2	1.214	50	54	59	rVB	9963	8970	0.55%	0.073%
3	1.304	75	82	98	rVB	277347	278850	17.09%	2.262%
4	1.564	155	163	177	rVB	215682	240873	14.76%	1.954%
5	2.105	320	331	343	rBV	407265	586292	35.93%	4.756%
6	2.674	506	508	511	rBV2	516	349	0.02%	0.003%
7	2.966	596	599	603	rVB	685	408	0.03%	0.003%
8	3.124	644	648	651	rVB	772	553	0.03%	0.004%
9	3.243	682	685	695	rVB	560	773	0.05%	0.006%
10	3.359	718	721	723	rBV	576	390	0.02%	0.003%
11	3.622	799	803	806	rBV2	557	464	0.03%	0.004%
12	3.658	811	814	816	rBV	572	402	0.02%	0.003%
13	3.873	871	881	917	rBV	109475	310195	19.01%	2.516%
14	4.339	1009	1026	1057	rBV	254697	629372	38.57%	5.105%
15	4.641	1116	1120	1124	rBV3	931	989	0.06%	0.008%
16	4.728	1143	1147	1149	rBV2	868	579	0.04%	0.005%
17	5.040	1225	1244	1289	rBV2	614874	1631958	100.00%	13.238%
18	5.490	1374	1384	1388	rBV4	1029	1538	0.09%	0.012%
19	5.609	1407	1421	1449	rBV	430972	885077	54.23%	7.180%
20	5.902	1502	1512	1524	rBV10	3882	8664	0.53%	0.070%
21	6.063	1548	1562	1595	rBV	347146	730176	44.74%	5.923%
22	6.268	1621	1626	1631	rBV2	697	807	0.05%	0.007%
23	6.294	1631	1634	1639	rBV2	576	597	0.04%	0.005%
24	6.362	1651	1655	1659	rBV	424	379	0.02%	0.003%
25	6.616	1727	1734	1737	rBV5	1718	2014	0.12%	0.016%
26	6.979	1834	1847	1870	rBV	181563	334361	20.49%	2.712%
27	7.307	1936	1949	1970	rBV	747775	1330267	81.51%	10.791%
28	7.612	2034	2044	2069	rBV	124488	218449	13.39%	1.772%
29	7.838	2108	2114	2117	rBV3	742	792	0.05%	0.006%
30	7.937	2138	2145	2150	rBV4	1340	1950	0.12%	0.016%
31	8.005	2161	2166	2168	rBV	518	525	0.03%	0.004%
32	8.085	2180	2191	2222	rBV	403568	738083	45.23%	5.987%
33	8.436	2296	2300	2304	rVB2	785	655	0.04%	0.005%
34	8.461	2304	2308	2315	rBV5	809	728	0.04%	0.006%
35	8.516	2321	2325	2331	rVB4	852	799	0.05%	0.006%
36	8.574	2341	2343	2348	rBV4	553	418	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029764.D
 Acq On : 22 Dec 2022 17:27
 Operator : SY/MD
 Sample : N6193-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	8.619	2354	2357	2361	rBV4	453	379	0.02%	0.003%
38	8.754	2395	2399	2402	rBV2	665	471	0.03%	0.004%
39	8.844	2415	2427	2450	rBV	654967	1084408	66.45%	8.797%
40	9.098	2502	2506	2508	rBV3	591	397	0.02%	0.003%
41	9.130	2510	2516	2526	rVB3	2097	3721	0.23%	0.030%
42	9.178	2526	2531	2535	rBV4	657	725	0.04%	0.006%
43	9.339	2579	2581	2588	rVB4	379	365	0.02%	0.003%
44	9.439	2607	2612	2615	rVB3	490	421	0.03%	0.003%
45	9.612	2663	2666	2670	rBV2	444	403	0.02%	0.003%
46	9.683	2683	2688	2689	rBV	866	586	0.04%	0.005%
47	9.776	2711	2717	2720	rBV3	635	737	0.05%	0.006%
48	9.808	2724	2727	2728	rBV	818	502	0.03%	0.004%
49	9.857	2738	2742	2744	rBV2	587	378	0.02%	0.003%
50	9.918	2759	2761	2766	rVB4	477	359	0.02%	0.003%
51	9.963	2771	2775	2777	rBV	526	480	0.03%	0.004%
52	9.989	2780	2783	2788	rVB2	578	486	0.03%	0.004%
53	10.130	2822	2827	2829	rBV2	627	539	0.03%	0.004%
54	10.162	2829	2837	2840	rVV2	10508	14008	0.86%	0.114%
55	10.204	2840	2850	2876	rVB	528751	809615	49.61%	6.568%
56	10.374	2896	2903	2916	rVB2	2880	4963	0.30%	0.040%
57	10.442	2921	2924	2932	rBV2	916	970	0.06%	0.008%
58	10.538	2949	2954	2957	rVV4	964	891	0.05%	0.007%
59	10.567	2957	2963	2977	rVB4	6364	10769	0.66%	0.087%
60	10.638	2981	2985	2988	rBV2	365	366	0.02%	0.003%
61	10.699	3001	3004	3006	rBV	511	367	0.02%	0.003%
62	10.841	3043	3048	3050	rBV3	536	474	0.03%	0.004%
63	10.905	3062	3068	3076	rBV3	1680	2466	0.15%	0.020%
64	10.943	3076	3080	3082	rBV2	658	489	0.03%	0.004%
65	10.960	3082	3085	3089	rVB2	643	495	0.03%	0.004%
66	11.085	3120	3124	3126	rBV2	541	416	0.03%	0.003%
67	11.143	3135	3142	3149	rBV5	6006	9051	0.55%	0.073%
68	11.239	3160	3172	3192	rBV	731890	1145097	70.17%	9.289%
69	11.522	3254	3260	3264	rBV3	564	760	0.05%	0.006%
70	11.548	3264	3268	3270	rBV2	1511	1319	0.08%	0.011%
71	11.612	3276	3288	3308	rBV	773877	1210637	74.18%	9.821%
72	11.857	3360	3364	3370	rVB3	832	874	0.05%	0.007%
73	11.956	3391	3395	3398	rBV2	478	394	0.02%	0.003%
74	12.226	3475	3479	3480	rVV2	607	466	0.03%	0.004%
75	12.242	3480	3484	3492	rVB3	1201	1457	0.09%	0.012%
76	12.278	3492	3495	3500	rVB3	494	454	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029764.D
 Acq On : 22 Dec 2022 17:27
 Operator : SY/MD
 Sample : N6193-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	12.336	3504	3513	3523	rBV3	17243	25863	1.58%	0.210%
78	12.439	3542	3545	3549	rVB2	756	596	0.04%	0.005%
79	12.493	3559	3562	3565	rBV4	612	453	0.03%	0.004%
80	12.516	3565	3569	3572	rBV2	511	421	0.03%	0.003%
81	12.625	3596	3603	3605	rBV4	827	916	0.06%	0.007%
82	12.693	3618	3624	3625	rBV4	657	494	0.03%	0.004%
83	12.773	3646	3649	3653	rVB2	596	430	0.03%	0.003%
84	12.828	3663	3666	3669	rBV	594	466	0.03%	0.004%
85	12.918	3691	3694	3699	rVB3	943	812	0.05%	0.007%
86	13.050	3732	3735	3737	rBV2	711	446	0.03%	0.004%
87	13.078	3737	3744	3751	rVB6	645	1126	0.07%	0.009%
88	13.197	3778	3781	3784	rBV3	628	371	0.02%	0.003%
89	13.239	3791	3794	3795	rBV2	565	354	0.02%	0.003%
90	13.320	3813	3819	3822	rVB3	655	709	0.04%	0.006%
91	13.413	3845	3848	3851	rVB2	510	355	0.02%	0.003%
92	13.496	3868	3874	3881	rBV4	1521	1881	0.12%	0.015%
93	13.718	3938	3943	3944	rBV2	774	533	0.03%	0.004%
94	13.731	3944	3947	3949	rVB2	708	506	0.03%	0.004%
95	13.914	4001	4004	4008	rBV3	570	404	0.02%	0.003%
96	14.004	4028	4032	4035	rBV2	556	456	0.03%	0.004%
97	14.101	4059	4062	4068	rBV5	805	782	0.05%	0.006%
98	14.448	4167	4170	4174	rBV2	660	550	0.03%	0.004%
99	14.676	4237	4241	4243	rBV3	881	653	0.04%	0.005%
100	14.902	4307	4311	4315	rBV4	1018	1017	0.06%	0.008%




Sum of corrected areas: 12327463

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029764.D
Acq On : 22 Dec 2022 17:27
Operator : SY/MD
Sample : N6193-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

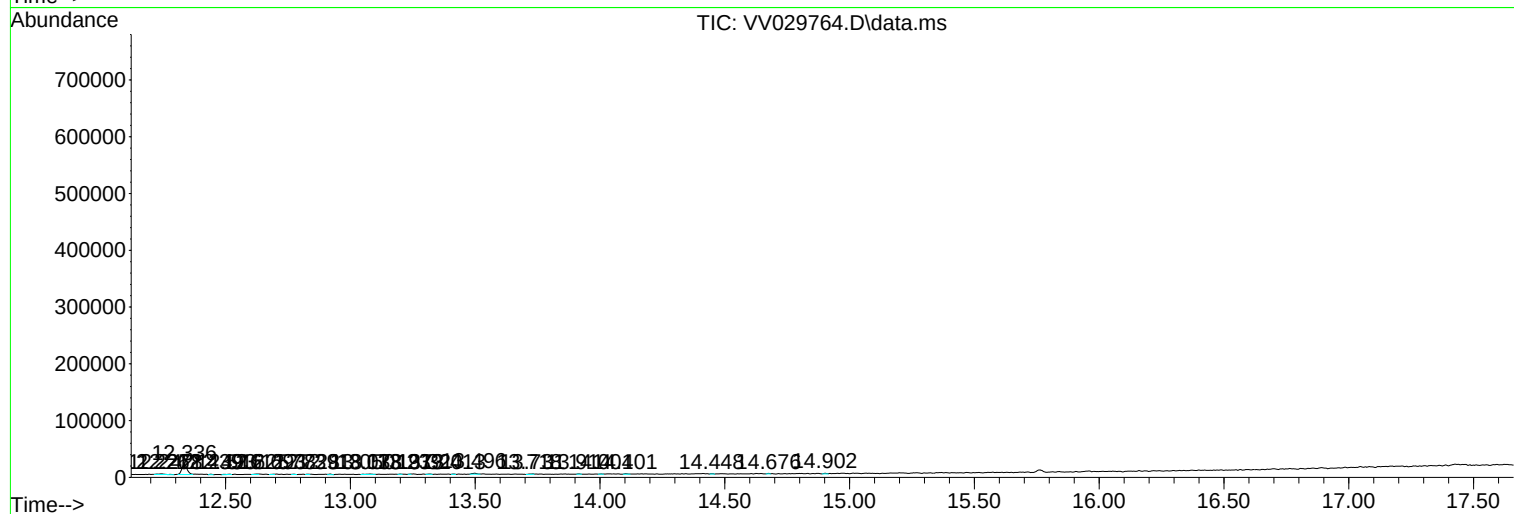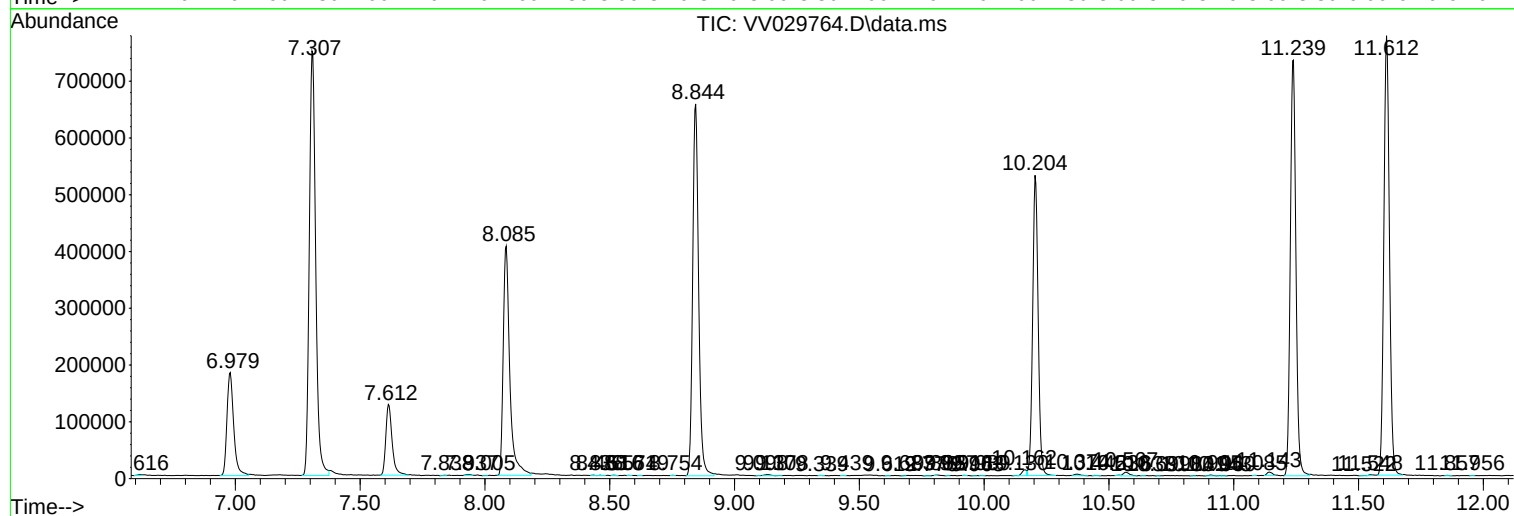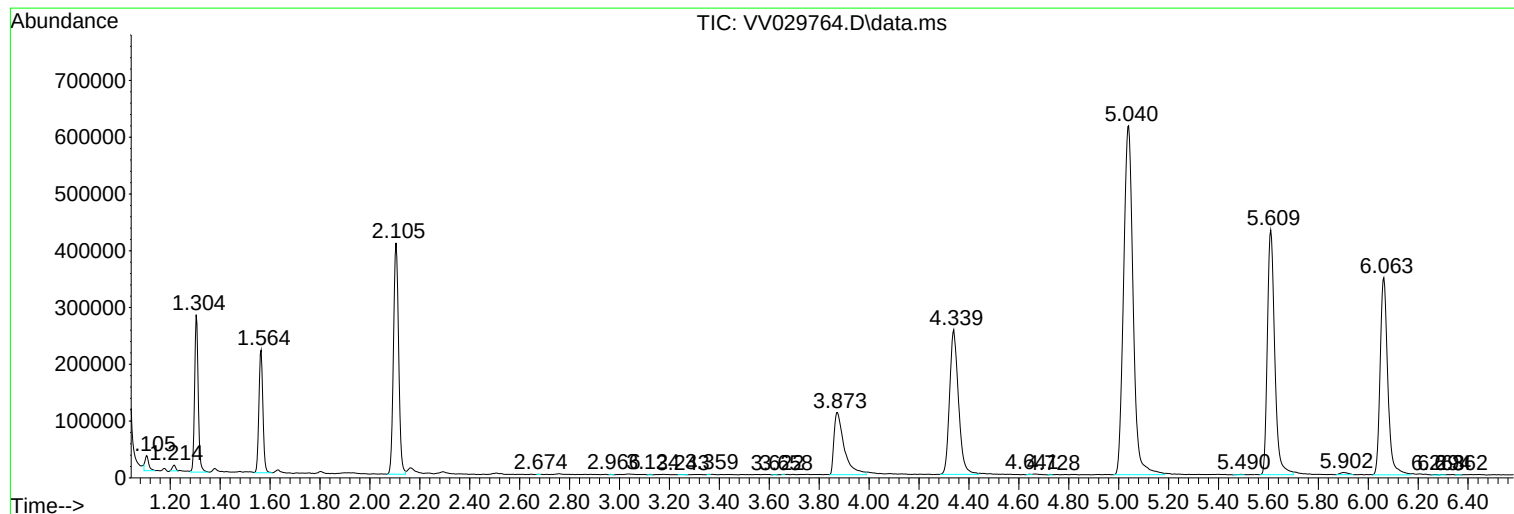

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029764.D
Acq On : 22 Dec 2022 17:27
Operator : SY/MD
Sample : N6193-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029764.D
Acq On : 22 Dec 2022 17:27
Operator : SY/MD
Sample : N6193-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------