

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029765.D
 Acq On : 22 Dec 2022 17:51
 Operator : SY/MD
 Sample : N6193-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029765.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	37	rVB	30289	31582	2.03%	0.259%
2	1.214	50	54	59	rVB2	7688	6442	0.41%	0.053%
3	1.304	75	82	99	rVB	253025	253374	16.28%	2.082%
4	1.378	100	105	115	rVB	8700	9882	0.63%	0.081%
5	1.565	155	163	175	rVV	202314	226159	14.53%	1.858%
6	1.632	178	184	194	rVB6	4348	6243	0.40%	0.051%
7	1.802	233	237	246	rVB3	4051	4550	0.29%	0.037%
8	2.105	320	331	343	rBV	382454	553756	35.57%	4.550%
9	2.401	419	423	428	rBV2	580	522	0.03%	0.004%
10	2.503	447	455	462	rBV7	2293	3351	0.22%	0.028%
11	2.745	527	530	531	rBV	573	337	0.02%	0.003%
12	2.876	568	571	576	rBV2	400	343	0.02%	0.003%
13	3.040	613	622	629	rVB5	1434	2447	0.16%	0.020%
14	3.082	629	635	637	rBV	351	393	0.03%	0.003%
15	3.507	764	767	770	rBV2	447	337	0.02%	0.003%
16	3.786	851	854	861	rVB3	599	512	0.03%	0.004%
17	3.822	861	865	868	rBV2	508	391	0.03%	0.003%
18	3.867	869	879	917	rBV	109154	295738	19.00%	2.430%
19	4.262	997	1002	1004	rBV	500	508	0.03%	0.004%
20	4.339	1008	1026	1056	rBV	240952	598503	38.45%	4.917%
21	4.661	1122	1126	1127	rBV3	626	376	0.02%	0.003%
22	4.741	1148	1151	1154	rVB	514	369	0.02%	0.003%
23	4.863	1186	1189	1191	rBV2	549	344	0.02%	0.003%
24	4.915	1200	1205	1213	rBV2	406	441	0.03%	0.004%
25	4.950	1213	1216	1220	rVB2	543	386	0.02%	0.003%
26	5.037	1225	1243	1299	rBV2	585110	1556655	100.00%	12.789%
27	5.394	1349	1354	1357	rBV3	377	393	0.03%	0.003%
28	5.468	1372	1377	1381	rBV3	513	582	0.04%	0.005%
29	5.609	1408	1421	1460	rVV	465641	958927	61.60%	7.878%
30	5.902	1501	1512	1523	rVB4	3298	6817	0.44%	0.056%
31	6.060	1548	1561	1595	rBV	332161	693614	44.56%	5.699%
32	6.291	1625	1633	1635	rBV2	564	616	0.04%	0.005%
33	6.307	1635	1638	1642	rVV3	612	565	0.04%	0.005%
34	6.416	1669	1672	1676	rVB2	717	531	0.03%	0.004%
35	6.442	1676	1680	1685	rVB2	484	412	0.03%	0.003%
36	6.506	1695	1700	1703	rBV	707	684	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029765.D
 Acq On : 22 Dec 2022 17:51
 Operator : SY/MD
 Sample : N6193-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.606	1727	1731	1732	rBV2	850	523	0.03%	0.004%
38	6.828	1796	1800	1804	rBV	436	391	0.03%	0.003%
39	6.905	1820	1824	1828	rVB3	345	342	0.02%	0.003%
40	6.934	1828	1833	1835	rBV4	435	334	0.02%	0.003%
41	6.976	1835	1846	1876	rBV	166094	313539	20.14%	2.576%
42	7.140	1894	1897	1898	rBV2	796	500	0.03%	0.004%
43	7.307	1936	1949	1987	rBV	709502	1268576	81.49%	10.422%
44	7.613	2034	2044	2066	rVV	118307	206832	13.29%	1.699%
45	7.799	2100	2102	2106	rVB3	911	582	0.04%	0.005%
46	7.828	2106	2111	2116	rBV5	322	412	0.03%	0.003%
47	8.082	2177	2190	2222	rBV	368312	678647	43.60%	5.576%
48	8.449	2301	2304	2308	rBV3	654	565	0.04%	0.005%
49	8.535	2328	2331	2335	rVB3	571	425	0.03%	0.003%
50	8.567	2335	2341	2343	rBV2	500	450	0.03%	0.004%
51	8.715	2379	2387	2394	rVB4	816	1217	0.08%	0.010%
52	8.751	2394	2398	2402	rBV2	631	510	0.03%	0.004%
53	8.844	2414	2427	2456	rBV	708611	1177326	75.63%	9.673%
54	9.092	2502	2504	2508	rVB2	763	501	0.03%	0.004%
55	9.133	2508	2517	2524	rVB6	1326	2009	0.13%	0.017%
56	9.214	2538	2542	2544	rBV	401	335	0.02%	0.003%
57	9.420	2603	2606	2612	rVB4	519	405	0.03%	0.003%
58	9.481	2621	2625	2627	rBV	598	345	0.02%	0.003%
59	9.516	2629	2636	2648	rVB7	2389	4319	0.28%	0.035%
60	9.603	2658	2663	2668	rVB3	381	464	0.03%	0.004%
61	9.693	2689	2691	2696	rVB3	545	507	0.03%	0.004%
62	9.725	2696	2701	2706	rBV3	637	585	0.04%	0.005%
63	9.767	2710	2714	2717	rBV3	433	350	0.02%	0.003%
64	9.802	2720	2725	2726	rBV3	1342	1105	0.07%	0.009%
65	10.162	2828	2837	2840	rBV	10674	14686	0.94%	0.121%
66	10.204	2840	2850	2868	rVB	493196	768369	49.36%	6.313%
67	10.378	2895	2904	2912	rBV4	1984	3717	0.24%	0.031%
68	10.510	2942	2945	2949	rVV2	422	405	0.03%	0.003%
69	10.571	2956	2964	2977	rVV	6312	10821	0.70%	0.089%
70	10.622	2977	2980	2986	rVB2	517	426	0.03%	0.003%
71	10.738	3010	3016	3017	rBV2	474	483	0.03%	0.004%
72	10.815	3037	3040	3044	rBV3	444	359	0.02%	0.003%
73	10.905	3063	3068	3071	rBV3	568	588	0.04%	0.005%
74	10.947	3078	3081	3084	rBV3	685	602	0.04%	0.005%
75	11.140	3134	3141	3152	rVV4	14019	20830	1.34%	0.171%
76	11.236	3159	3171	3198	rBV	821365	1254954	80.62%	10.311%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029765.D
 Acq On : 22 Dec 2022 17:51
 Operator : SY/MD
 Sample : N6193-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.374	3212	3214	3218	rVB2	702	443	0.03%	0.004%
78	11.397	3218	3221	3224	rVB2	644	408	0.03%	0.003%
79	11.468	3239	3243	3246	rBV3	831	624	0.04%	0.005%
80	11.497	3248	3252	3256	rBV3	403	344	0.02%	0.003%
81	11.551	3262	3269	3270	rBV5	1416	1217	0.08%	0.010%
82	11.612	3276	3288	3315	rBV	746234	1154028	74.14%	9.481%
83	12.008	3405	3411	3416	rBV3	478	689	0.04%	0.006%
84	12.120	3445	3446	3454	rVB3	444	477	0.03%	0.004%
85	12.204	3468	3472	3475	rBV4	461	362	0.02%	0.003%
86	12.333	3501	3512	3525	rBV2	33293	50067	3.22%	0.411%
87	12.419	3533	3539	3541	rBV2	568	409	0.03%	0.003%
88	12.490	3557	3561	3563	rBV2	609	463	0.03%	0.004%
89	12.535	3570	3575	3577	rBV2	363	339	0.02%	0.003%
90	12.632	3601	3605	3606	rBV3	647	451	0.03%	0.004%
91	12.834	3664	3668	3674	rVB3	642	577	0.04%	0.005%
92	12.911	3687	3692	3695	rBV4	478	463	0.03%	0.004%
93	12.947	3700	3703	3707	rBV3	611	474	0.03%	0.004%
94	13.249	3794	3797	3799	rBV2	565	458	0.03%	0.004%
95	13.326	3814	3821	3824	rBV3	642	803	0.05%	0.007%
96	13.429	3848	3853	3859	rVB6	1342	1424	0.09%	0.012%
97	13.484	3867	3870	3871	rBV2	789	424	0.03%	0.003%
98	13.548	3886	3890	3893	rBV3	435	383	0.02%	0.003%
99	13.564	3893	3895	3898	rVB2	710	343	0.02%	0.003%
100	15.050	4355	4357	4360	rVB4	1090	468	0.03%	0.004%




Sum of corrected areas: 12171556

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029765.D
Acq On : 22 Dec 2022 17:51
Operator : SY/MD
Sample : N6193-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

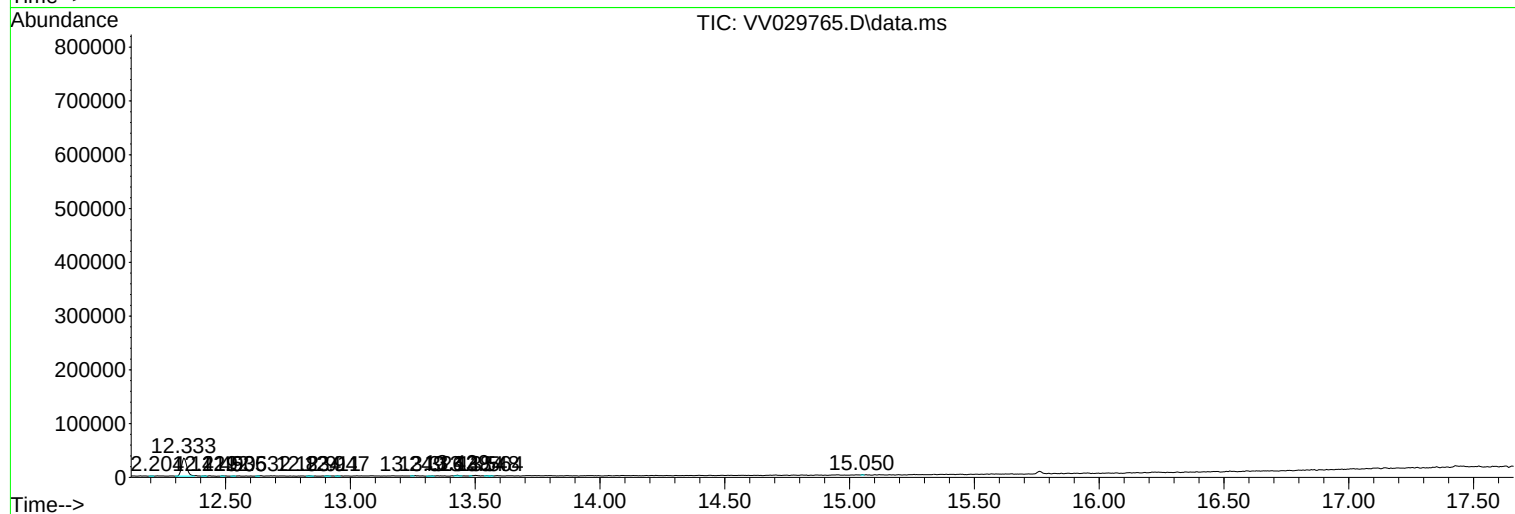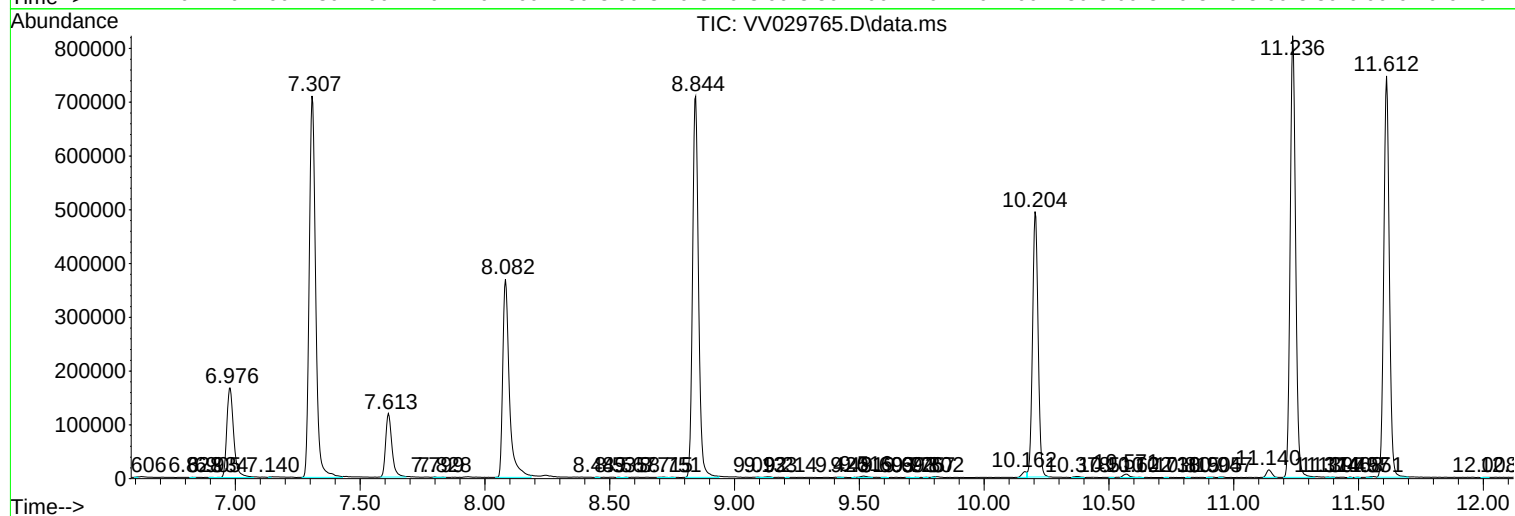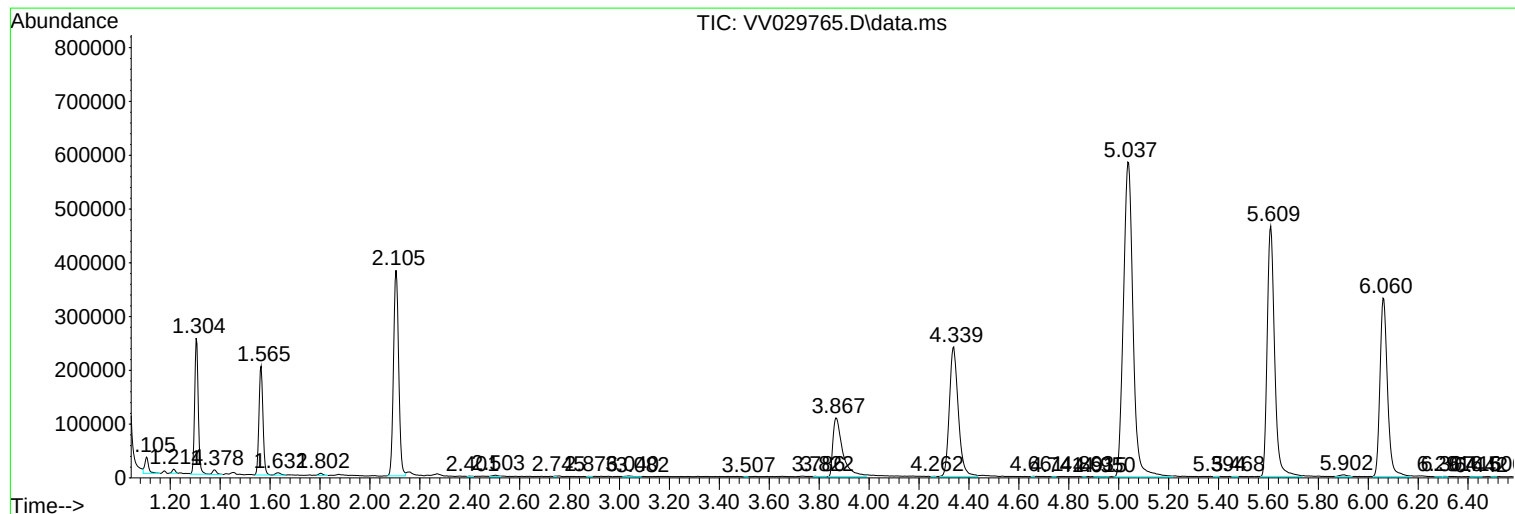

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029765.D
Acq On : 22 Dec 2022 17:51
Operator : SY/MD
Sample : N6193-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029765.D
Acq On : 22 Dec 2022 17:51
Operator : SY/MD
Sample : N6193-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc