

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029766.D
 Acq On : 22 Dec 2022 18:14
 Operator : SY/MD
 Sample : N6193-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029766.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	248726	249089	16.01%	2.044%
2	1.565	155	163	178	rVB	205308	229710	14.76%	1.885%
3	2.105	319	331	343	rBV	390004	558513	35.90%	4.584%
4	2.275	377	384	394	rVB3	5224	9967	0.64%	0.082%
5	2.442	432	436	441	rBV3	304	316	0.02%	0.003%
6	2.500	449	454	465	rVB5	1758	2591	0.17%	0.021%
7	2.716	518	521	527	rVB2	316	251	0.02%	0.002%
8	3.031	615	619	622	rBV2	259	237	0.02%	0.002%
9	3.127	646	649	657	rVB	270	269	0.02%	0.002%
10	3.240	681	684	687	rBV2	349	290	0.02%	0.002%
11	3.368	720	724	728	rBV2	284	240	0.02%	0.002%
12	3.535	771	776	779	rBV2	206	245	0.02%	0.002%
13	3.577	784	789	792	rBV2	235	235	0.02%	0.002%
14	3.622	799	803	807	rBV2	431	446	0.03%	0.004%
15	3.712	827	831	834	rBV	375	319	0.02%	0.003%
16	3.867	870	879	923	rBV	107646	299837	19.27%	2.461%
17	4.207	981	985	989	rBV3	425	401	0.03%	0.003%
18	4.339	1006	1026	1061	rBV	237382	610730	39.25%	5.012%
19	4.687	1131	1134	1137	rBV2	417	351	0.02%	0.003%
20	5.037	1226	1243	1294	rBV2	586293	1555810	100.00%	12.769%
21	5.281	1315	1319	1323	rVB3	591	518	0.03%	0.004%
22	5.326	1330	1333	1338	rBV2	360	279	0.02%	0.002%
23	5.413	1356	1360	1368	rVB4	429	457	0.03%	0.004%
24	5.478	1374	1380	1387	rVB3	486	747	0.05%	0.006%
25	5.609	1407	1421	1450	rBV	488912	996393	64.04%	8.178%
26	5.841	1490	1493	1498	rVB2	490	261	0.02%	0.002%
27	5.902	1502	1512	1527	rBV3	4209	8395	0.54%	0.069%
28	5.953	1527	1528	1537	rVB4	555	406	0.03%	0.003%
29	6.059	1547	1561	1590	rBV	324373	682298	43.85%	5.600%
30	6.304	1635	1637	1642	rVB2	324	254	0.02%	0.002%
31	6.381	1654	1661	1666	rVB	441	541	0.03%	0.004%
32	6.416	1666	1672	1675	rBV2	300	293	0.02%	0.002%
33	6.619	1728	1735	1737	rBV5	1620	1728	0.11%	0.014%
34	6.860	1807	1810	1816	rVB2	375	410	0.03%	0.003%
35	6.895	1816	1821	1824	rBV	442	359	0.02%	0.003%
36	6.979	1831	1847	1874	rBV	170275	313459	20.15%	2.573%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029766.D
 Acq On : 22 Dec 2022 18:14
 Operator : SY/MD
 Sample : N6193-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.072	1874	1876	1881	rVB3	775	584	0.04%	0.005%
38	7.252	1927	1932	1936	rBV2	331	394	0.03%	0.003%
39	7.307	1936	1949	1984	rBV	725893	1266648	81.41%	10.396%
40	7.484	2002	2004	2007	rBV2	564	386	0.02%	0.003%
41	7.551	2021	2025	2029	rBV3	540	504	0.03%	0.004%
42	7.612	2034	2044	2072	rBV	118287	209627	13.47%	1.720%
43	7.934	2139	2144	2150	rBV4	904	1198	0.08%	0.010%
44	8.082	2177	2190	2221	rBV	380872	694240	44.62%	5.698%
45	8.474	2308	2312	2315	rBV3	562	479	0.03%	0.004%
46	8.522	2325	2327	2332	rVB2	489	335	0.02%	0.003%
47	8.558	2332	2338	2340	rBV3	608	635	0.04%	0.005%
48	8.712	2382	2386	2392	rBV2	400	444	0.03%	0.004%
49	8.751	2392	2398	2402	rBV2	251	288	0.02%	0.002%
50	8.789	2407	2410	2414	rVB3	357	249	0.02%	0.002%
51	8.844	2414	2427	2460	rBV	735599	1223589	78.65%	10.042%
52	9.185	2530	2533	2538	rBV2	341	253	0.02%	0.002%
53	9.590	2653	2659	2666	rVB3	450	518	0.03%	0.004%
54	9.654	2676	2679	2682	rBV	247	237	0.02%	0.002%
55	9.693	2688	2691	2695	rBV	255	245	0.02%	0.002%
56	9.873	2745	2747	2752	rVB2	514	276	0.02%	0.002%
57	9.918	2758	2761	2766	rBV3	306	235	0.02%	0.002%
58	9.947	2766	2770	2774	rBV2	462	364	0.02%	0.003%
59	10.120	2819	2824	2829	rVB2	425	529	0.03%	0.004%
60	10.165	2829	2838	2840	rBV2	10896	13976	0.90%	0.115%
61	10.204	2840	2850	2873	rVV	483859	765713	49.22%	6.284%
62	10.304	2877	2881	2884	rVV2	597	465	0.03%	0.004%
63	10.326	2884	2888	2891	rVB3	477	371	0.02%	0.003%
64	10.346	2891	2894	2898	rBV2	324	339	0.02%	0.003%
65	10.378	2898	2904	2914	rVB4	1333	1819	0.12%	0.015%
66	10.461	2925	2930	2932	rBV	402	365	0.02%	0.003%
67	10.516	2945	2947	2954	rVB2	292	260	0.02%	0.002%
68	10.567	2954	2963	2973	rBV2	6632	10711	0.69%	0.088%
69	10.821	3038	3042	3044	rBV2	319	255	0.02%	0.002%
70	10.915	3066	3071	3073	rBV2	339	280	0.02%	0.002%
71	11.098	3126	3128	3133	rVB2	377	278	0.02%	0.002%
72	11.236	3159	3171	3199	rBV	829990	1293297	83.13%	10.614%
73	11.368	3209	3212	3217	rBV4	517	458	0.03%	0.004%
74	11.435	3231	3233	3237	rVB2	547	284	0.02%	0.002%
75	11.548	3262	3268	3269	rBV3	1390	979	0.06%	0.008%
76	11.612	3276	3288	3312	rBV	744671	1153373	74.13%	9.466%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029766.D
 Acq On : 22 Dec 2022 18:14
 Operator : SY/MD
 Sample : N6193-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.757	3328	3333	3335	rBV5	384	325	0.02%	0.003%
78	11.773	3336	3338	3342	rVV3	342	236	0.02%	0.002%
79	11.918	3379	3383	3385	rVV3	344	291	0.02%	0.002%
80	12.062	3424	3428	3431	rBV3	493	369	0.02%	0.003%
81	12.156	3453	3457	3459	rBV	417	303	0.02%	0.002%
82	12.172	3459	3462	3465	rVV2	474	383	0.02%	0.003%
83	12.333	3508	3512	3513	rBV2	2230	1267	0.08%	0.010%
84	12.416	3535	3538	3541	rBV2	382	285	0.02%	0.002%
85	12.551	3576	3580	3583	rVB3	496	378	0.02%	0.003%
86	12.712	3622	3630	3633	rBV3	443	668	0.04%	0.005%
87	12.747	3638	3641	3643	rBV3	387	313	0.02%	0.003%
88	12.837	3665	3669	3673	rBV4	813	578	0.04%	0.005%
89	13.082	3743	3745	3749	rVB2	446	269	0.02%	0.002%
90	13.255	3795	3799	3802	rBV2	423	395	0.03%	0.003%
91	13.304	3809	3814	3817	rBV3	522	476	0.03%	0.004%
92	13.326	3817	3821	3823	rBV2	574	463	0.03%	0.004%
93	13.497	3869	3874	3883	rVV6	1102	1458	0.09%	0.012%
94	13.535	3883	3886	3889	rVB3	480	334	0.02%	0.003%
95	13.789	3962	3965	3966	rBV2	485	235	0.02%	0.002%
96	13.873	3986	3991	3996	rBV5	500	676	0.04%	0.006%
97	14.021	4033	4037	4042	rBV5	768	658	0.04%	0.005%
98	14.165	4080	4082	4086	rBV3	536	391	0.03%	0.003%
99	14.365	4140	4144	4148	rBV4	647	636	0.04%	0.005%
100	15.223	4408	4411	4414	rBV4	1277	952	0.06%	0.008%


Sum of corrected areas: 12184464

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029766.D
Acq On : 22 Dec 2022 18:14
Operator : SY/MD
Sample : N6193-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

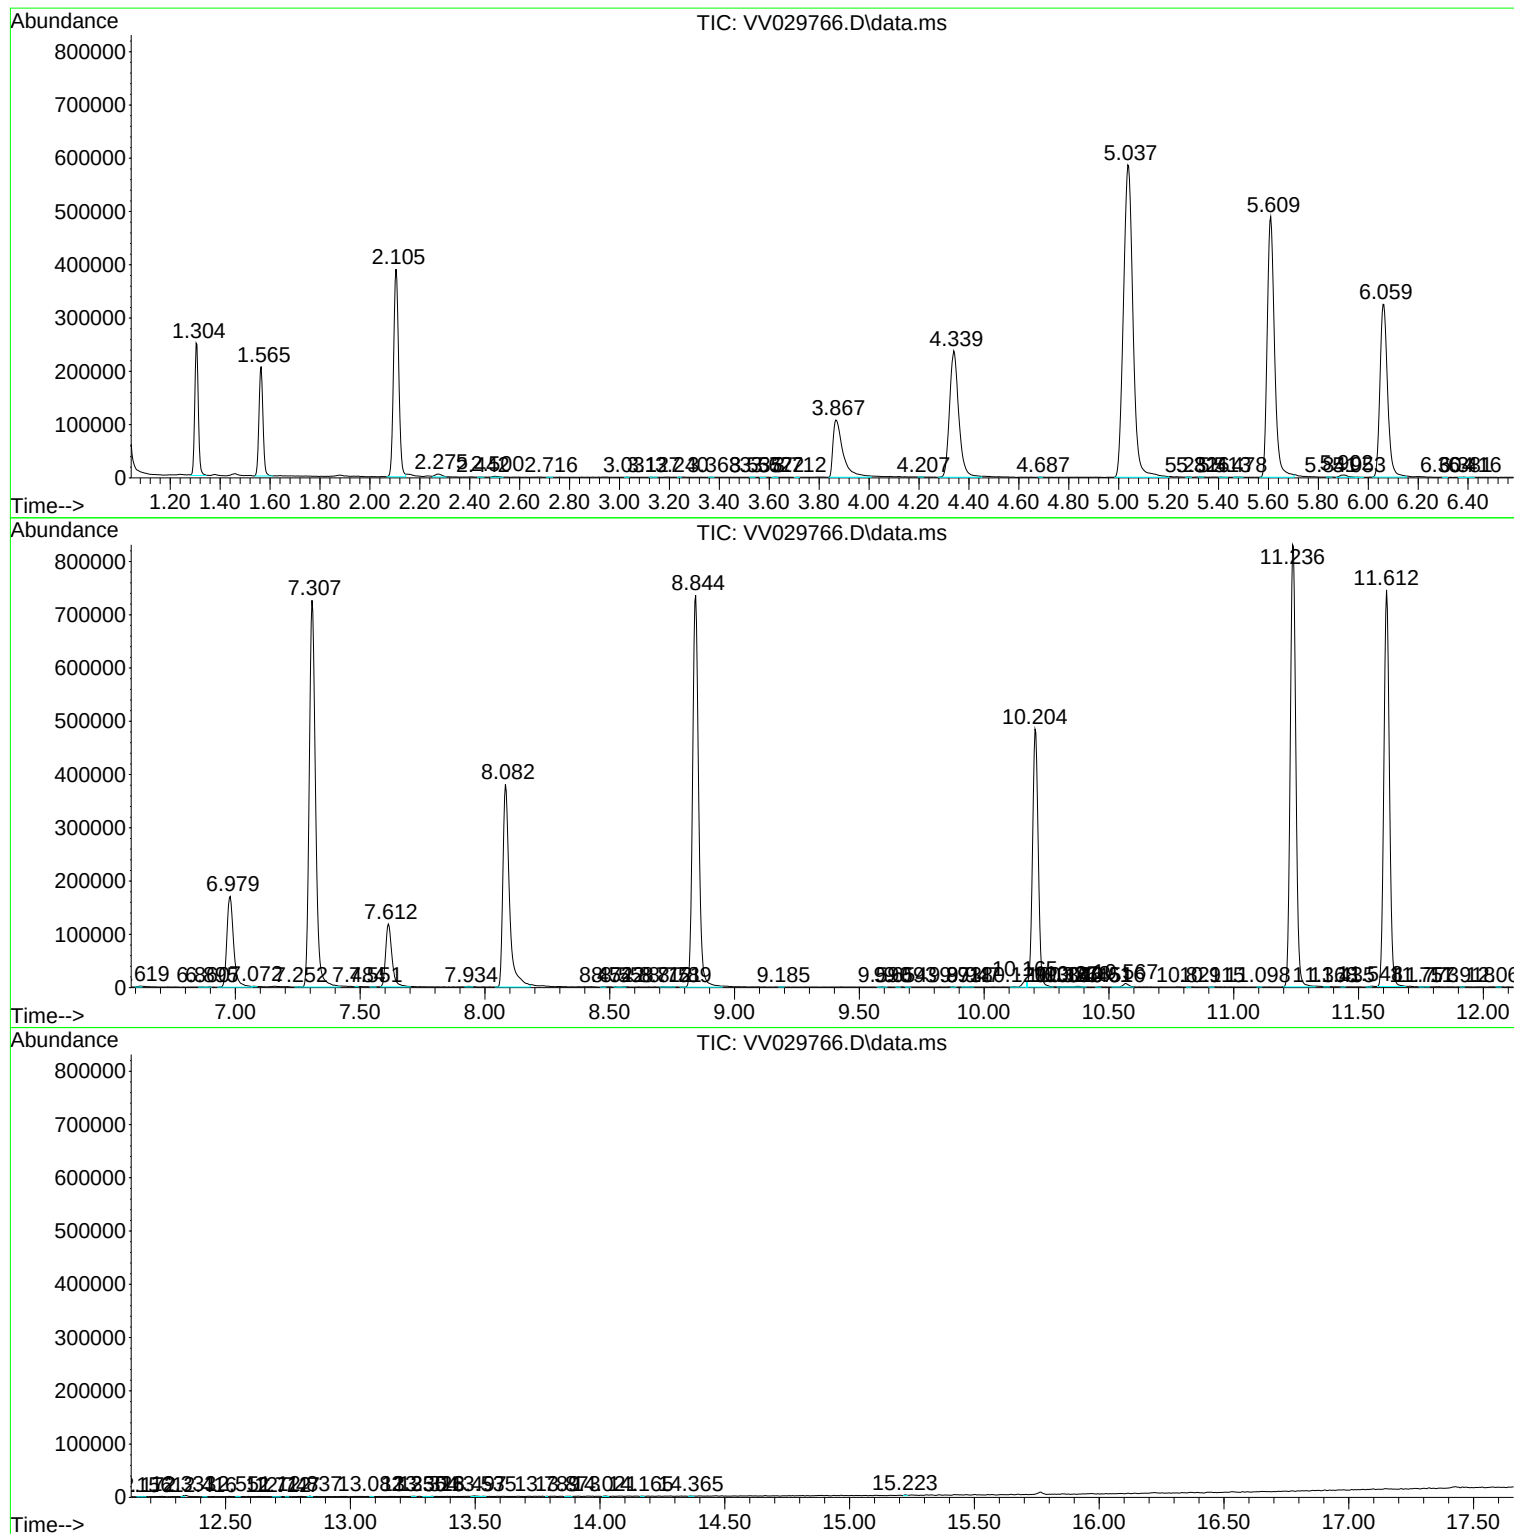

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029766.D
Acq On : 22 Dec 2022 18:14
Operator : SY/MD
Sample : N6193-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029766.D
Acq On : 22 Dec 2022 18:14
Operator : SY/MD
Sample : N6193-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------