

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029767.D
 Acq On : 22 Dec 2022 18:38
 Operator : SY/MD
 Sample : N6195-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	33	rVB	46743	44815	2.74%	0.344%
2	1.175	38	42	48	rVV	11103	9822	0.60%	0.075%
3	1.304	75	82	97	rVB	261080	268793	16.45%	2.063%
4	1.378	100	105	111	rBV	8755	9046	0.55%	0.069%
5	1.564	155	163	177	rBV	215867	239217	14.64%	1.836%
6	1.764	220	225	231	rVB4	1958	2363	0.14%	0.018%
7	2.105	320	331	343	rBV	408512	579103	35.44%	4.445%
8	2.455	437	440	445	rVB3	553	497	0.03%	0.004%
9	2.503	445	455	464	rBV3	1996	3936	0.24%	0.030%
10	2.548	467	469	478	rVB3	552	558	0.03%	0.004%
11	2.757	530	534	541	rVB5	487	565	0.03%	0.004%
12	2.950	590	594	599	rVB4	534	534	0.03%	0.004%
13	3.166	655	661	662	rBV	302	273	0.02%	0.002%
14	3.336	711	714	722	rVB2	293	267	0.02%	0.002%
15	3.867	869	879	921	rBV	108528	307353	18.81%	2.359%
16	4.339	1008	1026	1055	rBV	246453	624771	38.23%	4.796%
17	4.584	1097	1102	1105	rBV3	236	274	0.02%	0.002%
18	4.873	1189	1192	1196	rBV2	405	333	0.02%	0.003%
19	5.040	1221	1244	1285	rBV2	608008	1634125	100.00%	12.544%
20	5.609	1408	1421	1463	rBV	523110	1083264	66.29%	8.315%
21	5.899	1502	1511	1523	rBV5	3403	7327	0.45%	0.056%
22	6.059	1547	1561	1595	rBV	345710	727154	44.50%	5.582%
23	6.262	1622	1624	1631	rVB5	601	373	0.02%	0.003%
24	6.622	1726	1736	1746	rBV6	1831	3927	0.24%	0.030%
25	6.683	1752	1755	1759	rVV2	422	285	0.02%	0.002%
26	6.744	1771	1774	1779	rBV2	355	287	0.02%	0.002%
27	6.780	1779	1785	1787	rBV	365	317	0.02%	0.002%
28	6.979	1835	1847	1878	rBV	179858	330760	20.24%	2.539%
29	7.133	1891	1895	1896	rBV	547	352	0.02%	0.003%
30	7.159	1900	1903	1907	rVV4	724	545	0.03%	0.004%
31	7.214	1917	1920	1924	rVB3	566	405	0.02%	0.003%
32	7.249	1929	1931	1936	rVB2	557	415	0.03%	0.003%
33	7.307	1936	1949	1968	rBV	744576	1322388	80.92%	10.151%
34	7.612	2033	2044	2070	rBV	121646	218415	13.37%	1.677%
35	7.818	2105	2108	2112	rVB4	602	410	0.03%	0.003%
36	7.844	2114	2116	2119	rBV2	301	251	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029767.D
 Acq On : 22 Dec 2022 18:38
 Operator : SY/MD
 Sample : N6195-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	8.082	2179	2190	2230	rBV	390238	720484	44.09%	5.531%
38	8.333	2264	2268	2270	rBV4	640	427	0.03%	0.003%
39	8.471	2309	2311	2316	rBV2	423	442	0.03%	0.003%
40	8.506	2320	2322	2326	rVB2	400	265	0.02%	0.002%
41	8.535	2326	2331	2338	rBV4	645	833	0.05%	0.006%
42	8.587	2343	2347	2351	rVB4	458	429	0.03%	0.003%
43	8.616	2351	2356	2357	rBV4	402	272	0.02%	0.002%
44	8.712	2381	2386	2389	rBV3	401	440	0.03%	0.003%
45	8.844	2414	2427	2461	rBV	803780	1329051	81.33%	10.202%
46	9.091	2500	2504	2507	rVB2	524	475	0.03%	0.004%
47	9.133	2507	2517	2527	rBV7	2128	4279	0.26%	0.033%
48	9.175	2527	2530	2533	rVV2	508	339	0.02%	0.003%
49	9.230	2545	2547	2550	rBV2	522	264	0.02%	0.002%
50	9.342	2580	2582	2587	rBV2	250	258	0.02%	0.002%
51	9.371	2589	2591	2595	rVB	374	260	0.02%	0.002%
52	9.522	2634	2638	2640	rVV2	424	291	0.02%	0.002%
53	9.535	2640	2642	2646	rVV3	432	302	0.02%	0.002%
54	9.776	2712	2717	2722	rVV	289	368	0.02%	0.003%
55	9.809	2722	2727	2734	rVV5	1779	2539	0.16%	0.019%
56	9.931	2759	2765	2767	rBV3	496	544	0.03%	0.004%
57	10.027	2790	2795	2800	rBV2	484	463	0.03%	0.004%
58	10.162	2828	2837	2840	rBV3	10848	14997	0.92%	0.115%
59	10.204	2840	2850	2875	rVB	505011	804501	49.23%	6.175%
60	10.374	2897	2903	2913	rVB3	1569	2414	0.15%	0.019%
61	10.522	2945	2949	2954	rBV3	436	429	0.03%	0.003%
62	10.567	2955	2963	2976	rVB2	6908	11009	0.67%	0.085%
63	10.841	3045	3048	3054	rVB4	526	517	0.03%	0.004%
64	10.902	3060	3067	3070	rBV4	783	912	0.06%	0.007%
65	11.017	3098	3103	3105	rBV2	359	300	0.02%	0.002%
66	11.082	3119	3123	3125	rBV2	532	413	0.03%	0.003%
67	11.140	3130	3141	3155	rVB6	11010	17442	1.07%	0.134%
68	11.236	3159	3171	3197	rBV	898631	1406073	86.04%	10.793%
69	11.516	3255	3258	3263	rVB2	442	451	0.03%	0.003%
70	11.551	3263	3269	3275	rBV7	1879	2759	0.17%	0.021%
71	11.612	3275	3288	3309	rBV	777824	1230681	75.31%	9.447%
72	11.767	3333	3336	3341	rVB2	507	472	0.03%	0.004%
73	11.837	3354	3358	3360	rBV3	454	266	0.02%	0.002%
74	11.866	3360	3367	3370	rVV5	534	564	0.03%	0.004%
75	11.886	3370	3373	3377	rBV3	322	272	0.02%	0.002%
76	12.133	3446	3450	3455	rVB4	452	484	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029767.D
 Acq On : 22 Dec 2022 18:38
 Operator : SY/MD
 Sample : N6195-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	12.197	3468	3470	3473	rVB3	541	275	0.02%	0.002%
78	12.220	3473	3477	3479	rBV2	602	485	0.03%	0.004%
79	12.336	3503	3513	3523	rBV3	22432	34294	2.10%	0.263%
80	12.513	3564	3568	3569	rBV2	364	279	0.02%	0.002%
81	12.558	3576	3582	3584	rBV	514	486	0.03%	0.004%
82	12.715	3627	3631	3633	rBV	384	315	0.02%	0.002%
83	12.834	3663	3668	3671	rBV3	796	665	0.04%	0.005%
84	12.850	3671	3673	3676	rVV2	517	252	0.02%	0.002%
85	12.866	3676	3678	3684	rVB3	615	560	0.03%	0.004%
86	12.898	3685	3688	3690	rBV2	429	295	0.02%	0.002%
87	12.947	3700	3703	3705	rBV2	486	297	0.02%	0.002%
88	13.021	3721	3726	3730	rBV3	621	502	0.03%	0.004%
89	13.043	3730	3733	3736	rBV2	474	286	0.02%	0.002%
90	13.120	3755	3757	3760	rVB2	578	302	0.02%	0.002%
91	13.175	3770	3774	3779	rBV2	431	477	0.03%	0.004%
92	13.246	3793	3796	3799	rBV3	801	440	0.03%	0.003%
93	13.384	3834	3839	3841	rBV3	363	378	0.02%	0.003%
94	13.406	3842	3846	3849	rVV3	439	444	0.03%	0.003%
95	13.496	3867	3874	3884	rVB6	1071	1970	0.12%	0.015%
96	13.554	3890	3892	3897	rVB3	591	455	0.03%	0.003%
97	13.580	3897	3900	3911	rBV3	491	761	0.05%	0.006%
98	13.635	3911	3917	3919	rBV4	715	686	0.04%	0.005%
99	13.705	3936	3939	3942	rVB3	597	352	0.02%	0.003%
100	14.799	4277	4279	4283	rVB4	1090	579	0.04%	0.004%




Sum of corrected areas: 13027336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029767.D
Acq On : 22 Dec 2022 18:38
Operator : SY/MD
Sample : N6195-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

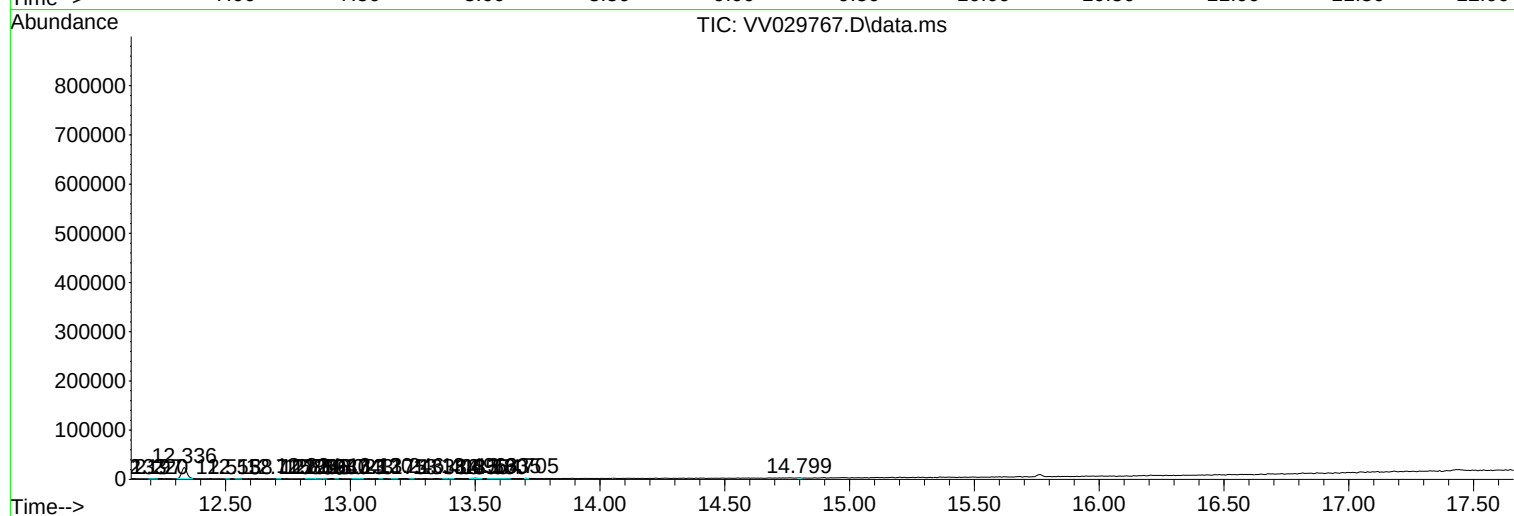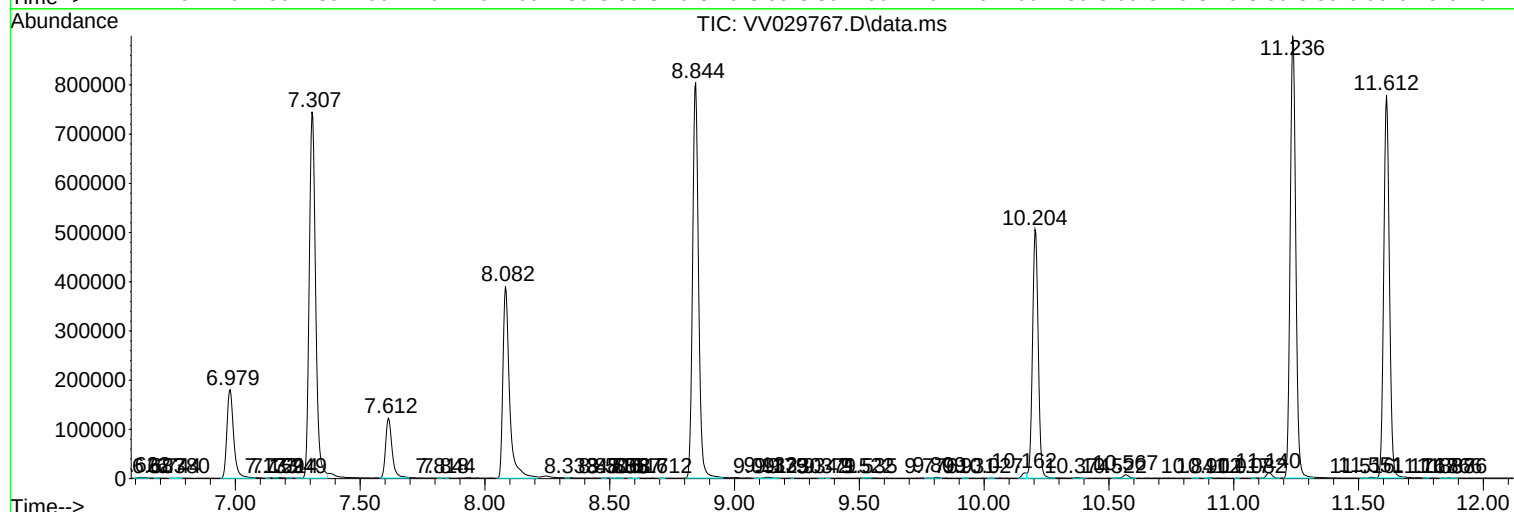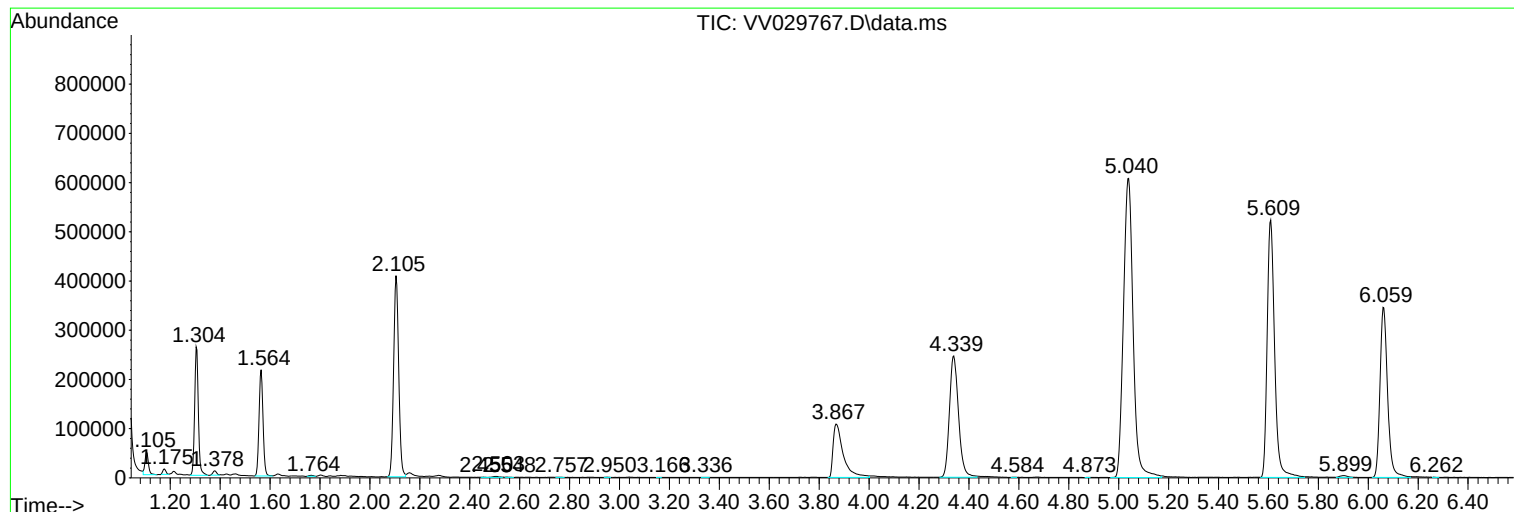

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029767.D
Acq On : 22 Dec 2022 18:38
Operator : SY/MD
Sample : N6195-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029767.D
Acq On : 22 Dec 2022 18:38
Operator : SY/MD
Sample : N6195-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------