

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029768.D
 Acq On : 22 Dec 2022 19:01
 Operator : SY/MD
 Sample : N6195-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	17	20	37	rVB	35959	35039	2.27%	0.281%
2	1.304	75	82	97	rVB	258578	262577	16.98%	2.103%
3	1.565	156	163	176	rVB	204640	227745	14.73%	1.824%
4	2.105	321	331	344	rBV	381826	548497	35.47%	4.392%
5	2.712	518	520	521	rBV	227	85	0.01%	0.001%
6	2.751	528	532	539	rBV3	794	916	0.06%	0.007%
7	3.034	614	620	623	rBV4	1072	1384	0.09%	0.011%
8	3.163	657	660	662	rBV	188	110	0.01%	0.001%
9	3.253	687	688	689	rBV	169	59	0.00%	0.000%
10	3.378	723	727	732	rBV2	215	289	0.02%	0.002%
11	3.436	740	745	750	rBV3	341	385	0.02%	0.003%
12	3.474	753	757	760	rVB2	200	157	0.01%	0.001%
13	3.590	792	793	794	rBV2	128	43	0.00%	0.000%
14	3.645	807	810	817	rBB2	108	103	0.01%	0.001%
15	3.870	870	880	920	rBV	100329	282472	18.26%	2.262%
16	4.343	1009	1027	1058	rBV	230684	594343	38.43%	4.760%
17	4.613	1109	1111	1113	rVB2	141	59	0.00%	0.000%
18	4.629	1113	1116	1120	rBV3	295	254	0.02%	0.002%
19	4.664	1125	1127	1131	rBV	287	257	0.02%	0.002%
20	4.754	1150	1155	1158	rBV2	177	201	0.01%	0.002%
21	4.925	1205	1208	1211	rVB2	245	176	0.01%	0.001%
22	4.953	1215	1217	1221	rVB2	150	101	0.01%	0.001%
23	5.040	1221	1244	1294	rBV2	578388	1546573	100.00%	12.385%
24	5.429	1363	1365	1367	rBV	194	130	0.01%	0.001%
25	5.500	1385	1387	1390	rVB2	412	205	0.01%	0.002%
26	5.609	1407	1421	1460	rBV	517242	1059978	68.54%	8.488%
27	5.899	1503	1511	1526	rVB3	3777	7677	0.50%	0.061%
28	5.973	1531	1534	1535	rBV	404	218	0.01%	0.002%
29	6.059	1547	1561	1600	rBV	325842	690417	44.64%	5.529%
30	6.445	1679	1681	1684	rBV	134	72	0.00%	0.001%
31	6.461	1684	1686	1689	rVB2	154	78	0.01%	0.001%
32	6.481	1689	1692	1695	rBV	208	194	0.01%	0.002%
33	6.564	1712	1718	1720	rBV2	367	305	0.02%	0.002%
34	6.625	1727	1737	1745	rBV6	1805	4172	0.27%	0.033%
35	6.818	1793	1797	1801	rBV2	390	370	0.02%	0.003%
36	6.879	1813	1816	1819	rVB2	253	133	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029768.D
 Acq On : 22 Dec 2022 19:01
 Operator : SY/MD
 Sample : N6195-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.899	1819	1822	1824	rBV	151	95	0.01%	0.001%
38	6.915	1824	1827	1829	rBV3	267	133	0.01%	0.001%
39	6.928	1829	1831	1833	rBV2	172	104	0.01%	0.001%
40	6.979	1835	1847	1875	rBV	166531	310146	20.05%	2.484%
41	7.307	1936	1949	1974	rBV	717310	1257389	81.30%	10.069%
42	7.612	2034	2044	2067	rBV	115300	206542	13.35%	1.654%
43	7.844	2112	2116	2118	rVB	258	162	0.01%	0.001%
44	7.912	2134	2137	2138	rBV2	420	239	0.02%	0.002%
45	7.976	2153	2157	2162	rBV3	433	398	0.03%	0.003%
46	8.082	2180	2190	2231	rBV	365952	684729	44.27%	5.483%
47	8.490	2313	2317	2319	rBV3	326	234	0.02%	0.002%
48	8.548	2333	2335	2338	rBV3	245	142	0.01%	0.001%
49	8.635	2360	2362	2365	rVB2	187	91	0.01%	0.001%
50	8.654	2365	2368	2370	rBV	198	148	0.01%	0.001%
51	8.690	2377	2379	2385	rVB2	371	315	0.02%	0.003%
52	8.844	2413	2427	2459	rBV	785418	1309815	84.69%	10.489%
53	9.130	2511	2516	2523	rBV6	1580	2102	0.14%	0.017%
54	9.397	2595	2599	2602	rBV2	267	203	0.01%	0.002%
55	9.432	2608	2610	2613	rBV2	285	182	0.01%	0.001%
56	9.481	2623	2625	2628	rBV2	253	158	0.01%	0.001%
57	9.510	2631	2634	2638	rBV3	591	524	0.03%	0.004%
58	9.590	2657	2659	2661	rVB	244	77	0.00%	0.001%
59	9.764	2711	2713	2718	rVB2	297	179	0.01%	0.001%
60	9.809	2719	2727	2733	rBV4	2374	3414	0.22%	0.027%
61	9.931	2761	2765	2771	rVB2	398	404	0.03%	0.003%
62	9.956	2771	2773	2776	rBV2	257	146	0.01%	0.001%
63	10.021	2791	2793	2795	rBV2	206	86	0.01%	0.001%
64	10.046	2799	2801	2805	rBB2	137	90	0.01%	0.001%
65	10.072	2805	2809	2812	rBV2	225	221	0.01%	0.002%
66	10.165	2827	2838	2840	rBV2	11175	14578	0.94%	0.117%
67	10.204	2841	2850	2875	rVB	478924	760530	49.18%	6.090%
68	10.371	2895	2902	2904	rBV3	1412	1386	0.09%	0.011%
69	10.439	2919	2923	2926	rBV2	331	354	0.02%	0.003%
70	10.571	2955	2964	2976	rBV3	6009	10037	0.65%	0.080%
71	10.776	3025	3028	3032	rBV	314	246	0.02%	0.002%
72	11.143	3133	3142	3152	rBV3	12918	19097	1.23%	0.153%
73	11.236	3159	3171	3193	rBV	915510	1399830	90.51%	11.210%
74	11.548	3262	3268	3276	rBV6	1652	2789	0.18%	0.022%
75	11.612	3276	3288	3314	rVV	757618	1182436	76.46%	9.469%
76	12.207	3471	3473	3477	rBV2	465	398	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029768.D
Acq On : 22 Dec 2022 19:01
Operator : SY/MD
Sample : N6195-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Title : VOC Analysis

77	12.336	3504	3513	3524	rBV2	33195	51108	3.30%	0.409%
78	12.638	3605	3607	3613	rBV3	449	369	0.02%	0.003%




Sum of corrected areas: 12487400

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029768.D
Acq On : 22 Dec 2022 19:01
Operator : SY/MD
Sample : N6195-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

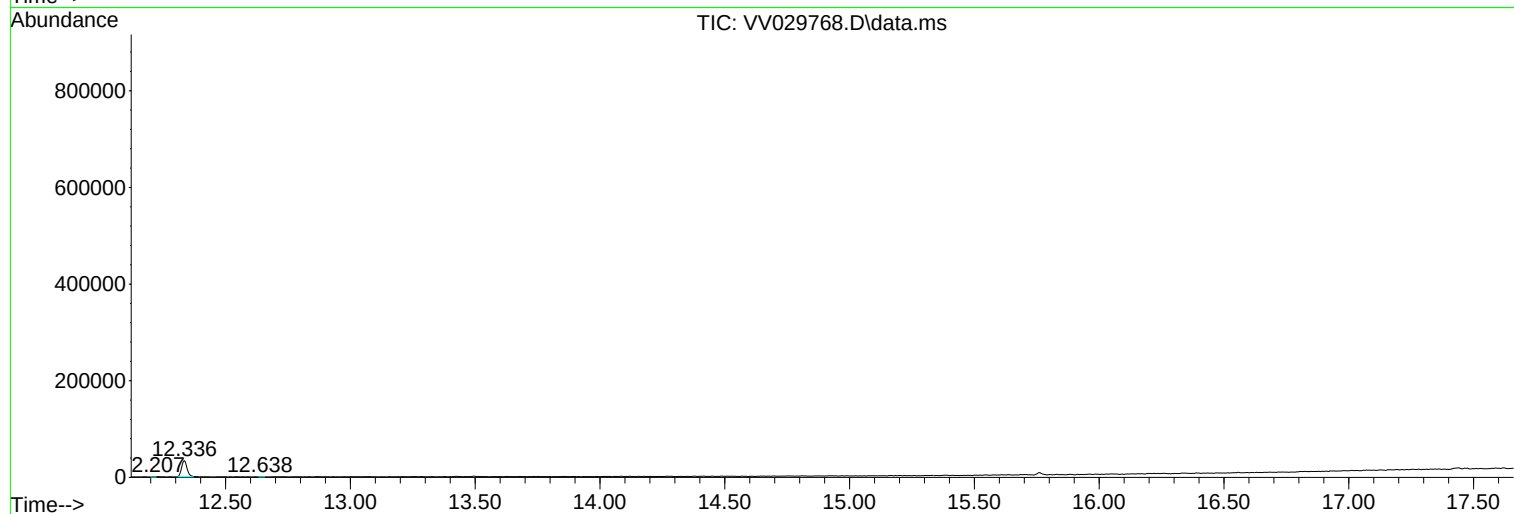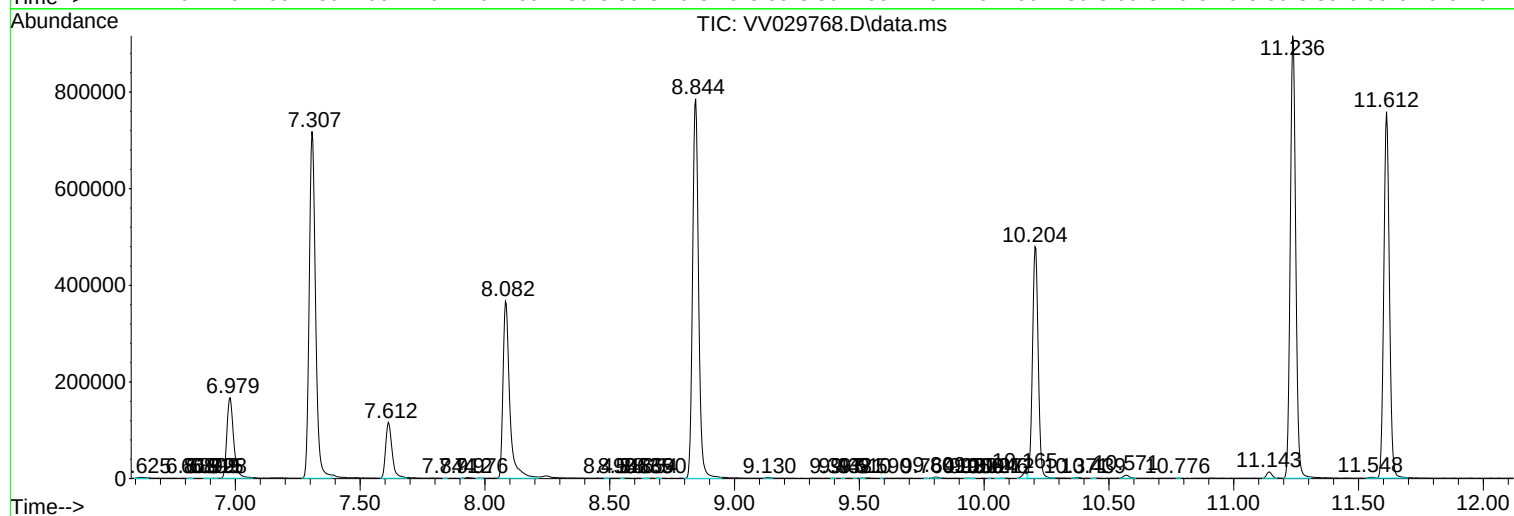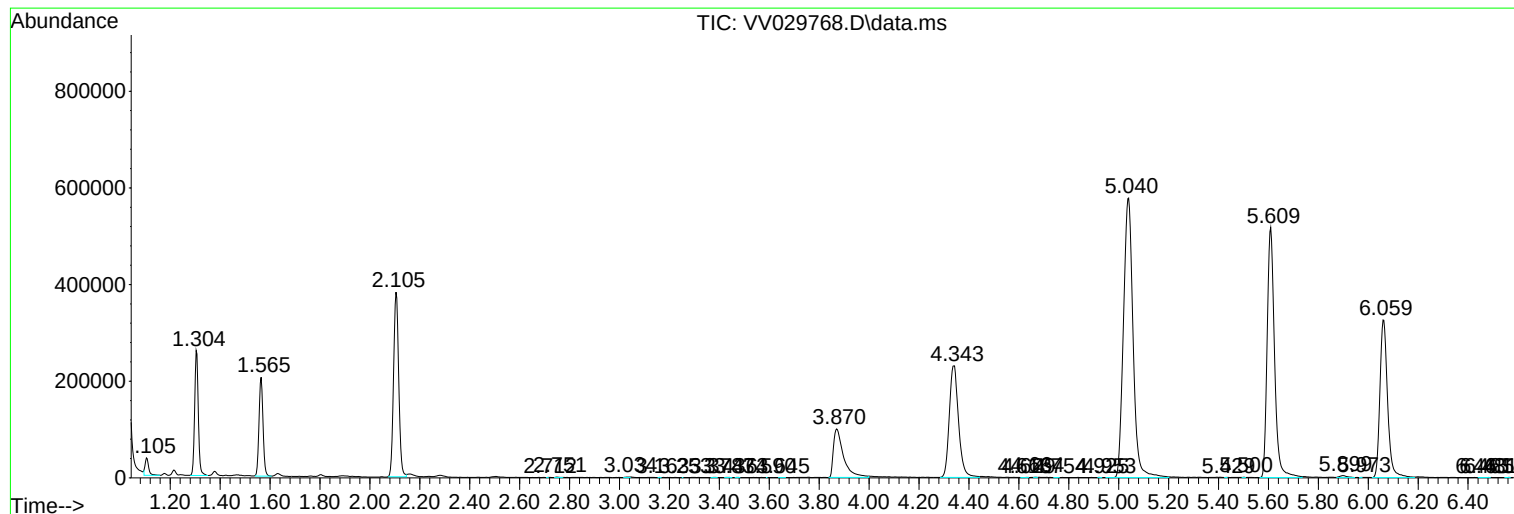

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029768.D
Acq On : 22 Dec 2022 19:01
Operator : SY/MD
Sample : N6195-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029768.D
Acq On : 22 Dec 2022 19:01
Operator : SY/MD
Sample : N6195-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------