

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029770.D
 Acq On : 22 Dec 2022 19:48
 Operator : SY/MD
 Sample : N6195-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	32	rVB	56131	52725	3.22%	0.398%
2	1.214	50	54	60	rVB	10326	8539	0.52%	0.064%
3	1.304	74	82	98	rVB	267881	277741	16.95%	2.097%
4	1.378	101	105	112	rVB	6446	6483	0.40%	0.049%
5	1.564	155	163	176	rVB	218229	240755	14.69%	1.818%
6	1.632	179	184	194	rVB5	5596	6936	0.42%	0.052%
7	1.802	233	237	244	rVB2	5407	5852	0.36%	0.044%
8	2.015	300	303	305	rVB2	677	312	0.02%	0.002%
9	2.105	319	331	343	rBV	408607	582863	35.56%	4.402%
10	2.445	433	437	441	rVV2	404	373	0.02%	0.003%
11	2.503	448	455	456	rBV3	1455	1477	0.09%	0.011%
12	2.761	526	535	539	rBV4	841	1421	0.09%	0.011%
13	2.912	578	582	586	rBV3	328	308	0.02%	0.002%
14	3.037	614	621	630	rVB4	1528	2668	0.16%	0.020%
15	3.606	795	798	802	rBV	372	278	0.02%	0.002%
16	3.716	828	832	837	rBV4	942	1068	0.07%	0.008%
17	3.780	850	852	859	rVB3	509	437	0.03%	0.003%
18	3.870	870	880	930	rBV	105422	309718	18.90%	2.339%
19	4.339	1008	1026	1059	rBV	248963	627925	38.31%	4.742%
20	4.603	1104	1108	1113	rVB2	365	344	0.02%	0.003%
21	4.690	1132	1135	1142	rVB3	389	427	0.03%	0.003%
22	4.754	1153	1155	1161	rVB3	280	289	0.02%	0.002%
23	5.040	1225	1244	1295	rBV2	616268	1638986	100.00%	12.378%
24	5.400	1352	1356	1359	rBV3	372	353	0.02%	0.003%
25	5.487	1379	1383	1389	rVB4	1242	1297	0.08%	0.010%
26	5.542	1394	1400	1408	rBV4	358	665	0.04%	0.005%
27	5.609	1408	1421	1462	rBV	540905	1108526	67.63%	8.372%
28	5.793	1476	1478	1487	rVB3	540	480	0.03%	0.004%
29	5.854	1495	1497	1502	rBV2	413	298	0.02%	0.002%
30	5.899	1502	1511	1512	rBV4	3191	4042	0.25%	0.031%
31	6.059	1547	1561	1593	rBV	349062	731668	44.64%	5.526%
32	6.243	1616	1618	1621	rVB3	589	335	0.02%	0.003%
33	6.313	1633	1640	1643	rBV5	891	913	0.06%	0.007%
34	6.330	1643	1645	1648	rVV2	840	539	0.03%	0.004%
35	6.342	1648	1649	1653	rVB2	648	298	0.02%	0.002%
36	6.629	1727	1738	1741	rBV4	2016	3437	0.21%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029770.D
 Acq On : 22 Dec 2022 19:48
 Operator : SY/MD
 Sample : N6195-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.979	1835	1847	1870	rBV	176872	329928	20.13%	2.492%
38	7.156	1893	1902	1904	rBV6	1180	1572	0.10%	0.012%
39	7.239	1924	1928	1933	rVB5	615	640	0.04%	0.005%
40	7.307	1933	1949	1985	rBV	753915	1344989	82.06%	10.157%
41	7.612	2034	2044	2068	rBV	125844	221168	13.49%	1.670%
42	7.786	2095	2098	2104	rVB4	358	394	0.02%	0.003%
43	7.902	2129	2134	2137	rBV3	376	417	0.03%	0.003%
44	7.934	2137	2144	2152	rVV5	1047	1705	0.10%	0.013%
45	8.082	2179	2190	2231	rBV	385221	725393	44.26%	5.478%
46	8.246	2234	2241	2254	rVB9	3979	9141	0.56%	0.069%
47	8.503	2318	2321	2324	rBV2	577	351	0.02%	0.003%
48	8.545	2330	2334	2337	rBV4	408	377	0.02%	0.003%
49	8.564	2337	2340	2344	rVB3	381	305	0.02%	0.002%
50	8.590	2344	2348	2354	rBV2	405	422	0.03%	0.003%
51	8.664	2368	2371	2374	rVB3	385	274	0.02%	0.002%
52	8.844	2414	2427	2473	rBV	815577	1366033	83.35%	10.316%
53	9.053	2489	2492	2494	rBV2	407	281	0.02%	0.002%
54	9.127	2510	2515	2516	rBV4	1158	950	0.06%	0.007%
55	9.198	2534	2537	2538	rVV	479	281	0.02%	0.002%
56	9.210	2538	2541	2548	rVB3	546	566	0.03%	0.004%
57	9.358	2581	2587	2591	rBV3	269	298	0.02%	0.002%
58	9.403	2599	2601	2606	rVB2	374	300	0.02%	0.002%
59	9.513	2629	2635	2638	rBV4	820	966	0.06%	0.007%
60	9.606	2659	2664	2667	rBV2	284	288	0.02%	0.002%
61	9.699	2688	2693	2697	rBV2	415	436	0.03%	0.003%
62	9.718	2697	2699	2704	rVV3	481	398	0.02%	0.003%
63	9.809	2719	2727	2738	rVV6	3153	5105	0.31%	0.039%
64	9.927	2761	2764	2768	rVV2	393	285	0.02%	0.002%
65	10.050	2798	2802	2805	rVB3	391	310	0.02%	0.002%
66	10.162	2829	2837	2840	rVV2	11120	14745	0.90%	0.111%
67	10.204	2840	2850	2873	rVB	510199	815134	49.73%	6.156%
68	10.345	2891	2894	2896	rBV3	492	292	0.02%	0.002%
69	10.374	2896	2903	2913	rVB3	1539	2518	0.15%	0.019%
70	10.567	2954	2963	2973	rBV	6928	10750	0.66%	0.081%
71	10.699	3000	3004	3007	rVV3	306	279	0.02%	0.002%
72	10.738	3013	3016	3021	rVB3	365	342	0.02%	0.003%
73	10.911	3063	3070	3073	rBV4	674	775	0.05%	0.006%
74	10.950	3079	3082	3088	rBV4	329	362	0.02%	0.003%
75	10.982	3088	3092	3100	rVB3	486	578	0.04%	0.004%
76	11.143	3133	3142	3158	rBV6	13008	19488	1.19%	0.147%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029770.D
 Acq On : 22 Dec 2022 19:48
 Operator : SY/MD
 Sample : N6195-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSN9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.236	3158	3171	3201	rBV	948050	1454036	88.72%	10.981%
78	11.407	3222	3224	3229	rVB3	622	402	0.02%	0.003%
79	11.439	3232	3234	3238	rBV3	435	323	0.02%	0.002%
80	11.554	3263	3270	3276	rBV6	1723	3093	0.19%	0.023%
81	11.612	3276	3288	3305	rBV	793363	1232698	75.21%	9.309%
82	11.857	3361	3364	3368	rBV2	371	320	0.02%	0.002%
83	11.911	3377	3381	3386	rBV3	484	515	0.03%	0.004%
84	11.950	3390	3393	3395	rBV3	432	280	0.02%	0.002%
85	12.169	3459	3461	3466	rVB3	493	420	0.03%	0.003%
86	12.236	3480	3482	3487	rVB3	536	399	0.02%	0.003%
87	12.300	3497	3502	3503	rBV2	589	447	0.03%	0.003%
88	12.333	3504	3512	3528	rVB2	27621	41873	2.55%	0.316%
89	12.464	3545	3553	3560	rBV5	587	1027	0.06%	0.008%
90	12.834	3665	3668	3674	rVB3	743	797	0.05%	0.006%
91	13.123	3752	3758	3760	rBV3	437	404	0.02%	0.003%
92	13.175	3770	3774	3776	rBV2	500	340	0.02%	0.003%
93	13.220	3784	3788	3790	rBV2	474	317	0.02%	0.002%
94	13.349	3826	3828	3834	rVB2	676	454	0.03%	0.003%
95	13.387	3834	3840	3842	rBV3	551	507	0.03%	0.004%
96	13.423	3846	3851	3858	rVB6	1073	1363	0.08%	0.010%
97	13.638	3915	3918	3920	rBV2	544	329	0.02%	0.002%
98	13.882	3991	3994	3997	rBV3	645	484	0.03%	0.004%
99	14.548	4197	4201	4203	rBV5	994	748	0.05%	0.006%
100	14.586	4211	4213	4216	rBV2	658	408	0.02%	0.003%


Sum of corrected areas: 13241596

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029770.D
Acq On : 22 Dec 2022 19:48
Operator : SY/MD
Sample : N6195-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

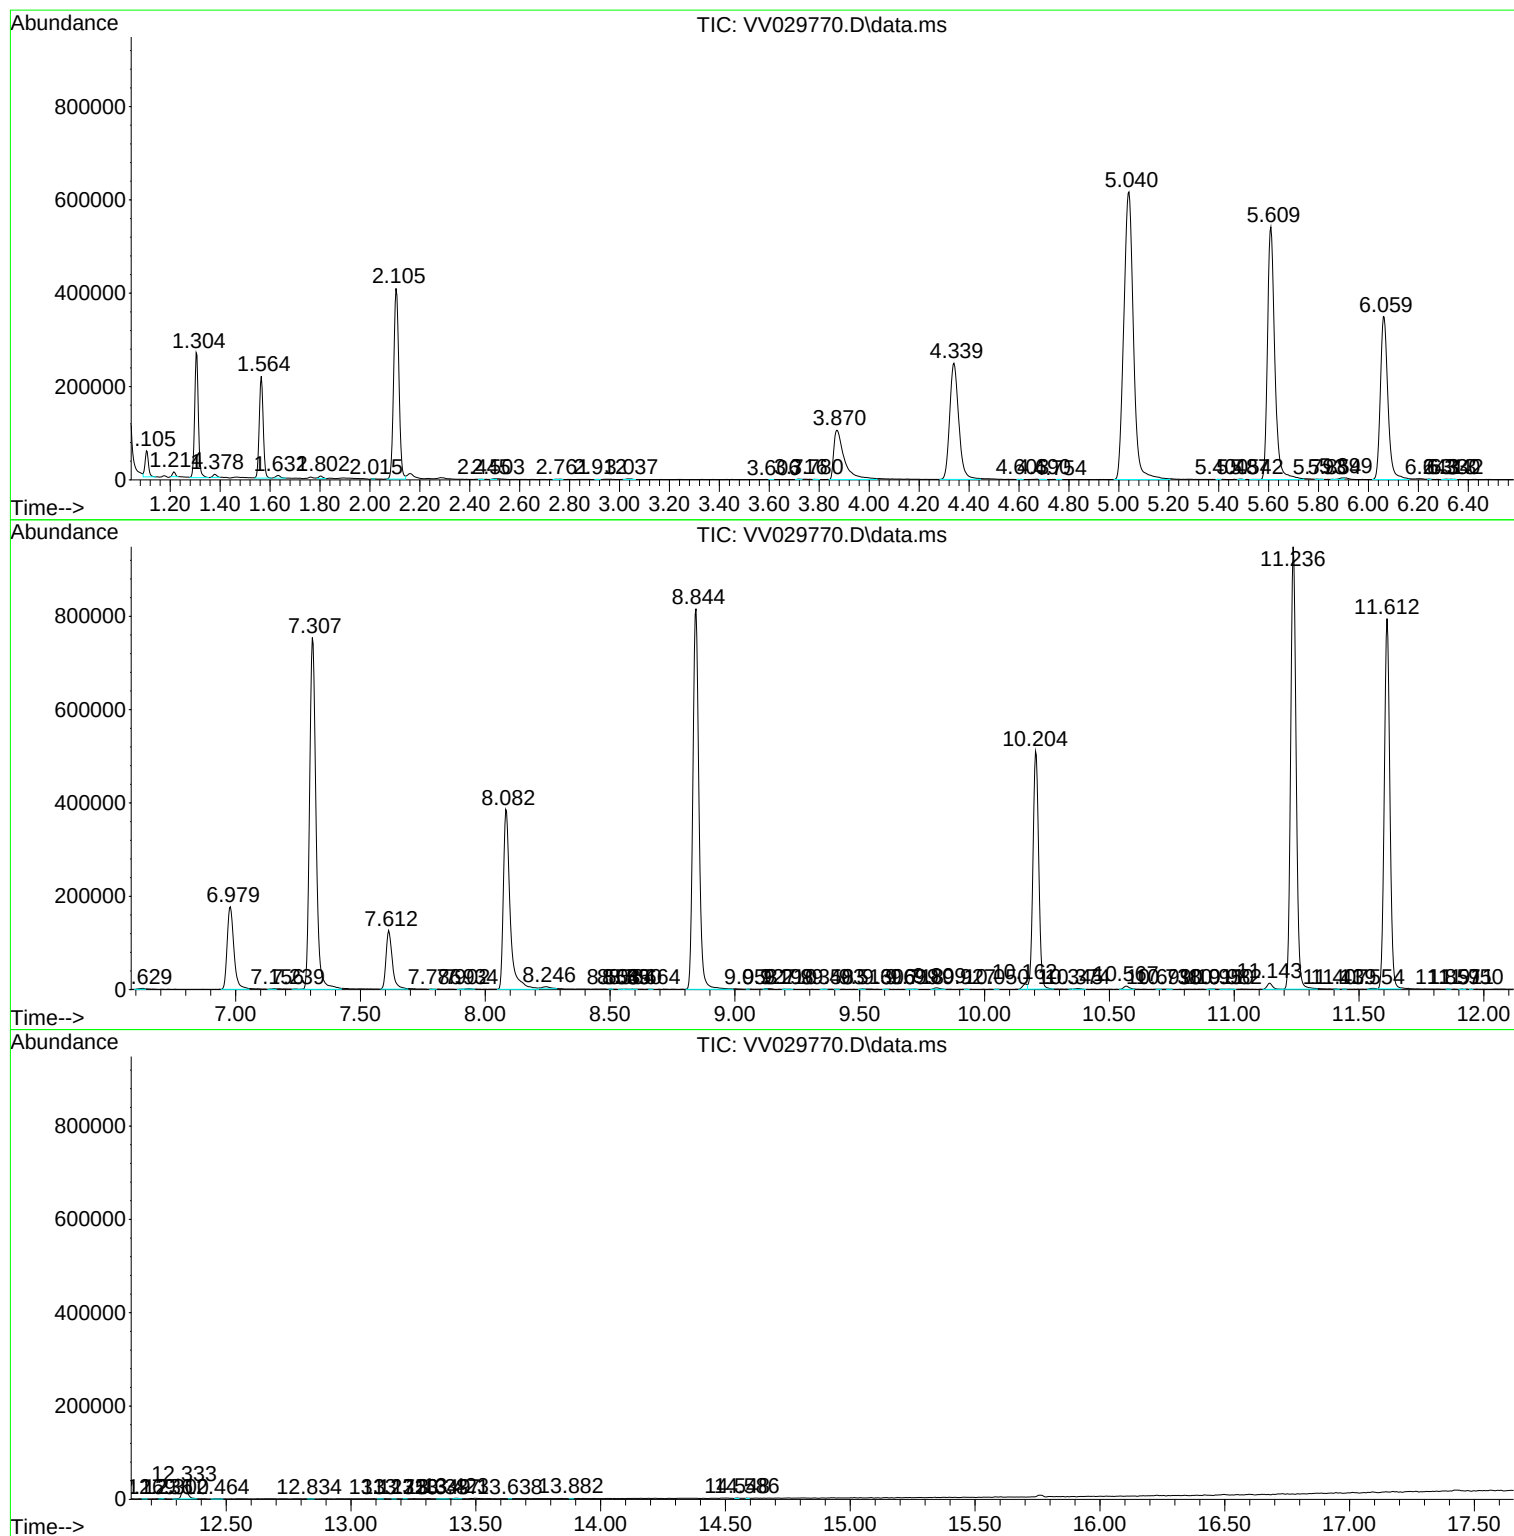

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029770.D
Acq On : 22 Dec 2022 19:48
Operator : SY/MD
Sample : N6195-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029770.D
Acq On : 22 Dec 2022 19:48
Operator : SY/MD
Sample : N6195-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc