

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029772.D
 Acq On : 22 Dec 2022 20:36
 Operator : SY/MD
 Sample : N6195-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029772.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	242131	242138	15.48%	1.944%
2	1.564	155	163	176	rVB	204888	228098	14.58%	1.831%
3	2.105	320	331	343	rBV	393248	556170	35.56%	4.465%
4	2.497	448	453	454	rBV2	1024	912	0.06%	0.007%
5	2.603	482	486	489	rVB4	287	210	0.01%	0.002%
6	2.632	492	495	497	rVB	245	121	0.01%	0.001%
7	2.648	497	500	501	rBV	263	142	0.01%	0.001%
8	2.815	549	552	555	rBV2	263	163	0.01%	0.001%
9	2.960	594	597	602	rBV	243	180	0.01%	0.001%
10	3.011	609	613	614	rBV2	286	186	0.01%	0.001%
11	3.166	657	661	666	rVB2	250	194	0.01%	0.002%
12	3.195	666	670	673	rBV	355	255	0.02%	0.002%
13	3.240	682	684	687	rBV	141	77	0.00%	0.001%
14	3.259	688	690	693	rVV2	160	51	0.00%	0.000%
15	3.307	702	705	707	rBV2	216	129	0.01%	0.001%
16	3.410	734	737	739	rBV	200	126	0.01%	0.001%
17	3.506	765	767	770	rBV	125	63	0.00%	0.001%
18	3.593	791	794	795	rBV	94	58	0.00%	0.000%
19	3.648	808	811	813	rVB2	89	42	0.00%	0.000%
20	3.796	848	857	860	rBV3	477	679	0.04%	0.005%
21	3.870	870	880	918	rBV	105219	300629	19.22%	2.413%
22	4.339	1009	1026	1053	rBV	237162	596222	38.12%	4.786%
23	4.635	1115	1118	1122	rVB2	483	328	0.02%	0.003%
24	4.654	1122	1124	1125	rBV	233	118	0.01%	0.001%
25	4.699	1135	1138	1139	rBV	173	97	0.01%	0.001%
26	4.741	1149	1151	1156	rBV2	339	244	0.02%	0.002%
27	4.776	1159	1162	1163	rBV	184	95	0.01%	0.001%
28	4.796	1166	1168	1170	rVB	154	68	0.00%	0.001%
29	4.844	1179	1183	1186	rBV2	155	108	0.01%	0.001%
30	4.921	1203	1207	1210	rBV2	139	120	0.01%	0.001%
31	4.957	1213	1218	1222	rBV4	371	339	0.02%	0.003%
32	5.040	1225	1244	1295	rBV2	587221	1564211	100.00%	12.557%
33	5.436	1364	1367	1369	rBV	222	144	0.01%	0.001%
34	5.461	1374	1375	1376	rBV	171	49	0.00%	0.000%
35	5.532	1392	1397	1399	rBV2	506	433	0.03%	0.003%
36	5.609	1408	1421	1452	rBV	511603	1043123	66.69%	8.374%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029772.D
 Acq On : 22 Dec 2022 20:36
 Operator : SY/MD
 Sample : N6195-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.063	1548	1562	1598	rBV	330545	692079	44.24%	5.556%
38	6.381	1660	1661	1663	rVB	233	66	0.00%	0.001%
39	6.471	1687	1689	1690	rBV	157	47	0.00%	0.000%
40	6.513	1699	1702	1704	rBV2	176	76	0.00%	0.001%
41	6.616	1729	1734	1741	rBV3	1281	2161	0.14%	0.017%
42	6.715	1764	1765	1767	rBV	228	66	0.00%	0.001%
43	6.799	1788	1791	1795	rVB2	315	159	0.01%	0.001%
44	6.863	1809	1811	1814	rBV	223	121	0.01%	0.001%
45	6.921	1825	1829	1831	rBV2	170	131	0.01%	0.001%
46	6.979	1835	1847	1875	rVV	170157	313491	20.04%	2.517%
47	7.259	1931	1934	1937	rBV2	371	254	0.02%	0.002%
48	7.307	1937	1949	1989	rBV	729484	1282854	82.01%	10.298%
49	7.612	2034	2044	2068	rBV	119055	207702	13.28%	1.667%
50	7.979	2155	2158	2159	rBV	313	175	0.01%	0.001%
51	8.082	2180	2190	2226	rBV	378558	712536	45.55%	5.720%
52	8.513	2322	2324	2327	rBV2	214	106	0.01%	0.001%
53	8.554	2334	2337	2341	rBV3	345	276	0.02%	0.002%
54	8.587	2346	2347	2350	rVB	340	143	0.01%	0.001%
55	8.606	2350	2353	2356	rBV2	195	119	0.01%	0.001%
56	8.712	2379	2386	2399	rVB2	3674	5540	0.35%	0.044%
57	8.844	2405	2427	2465	rBV	785248	1297771	82.97%	10.418%
58	9.133	2511	2517	2523	rBV7	1098	1651	0.11%	0.013%
59	9.159	2523	2525	2526	rBV7	284	82	0.01%	0.001%
60	9.220	2543	2544	2545	rBV7	178	58	0.00%	0.000%
61	9.336	2578	2580	2582	rBV	196	89	0.01%	0.001%
62	9.378	2591	2593	2597	rVB	357	158	0.01%	0.001%
63	9.397	2597	2599	2600	rBV	126	56	0.00%	0.000%
64	9.490	2626	2628	2631	rBV2	240	176	0.01%	0.001%
65	9.583	2653	2657	2659	rVB2	230	177	0.01%	0.001%
66	9.625	2666	2670	2676	rVB3	380	338	0.02%	0.003%
67	9.693	2689	2691	2694	rBV2	294	190	0.01%	0.002%
68	9.799	2722	2724	2726	rBV2	191	88	0.01%	0.001%
69	9.812	2726	2728	2731	rVV	342	179	0.01%	0.001%
70	9.870	2743	2746	2749	rBV	303	240	0.02%	0.002%
71	9.908	2755	2758	2759	rBV	307	152	0.01%	0.001%
72	9.982	2778	2781	2782	rBV	144	78	0.00%	0.001%
73	9.995	2782	2785	2789	rVB2	246	204	0.01%	0.002%
74	10.095	2808	2816	2817	rBV2	407	362	0.02%	0.003%
75	10.165	2829	2838	2840	rBV2	9771	12370	0.79%	0.099%
76	10.204	2841	2850	2871	rVB	497099	777665	49.72%	6.243%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029772.D
 Acq On : 22 Dec 2022 20:36
 Operator : SY/MD
 Sample : N6195-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.429	2917	2920	2922	rBV	239	129	0.01%	0.001%
78	10.442	2922	2924	2928	rVB	379	175	0.01%	0.001%
79	10.471	2928	2933	2936	rBV3	326	351	0.02%	0.003%
80	10.567	2954	2963	2980	rVB2	5871	10358	0.66%	0.083%
81	10.641	2983	2986	2989	rBV	338	282	0.02%	0.002%
82	10.689	2999	3001	3008	rVB2	369	236	0.02%	0.002%
83	11.107	3127	3131	3135	rBV4	490	465	0.03%	0.004%
84	11.143	3135	3142	3149	rBV6	2942	4076	0.26%	0.033%
85	11.236	3159	3171	3198	rBV	894560	1386175	88.62%	11.128%
86	11.612	3276	3288	3311	rBV	776338	1194661	76.37%	9.590%
87	12.332	3505	3512	3526	rVB6	8180	12649	0.81%	0.102%
88	12.416	3536	3538	3541	rBV	399	239	0.02%	0.002%
89	12.924	3691	3696	3698	rBV3	621	572	0.04%	0.005%
90	12.969	3707	3710	3712	rBV2	345	219	0.01%	0.002%




Sum of corrected areas: 12457095

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029772.D
Acq On : 22 Dec 2022 20:36
Operator : SY/MD
Sample : N6195-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

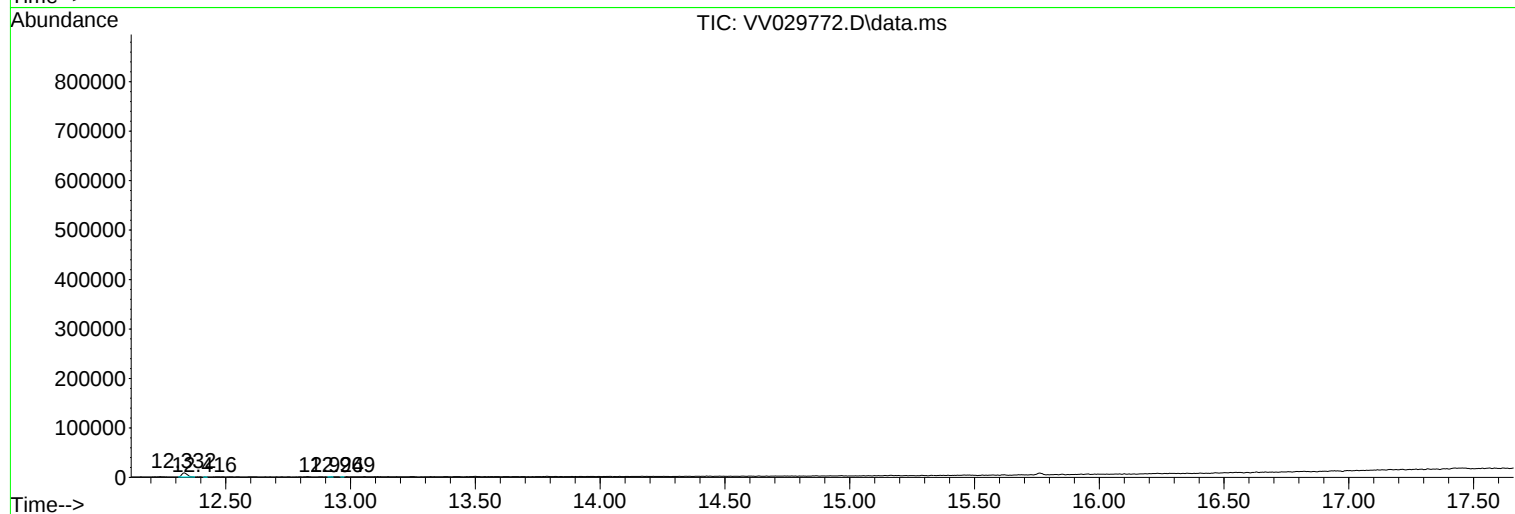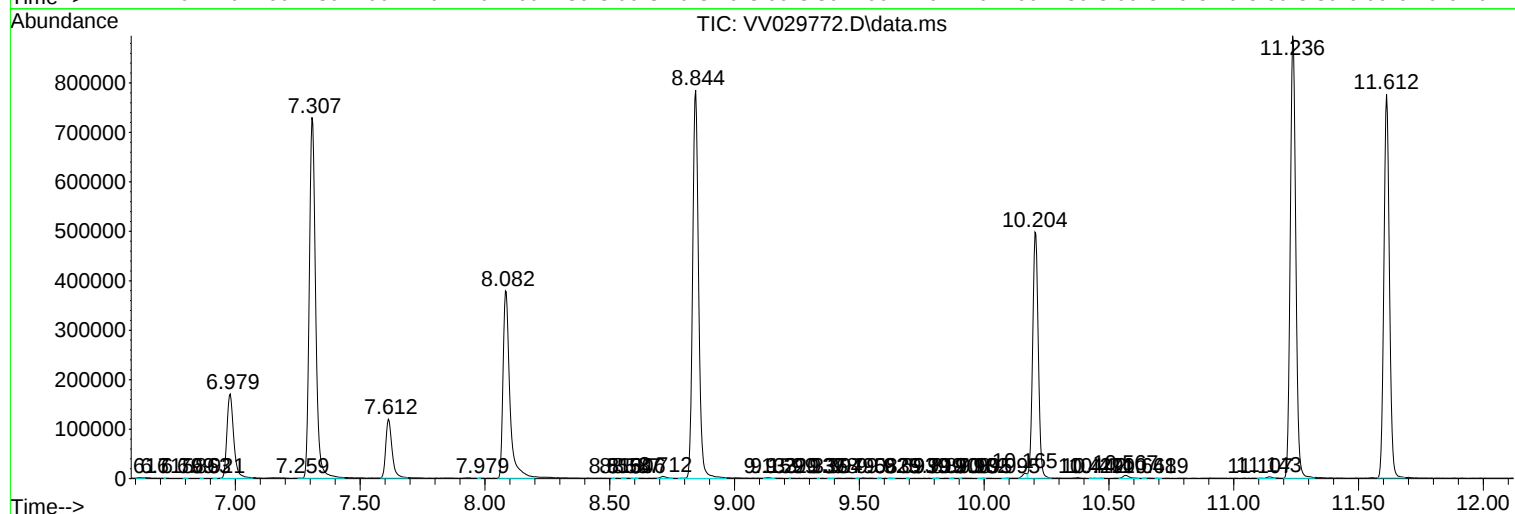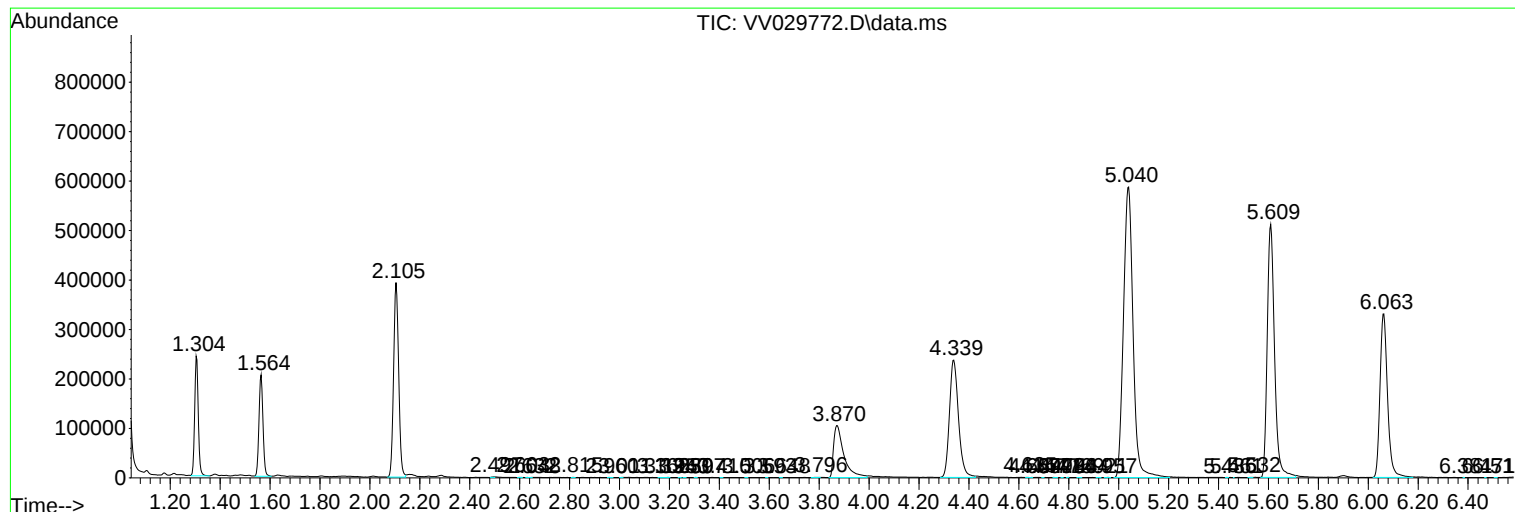

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029772.D
Acq On : 22 Dec 2022 20:36
Operator : SY/MD
Sample : N6195-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029772.D
Acq On : 22 Dec 2022 20:36
Operator : SY/MD
Sample : N6195-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc