

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029773.D
 Acq On : 22 Dec 2022 20:59
 Operator : SY/MD
 Sample : N6195-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029773.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	17	20	37	rVB	38668	37121	2.30%	0.290%
2	1.304	76	82	99	rVB	274898	275296	17.09%	2.151%
3	1.564	155	163	177	rVB	215764	239979	14.90%	1.875%
4	2.105	320	331	343	rBV	401530	576161	35.76%	4.501%
5	2.500	448	454	467	rBV6	1752	3767	0.23%	0.029%
6	2.651	498	501	507	rVB3	447	396	0.02%	0.003%
7	2.690	511	513	518	rVB2	407	242	0.02%	0.002%
8	2.728	521	525	526	rVB2	145	84	0.01%	0.001%
9	2.815	549	552	555	rBV	273	174	0.01%	0.001%
10	2.899	576	578	582	rVB	341	162	0.01%	0.001%
11	2.937	587	590	594	rBV	444	319	0.02%	0.002%
12	2.953	594	595	597	rBV	201	93	0.01%	0.001%
13	3.040	616	622	627	rBV7	1169	1507	0.09%	0.012%
14	3.066	628	630	633	rBV	178	80	0.00%	0.001%
15	3.108	640	643	645	rBV2	137	98	0.01%	0.001%
16	3.301	700	703	704	rBV2	159	91	0.01%	0.001%
17	3.336	709	714	716	rBV2	242	219	0.01%	0.002%
18	3.384	727	729	732	rBV	161	101	0.01%	0.001%
19	3.500	762	765	768	rBV2	98	82	0.01%	0.001%
20	3.542	774	778	779	rBV	135	99	0.01%	0.001%
21	3.574	786	788	793	rVB	159	119	0.01%	0.001%
22	3.609	793	799	800	rBV2	249	128	0.01%	0.001%
23	3.728	829	836	838	rBV3	628	536	0.03%	0.004%
24	3.783	850	853	856	rBV3	361	282	0.02%	0.002%
25	3.822	863	865	867	rBV2	183	91	0.01%	0.001%
26	3.870	870	880	918	rBV	106813	301816	18.74%	2.358%
27	4.339	1010	1026	1061	rBV	241509	616630	38.28%	4.818%
28	4.658	1121	1125	1128	rBV3	634	534	0.03%	0.004%
29	4.728	1144	1147	1149	rBV2	220	130	0.01%	0.001%
30	4.783	1162	1164	1170	rVB3	239	188	0.01%	0.001%
31	4.844	1181	1183	1186	rBV	141	86	0.01%	0.001%
32	4.899	1197	1200	1204	rVB2	258	164	0.01%	0.001%
33	4.928	1205	1209	1210	rBV	124	81	0.01%	0.001%
34	4.940	1210	1213	1217	rBV2	125	124	0.01%	0.001%
35	5.037	1223	1243	1287	rBV2	604578	1610973	100.00%	12.586%
36	5.442	1366	1369	1371	rBV2	344	261	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122222\
 Data File : VW029773.D
 Acq On : 22 Dec 2022 20:59
 Operator : SY/MD
 Sample : N6195-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.519	1387	1393	1396	rBV2	138	107	0.01%	0.001%
38	5.548	1400	1402	1405	rBV2	117	85	0.01%	0.001%
39	5.609	1408	1421	1465	rBV	513448	1050923	65.24%	8.211%
40	5.818	1484	1486	1489	rBV3	461	237	0.01%	0.002%
41	5.902	1503	1512	1525	rVB4	3297	6806	0.42%	0.053%
42	6.063	1547	1562	1598	rBV	343551	721478	44.79%	5.637%
43	6.342	1648	1649	1651	rBV	161	81	0.01%	0.001%
44	6.474	1683	1690	1692	rBV2	291	247	0.02%	0.002%
45	6.500	1692	1698	1700	rBV2	237	209	0.01%	0.002%
46	6.532	1700	1708	1713	rVB2	335	457	0.03%	0.004%
47	6.574	1718	1721	1725	rBV2	310	238	0.01%	0.002%
48	6.619	1728	1735	1746	rBV3	1515	3210	0.20%	0.025%
49	6.709	1760	1763	1764	rBV2	260	118	0.01%	0.001%
50	6.757	1776	1778	1780	rVB	204	83	0.01%	0.001%
51	6.799	1789	1791	1794	rVB2	262	127	0.01%	0.001%
52	6.895	1818	1821	1825	rBV3	197	147	0.01%	0.001%
53	6.921	1826	1829	1833	rVB2	338	183	0.01%	0.001%
54	6.979	1833	1847	1884	rBV	174916	325629	20.21%	2.544%
55	7.243	1926	1929	1930	rBV	269	160	0.01%	0.001%
56	7.307	1936	1949	1971	rBV	747889	1318663	81.86%	10.303%
57	7.612	2033	2044	2067	rBV	120573	216688	13.45%	1.693%
58	7.837	2112	2114	2118	rVB3	385	218	0.01%	0.002%
59	7.899	2126	2133	2136	rBV3	327	495	0.03%	0.004%
60	7.931	2139	2143	2154	rVB3	1006	1673	0.10%	0.013%
61	8.082	2180	2190	2224	rBV	381202	719241	44.65%	5.619%
62	8.436	2297	2300	2302	rBV3	293	178	0.01%	0.001%
63	8.677	2372	2375	2376	rBV	399	203	0.01%	0.002%
64	8.751	2395	2398	2401	rBV	296	209	0.01%	0.002%
65	8.844	2414	2427	2465	rBV	771738	1286648	79.87%	10.052%
66	9.140	2509	2519	2526	rVB5	1202	1914	0.12%	0.015%
67	9.217	2540	2543	2544	rBV	186	87	0.01%	0.001%
68	9.307	2565	2571	2576	rBV2	223	336	0.02%	0.003%
69	9.384	2591	2595	2599	rBV	253	222	0.01%	0.002%
70	9.477	2620	2624	2625	rBV2	367	238	0.01%	0.002%
71	9.680	2685	2687	2689	rBV	204	84	0.01%	0.001%
72	9.702	2691	2694	2696	rBV	276	205	0.01%	0.002%
73	9.734	2701	2704	2706	rBV2	249	165	0.01%	0.001%
74	9.763	2711	2713	2716	rBV	144	84	0.01%	0.001%
75	9.808	2720	2727	2738	rBV8	2418	4059	0.25%	0.032%
76	10.017	2789	2792	2796	rBV3	196	161	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029773.D
 Acq On : 22 Dec 2022 20:59
 Operator : SY/MD
 Sample : N6195-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.104	2817	2819	2823	rVB2	312	142	0.01%	0.001%
78	10.162	2828	2837	2840	rBV2	10647	14321	0.89%	0.112%
79	10.204	2841	2850	2871	rVB	507127	795277	49.37%	6.213%
80	10.439	2918	2923	2924	rBV	302	219	0.01%	0.002%
81	10.509	2943	2945	2949	rBV2	231	192	0.01%	0.002%
82	10.529	2949	2951	2952	rVV	233	89	0.01%	0.001%
83	10.567	2956	2963	2974	rVV3	6021	9153	0.57%	0.072%
84	10.651	2987	2989	2993	rVB3	245	185	0.01%	0.001%
85	10.738	3014	3016	3019	rBV2	201	131	0.01%	0.001%
86	10.892	3058	3064	3065	rBV2	491	396	0.02%	0.003%
87	11.021	3102	3104	3106	rBV2	356	165	0.01%	0.001%
88	11.143	3135	3142	3152	rBV4	9259	13187	0.82%	0.103%
89	11.236	3159	3171	3201	rBV	887278	1377161	85.49%	10.760%
90	11.413	3224	3226	3228	rBV	378	178	0.01%	0.001%
91	11.451	3236	3238	3239	rBV2	362	182	0.01%	0.001%
92	11.516	3255	3258	3259	rBV	382	204	0.01%	0.002%
93	11.551	3265	3269	3275	rBV4	869	1138	0.07%	0.009%
94	11.612	3276	3288	3314	rVV	783059	1222564	75.89%	9.552%
95	11.943	3389	3391	3394	rBV2	368	246	0.02%	0.002%
96	12.027	3414	3417	3424	rVB2	645	557	0.03%	0.004%
97	12.062	3424	3428	3431	rBV2	359	332	0.02%	0.003%
98	12.194	3464	3469	3473	rBV3	404	478	0.03%	0.004%
99	12.332	3504	3512	3529	rVB2	20947	32006	1.99%	0.250%
100	12.705	3626	3628	3631	rBV2	490	351	0.02%	0.003%




Sum of corrected areas: 12799364

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029773.D
Acq On : 22 Dec 2022 20:59
Operator : SY/MD
Sample : N6195-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

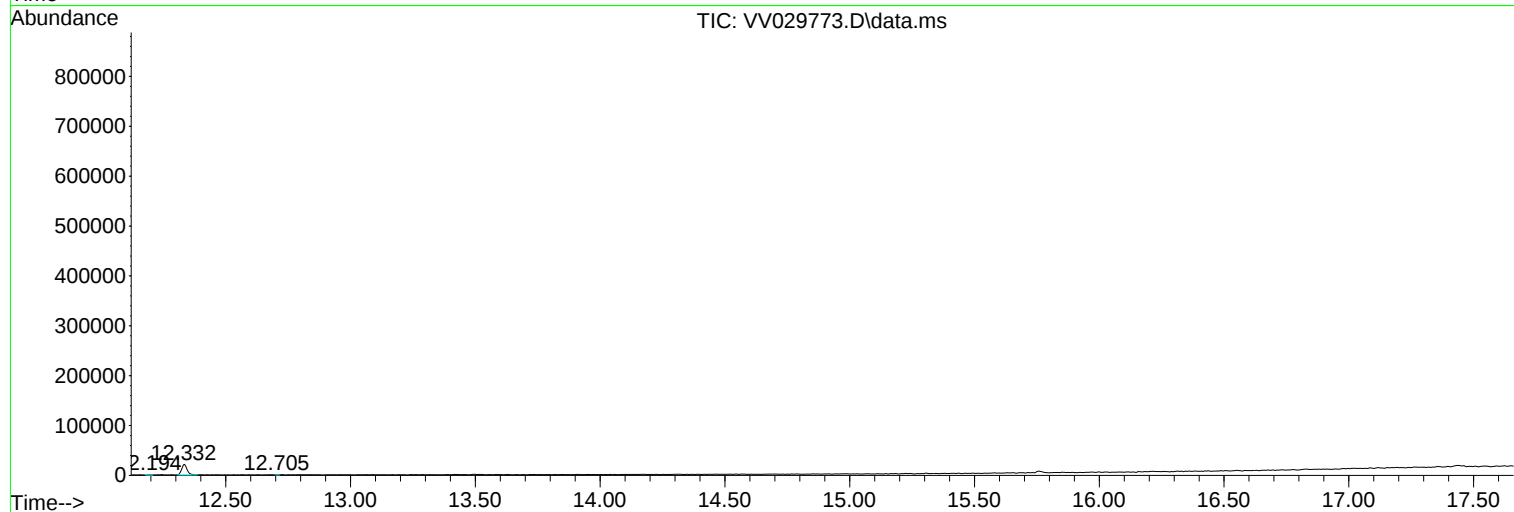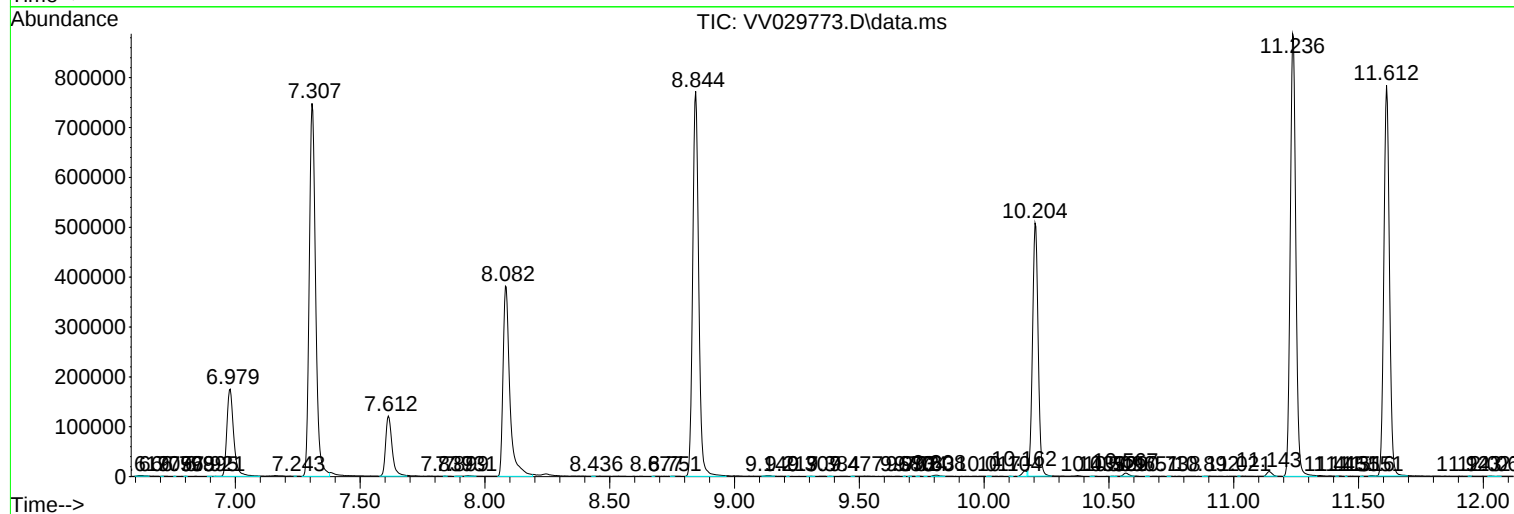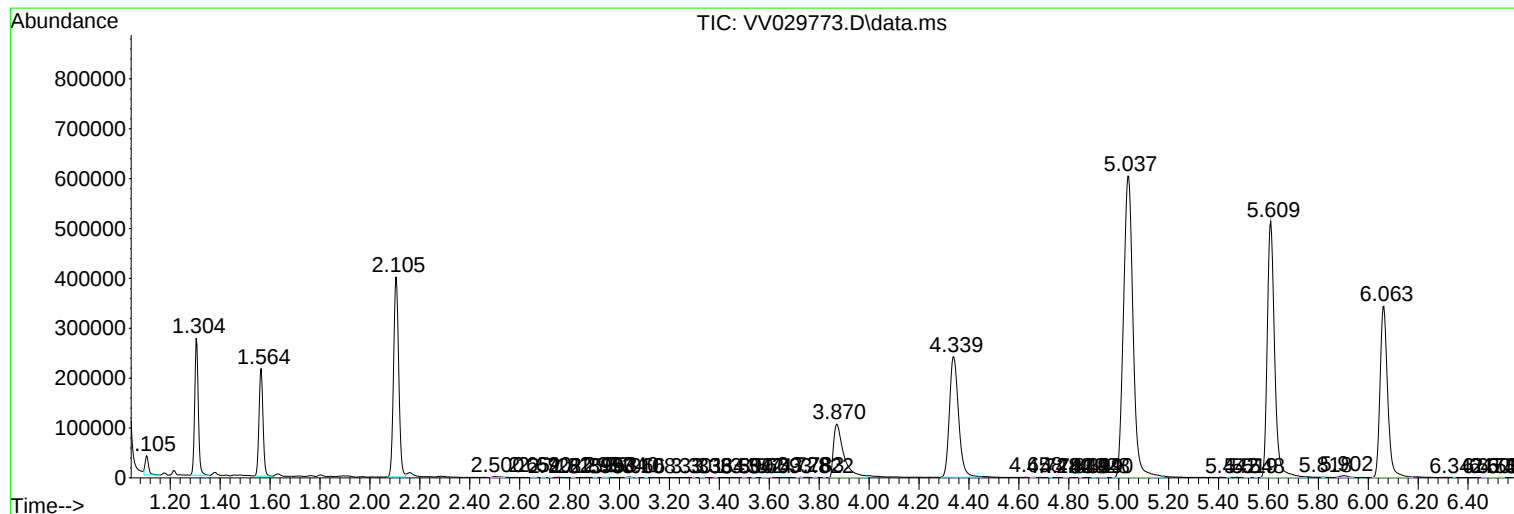

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029773.D
Acq On : 22 Dec 2022 20:59
Operator : SY/MD
Sample : N6195-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
Data File : VV029773.D
Acq On : 22 Dec 2022 20:59
Operator : SY/MD
Sample : N6195-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------