
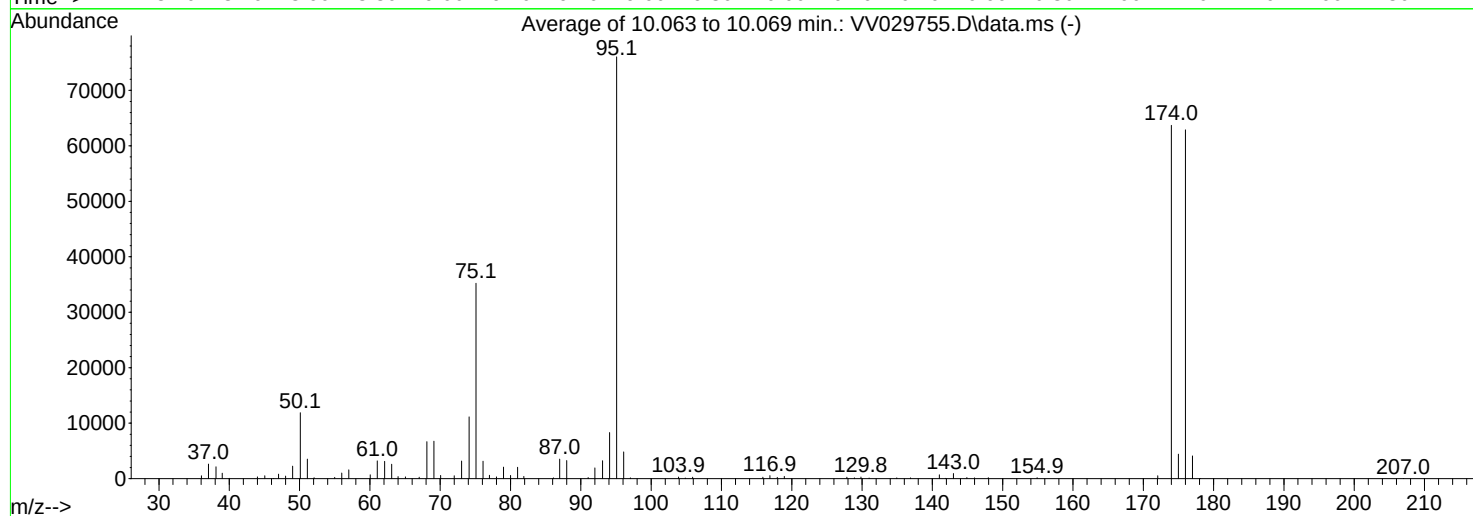


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122222\
 Data File : VV029755.D
 Acq On : 22 Dec 2022 10:07
 Operator : SY/MD
 Sample : BFB359
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB359

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 21 00:15:13 2022

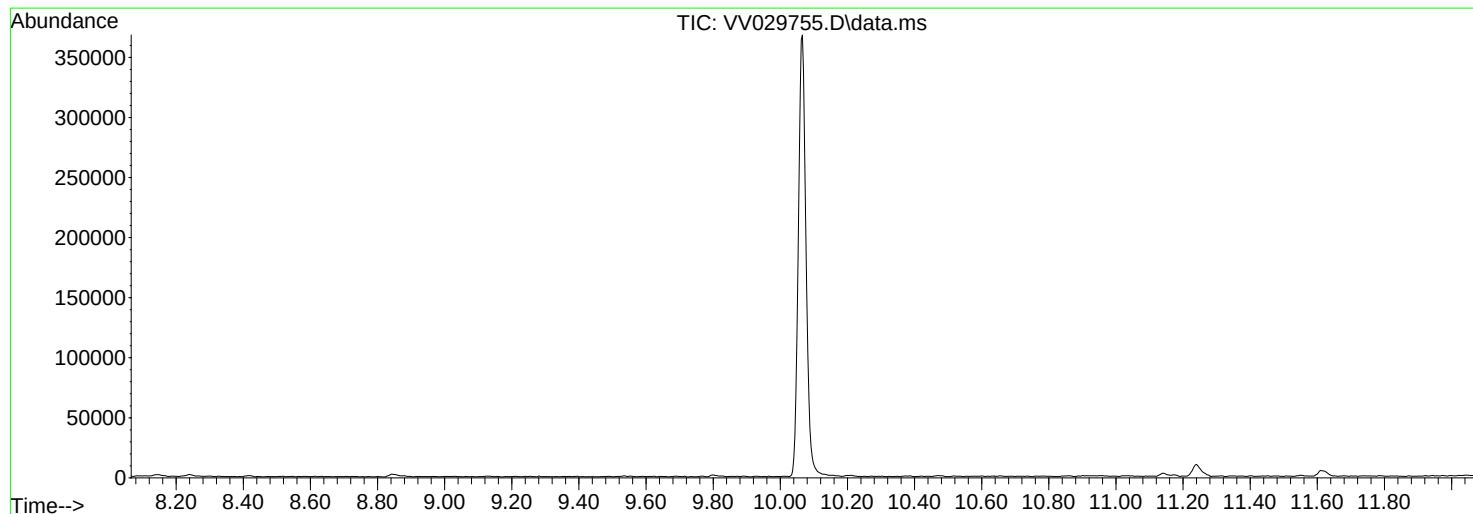

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	11885	PASS
75	95	30	80	46.3	35208	PASS
95	95	100	100	100.0	76040	PASS
96	95	5	9	6.3	4811	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.8	63691	PASS
175	174	5	9	6.9	4408	PASS
176	174	95	105	98.7	62883	PASS
177	176	5	10	6.5	4101	PASS

Scan 2794 (10.024 min): VV029755.D\data.ms
BFB359

m/z	Abundance
40.10	258.0
43.00	119.0
44.00	676.0
207.00	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359

m/z	Abundance
36.10	538.0
37.10	2721.0
38.10	2131.0
39.00	976.0
40.00	276.0
44.10	930.0
45.00	510.0
47.00	868.0
48.00	470.0
49.00	2396.0
50.10	12293.0
51.10	3701.0
52.00	214.0
55.00	229.0
56.00	1115.0
57.00	1648.0
60.00	731.0
61.10	3412.0
62.10	3252.0
63.10	2647.0
64.00	424.0
65.00	328.0
67.00	246.0
68.10	6889.0
69.10	7089.0
70.10	650.0
72.00	525.0
73.10	3219.0
74.10	11519.0
75.10	36176.0
76.10	3321.0
77.00	627.0
78.00	302.0
79.00	2084.0
80.00	561.0
81.00	2121.0
81.90	408.0
86.20	147.0
87.00	3671.0
88.00	3358.0
91.00	228.0
92.00	2050.0
93.10	3447.0
94.10	8695.0
95.10	78120.0
96.10	5026.0
97.10	185.0
103.90	295.0
104.90	110.0
105.90	270.0
115.90	290.0
116.90	555.0
118.00	220.0
118.90	431.0
127.90	234.0
128.90	150.0
129.90	297.0
131.00	127.0
134.90	135.0
136.90	132.0
141.00	726.0
141.90	112.0
143.00	940.0
144.90	206.0
146.00	122.0
147.90	225.0
154.90	169.0
172.10	510.0
174.00	63776.0
175.00	4658.0
176.00	63192.0
177.00	4067.0
178.10	103.0
207.00	219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359

m/z	Abundance
36.10	541.0
37.00	2761.0
38.10	2214.0
39.00	1015.0
40.00	305.0
44.00	1009.0
45.00	517.0
47.00	845.0
48.00	471.0
49.00	2291.0
50.10	12187.0
51.10	3616.0
52.00	202.0
55.00	252.0
56.00	1047.0
57.00	1644.0
60.00	704.0
61.10	3321.0
62.10	3237.0
63.10	2717.0
64.00	409.0
65.10	330.0
67.00	275.0
68.10	6893.0
69.10	6946.0
70.10	596.0
72.00	557.0
73.00	3327.0
74.10	11400.0
75.10	36304.0
76.10	3241.0
77.00	616.0
78.00	338.0
79.00	2151.0
80.00	606.0
81.00	2106.0
81.90	399.0
86.10	142.0
87.00	3676.0
88.00	3332.0
91.10	198.0
92.00	2022.0
93.10	3328.0
94.10	8524.0
95.10	78784.0
96.10	4947.0
97.10	148.0
103.90	304.0
104.80	128.0
105.90	279.0
115.90	270.0
116.90	579.0
118.00	239.0
119.00	393.0
127.90	276.0
128.90	145.0
129.90	318.0
131.00	131.0
134.90	138.0
136.90	145.0
141.00	710.0
141.90	104.0
143.00	966.0
144.90	213.0
146.00	165.0
148.00	200.0
154.90	170.0
172.10	532.0
174.00	65816.0
175.00	4520.0
176.00	65040.0
177.00	4211.0
207.00	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359

m/z	Abundance
36.00	492.0
37.00	2375.0
38.10	2100.0
39.00	993.0
40.00	338.0
44.00	1037.0
45.10	498.0
46.30	103.0
47.00	710.0
48.00	418.0
49.00	2051.0
50.10	11176.0
51.10	3277.0
52.10	154.0
55.00	213.0
56.00	845.0
57.00	1504.0
60.10	624.0
61.00	2884.0
62.10	2885.0
63.10	2465.0
64.00	317.0
65.10	341.0
67.00	259.0
68.10	6232.0
69.10	6239.0
70.00	532.0
72.00	499.0
73.00	3009.0
74.10	10490.0
75.10	33144.0
76.10	2844.0
77.00	559.0
78.00	358.0
79.00	2045.0
80.00	565.0
81.00	1903.0
81.90	368.0
86.00	119.0
87.00	3215.0
88.00	3129.0
91.00	153.0
92.00	1767.0
93.10	2906.0
94.10	7674.0
95.10	71216.0
96.10	4459.0
97.00	120.0
103.90	281.0
104.80	127.0
105.90	241.0
112.00	108.0
115.90	224.0
116.90	511.0
117.90	242.0
118.90	351.0
127.80	314.0
128.90	173.0
129.80	287.0
131.00	112.0
135.00	123.0
136.90	124.0
141.00	644.0
143.00	844.0
144.90	189.0
146.00	174.0
148.00	139.0
154.90	141.0
172.00	518.0
174.00	61480.0
175.00	4045.0
176.00	60416.0
177.00	4025.0
207.00	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB359