

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122319\
 Data File : VV014161.D
 Acq On : 23 Dec 2019 16:23
 Operator : SY/MD
 Sample : VV1223WBL01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK38

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122319WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	62	70	83	rBV	236677	246231	16.63%	2.168%
2	1.582	145	153	165	rBV	191120	214759	14.50%	1.891%
3	2.126	313	322	336	rVB	371129	510750	34.50%	4.496%
4	2.248	358	360	370	rVB10	14874	17988	1.21%	0.158%
5	2.531	438	448	457	rBV2	21823	36673	2.48%	0.323%
6	3.949	878	889	923	rBV	117454	460140	31.08%	4.051%
7	4.396	1009	1028	1052	rBV	244737	619798	41.86%	5.457%
8	5.093	1224	1245	1274	rBV2	596465	1480598	100.00%	13.035%
9	5.659	1407	1421	1440	rBV	444877	888899	60.04%	7.826%
10	5.949	1499	1511	1521	rBV	12949	29280	1.98%	0.258%
11	6.113	1548	1562	1585	rBV	336825	681163	46.01%	5.997%
12	7.026	1835	1846	1862	rBV	159432	288229	19.47%	2.537%
13	7.357	1936	1949	1966	rBV	640109	1126852	76.11%	9.920%
14	7.659	2033	2043	2065	rBV	92373	161178	10.89%	1.419%
15	8.132	2179	2190	2232	rBV	546962	1186699	80.15%	10.447%
16	8.891	2410	2426	2447	rBV	657383	1075953	72.67%	9.472%
17	10.257	2840	2851	2865	rBV	225121	354789	23.96%	3.123%
18	11.289	3161	3172	3186	rBV	601452	944856	63.82%	8.318%
19	11.666	3276	3289	3304	rBV	618941	983593	66.43%	8.659%
20	12.691	3599	3608	3616	rBV8	11131	16936	1.14%	0.149%
21	13.305	3792	3799	3807	rBV8	10806	17445	1.18%	0.154%
22	13.788	3941	3949	3957	rBV8	9404	16084	1.09%	0.142%


Sum of corrected areas: 11358893

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV122319\
Data File : VV014161.D
Acq On : 23 Dec 2019 16:23
Operator : SY/MD
Sample : VV1223WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK38

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

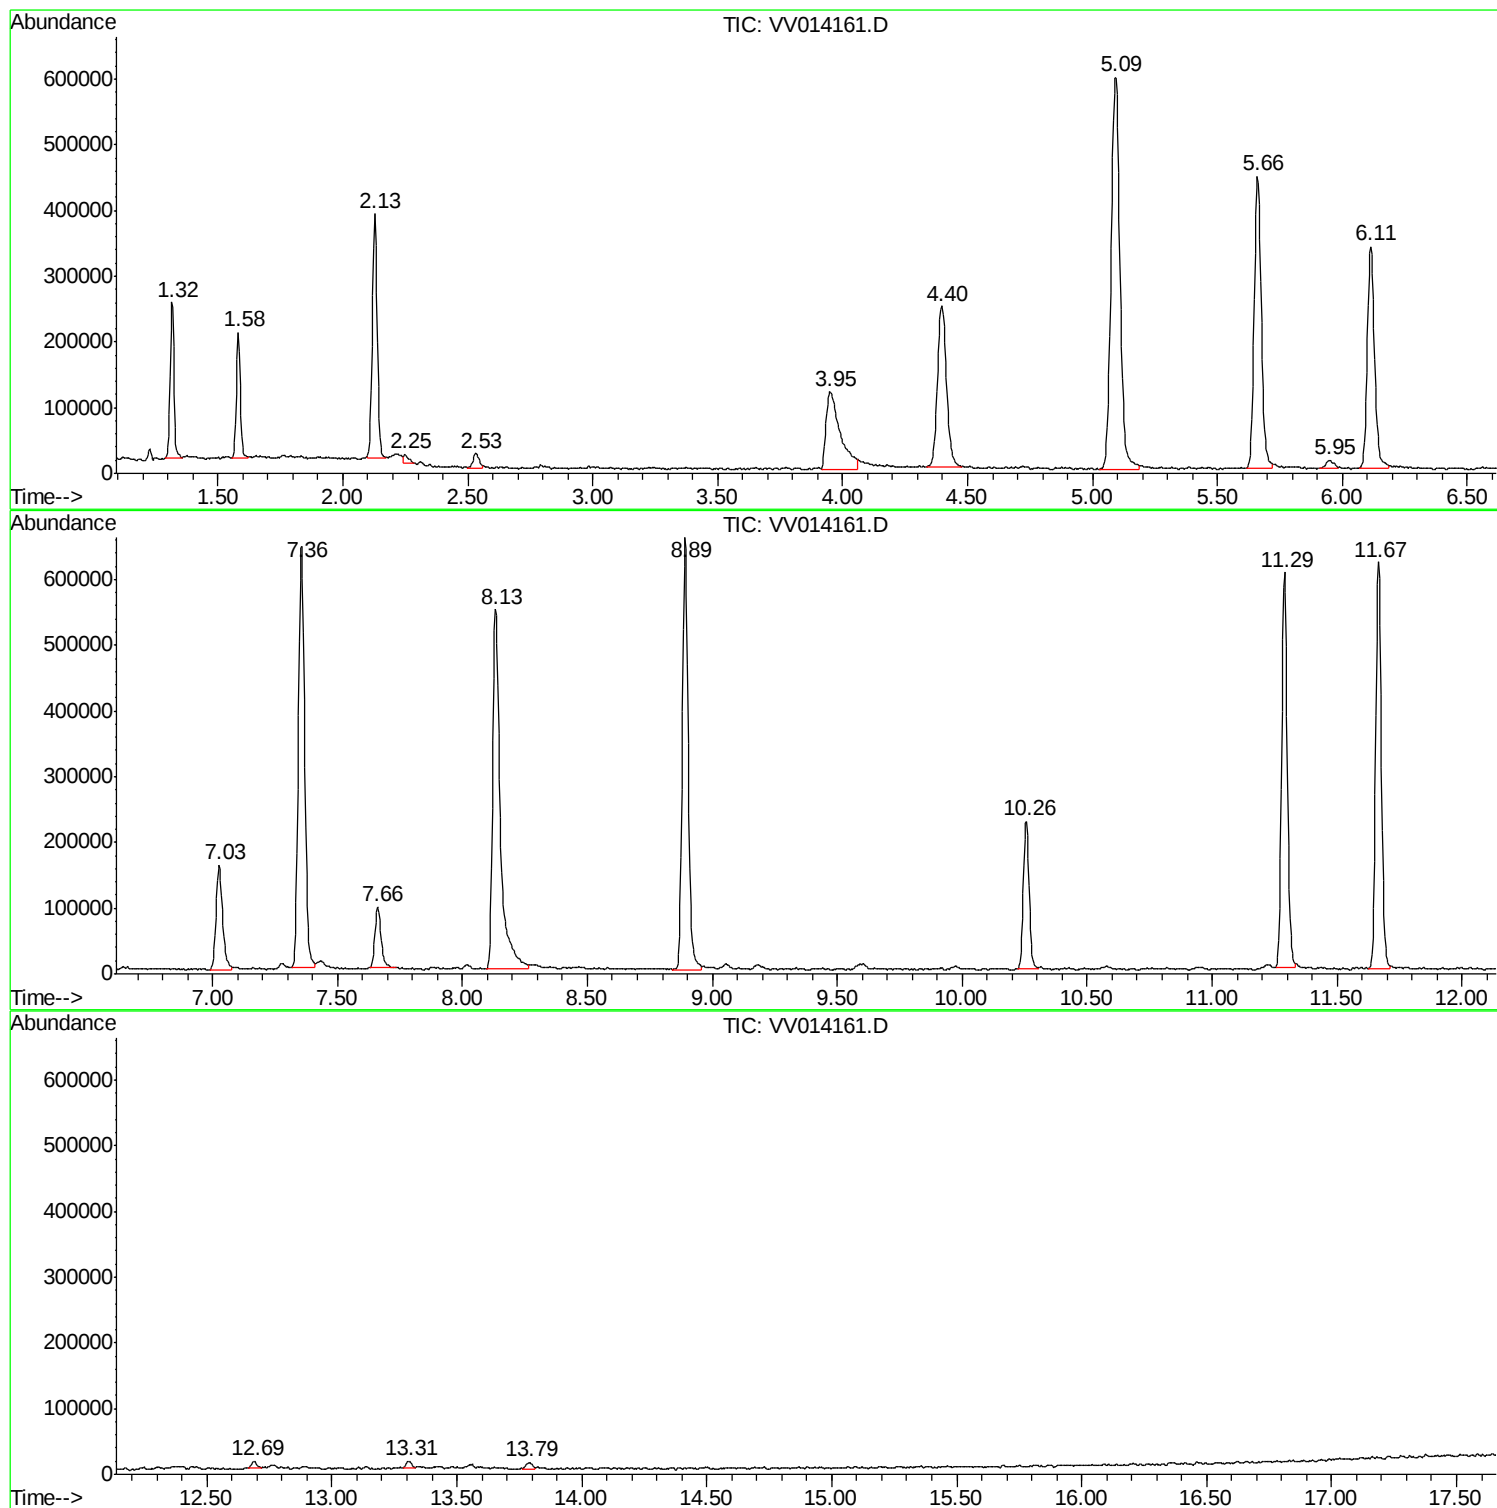

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV122319\
Data File : VV014161.D
Acq On : 23 Dec 2019 16:23
Operator : SY/MD
Sample : VV1223WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK38










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	1.62 ug/L	288229	1,4-Difluorobenzene	5.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	47
2		Thiophosgene	114	CCl2S	000463-71-8	38
3		1,3-Cyclohexadiene	80	C6H8	000592-57-4	32
4		.alpha.,.alpha.-Dichloromethyl m...	114	C2H4Cl2O	004885-02-3	25
5		3-Methylenecyclopentene	80	C6H8	000930-26-7	9

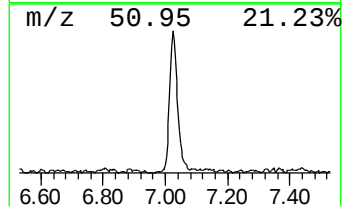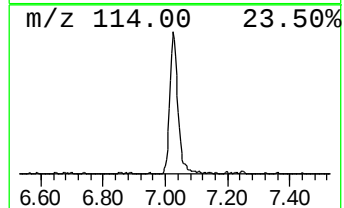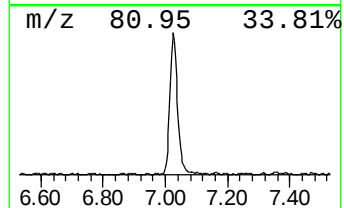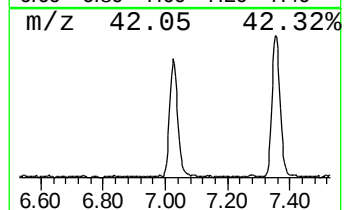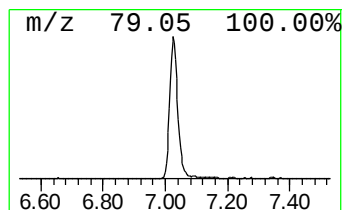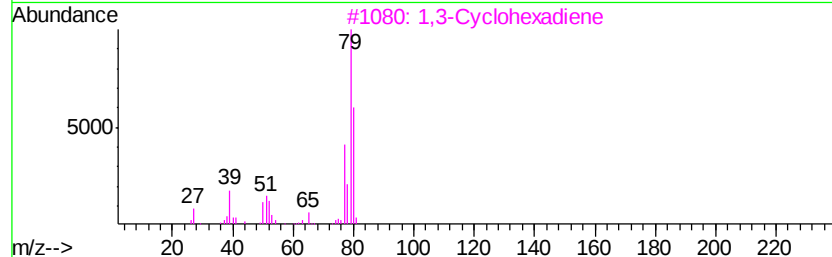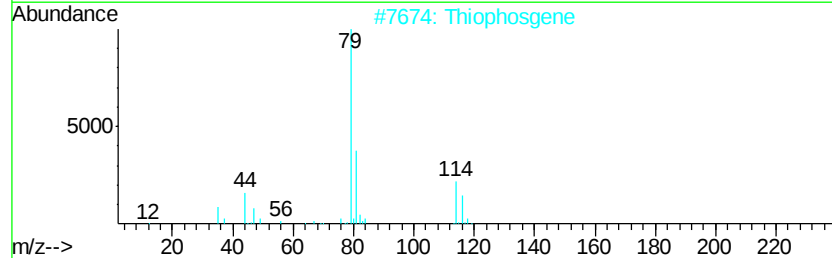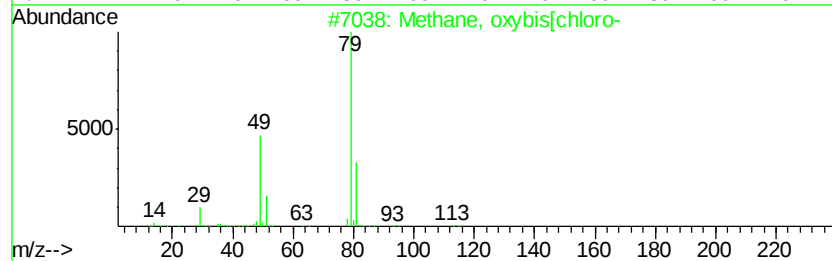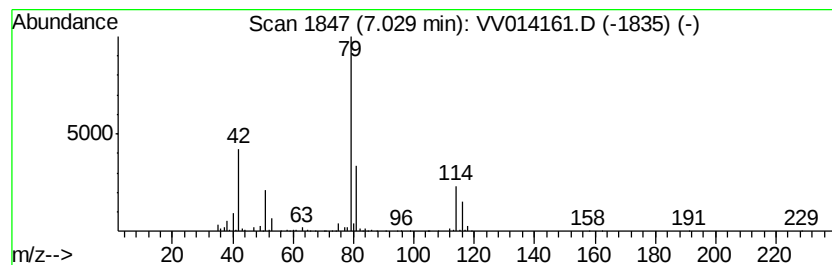

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122319\
Data File : VV014161.D
Acq On : 23 Dec 2019 16:23
Operator : SY/MD
Sample : VV1223WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK38

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.03	1.6	ug/L	288229	1	5.66	888899	5.0