

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122319\
 Data File : VV014165.D
 Acq On : 23 Dec 2019 18:19
 Operator : SY/MD
 Sample : K6404-13
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFE02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122319WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.226	37	42	47	rBV	18545	16629	1.19%	0.154%
2	1.316	62	70	84	rBV	221652	232461	16.63%	2.158%
3	1.582	145	153	163	rBV	177729	199541	14.28%	1.853%
4	2.129	313	323	336	rVB	328781	462521	33.09%	4.294%
5	3.949	877	889	912	rBV2	114876	390525	27.94%	3.626%
6	4.396	1013	1028	1052	rVB	236683	594564	42.54%	5.520%
7	5.094	1224	1245	1271	rBV2	567380	1397571	100.00%	12.975%
8	5.659	1406	1421	1440	rBV	411919	825121	59.04%	7.660%
9	6.113	1549	1562	1585	rBV	319891	657215	47.03%	6.102%
10	7.026	1834	1846	1863	rBV2	154954	283778	20.31%	2.635%
11	7.357	1936	1949	1964	rBV	647904	1129705	80.83%	10.488%
12	7.431	1964	1972	1983	rVB	23397	44543	3.19%	0.414%
13	7.659	2033	2043	2059	rBV	96575	163343	11.69%	1.516%
14	8.132	2180	2190	2217	rBV	542190	1161791	83.13%	10.786%
15	8.290	2233	2239	2247	rVB	10373	14575	1.04%	0.135%
16	8.891	2415	2426	2441	rBV	619416	995404	71.22%	9.241%
17	9.595	2636	2645	2658	rBV8	13218	25431	1.82%	0.236%
18	10.254	2839	2850	2869	rBV	217797	353704	25.31%	3.284%
19	11.289	3159	3172	3193	rBV	557746	872733	62.45%	8.102%
20	11.666	3276	3289	3305	rBV	587973	909953	65.11%	8.448%
21	12.389	3504	3514	3531	rBV9	23118	40137	2.87%	0.373%


Sum of corrected areas: 10771245

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV122319\
Data File : VV014165.D
Acq On : 23 Dec 2019 18:19
Operator : SY/MD
Sample : K6404-13
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFE02

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

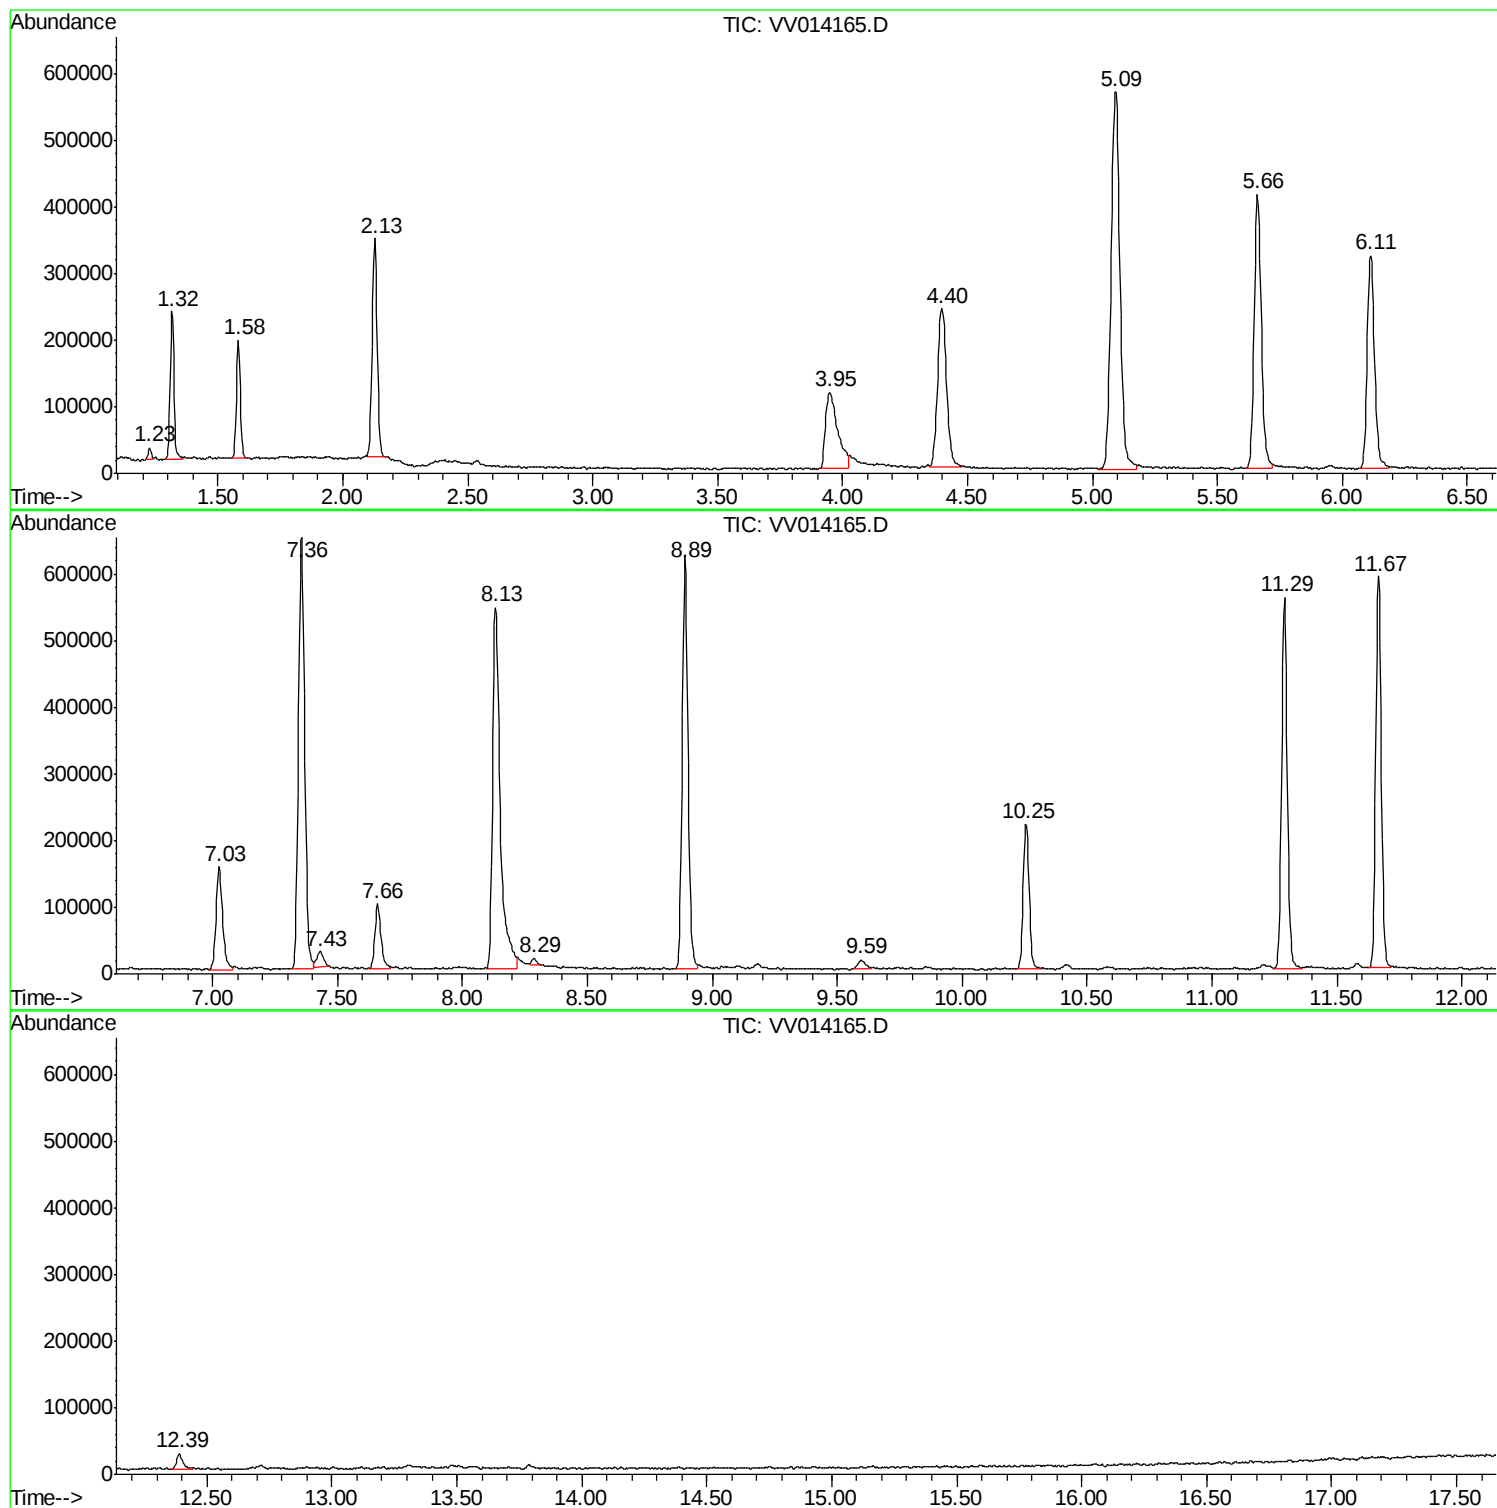

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV122319\
Data File : VV014165.D
Acq On : 23 Dec 2019 18:19
Operator : SY/MD
Sample : K6404-13
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFE02










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.03	1.72 ug/L	283778	1,4-Difluorobenzene	5.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	37
2		Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25
3		2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9
4		2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9
5		1,3-Cyclohexadiene	80	C6H8	000592-57-4	9

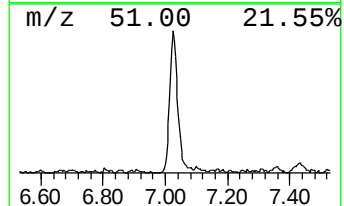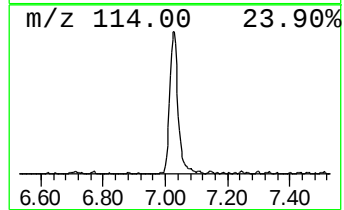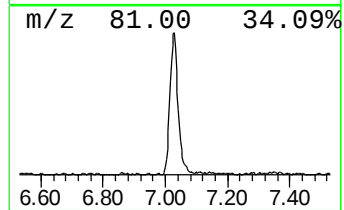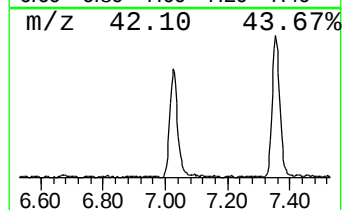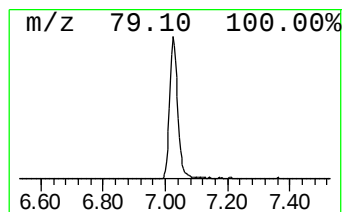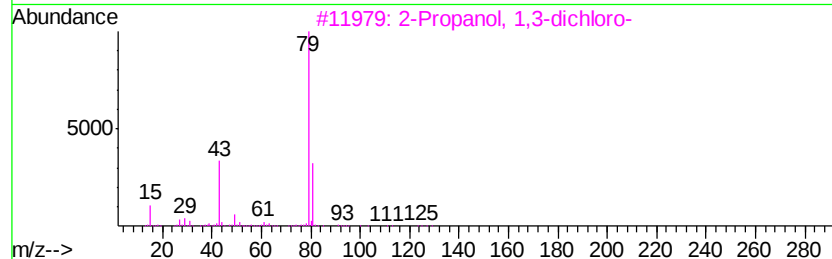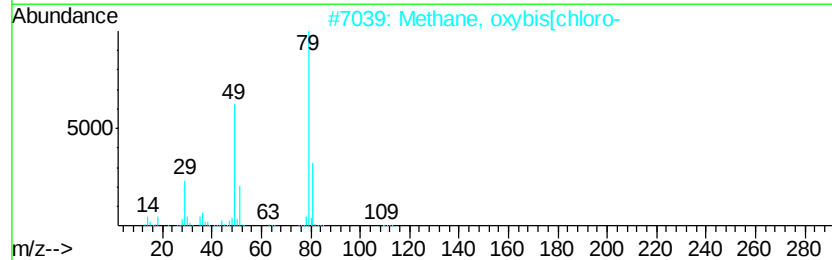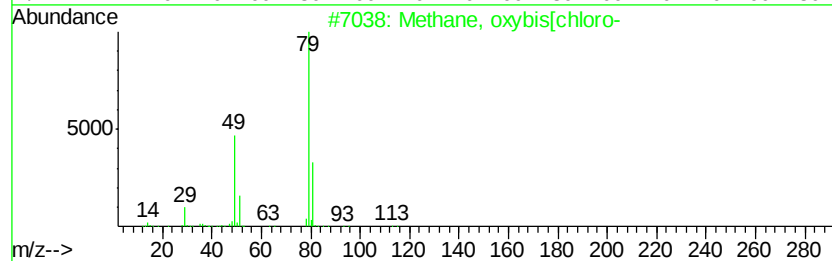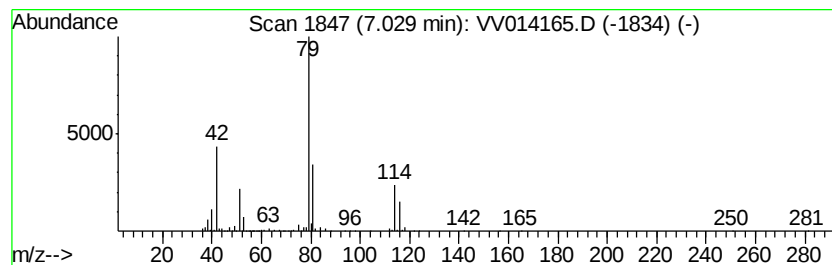

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122319\
Data File : VV014165.D
Acq On : 23 Dec 2019 18:19
Operator : SY/MD
Sample : K6404-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFE02

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122319WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.03	1.7	ug/L	283778	1	5.66	825121	5.0