


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122319\
 Data File : VV014153.D
 Acq On : 23 Dec 2019 08:59
 Operator : SY/MD
 Sample : BFB44
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB44

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122319WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Dec 23 10:55:37 2019

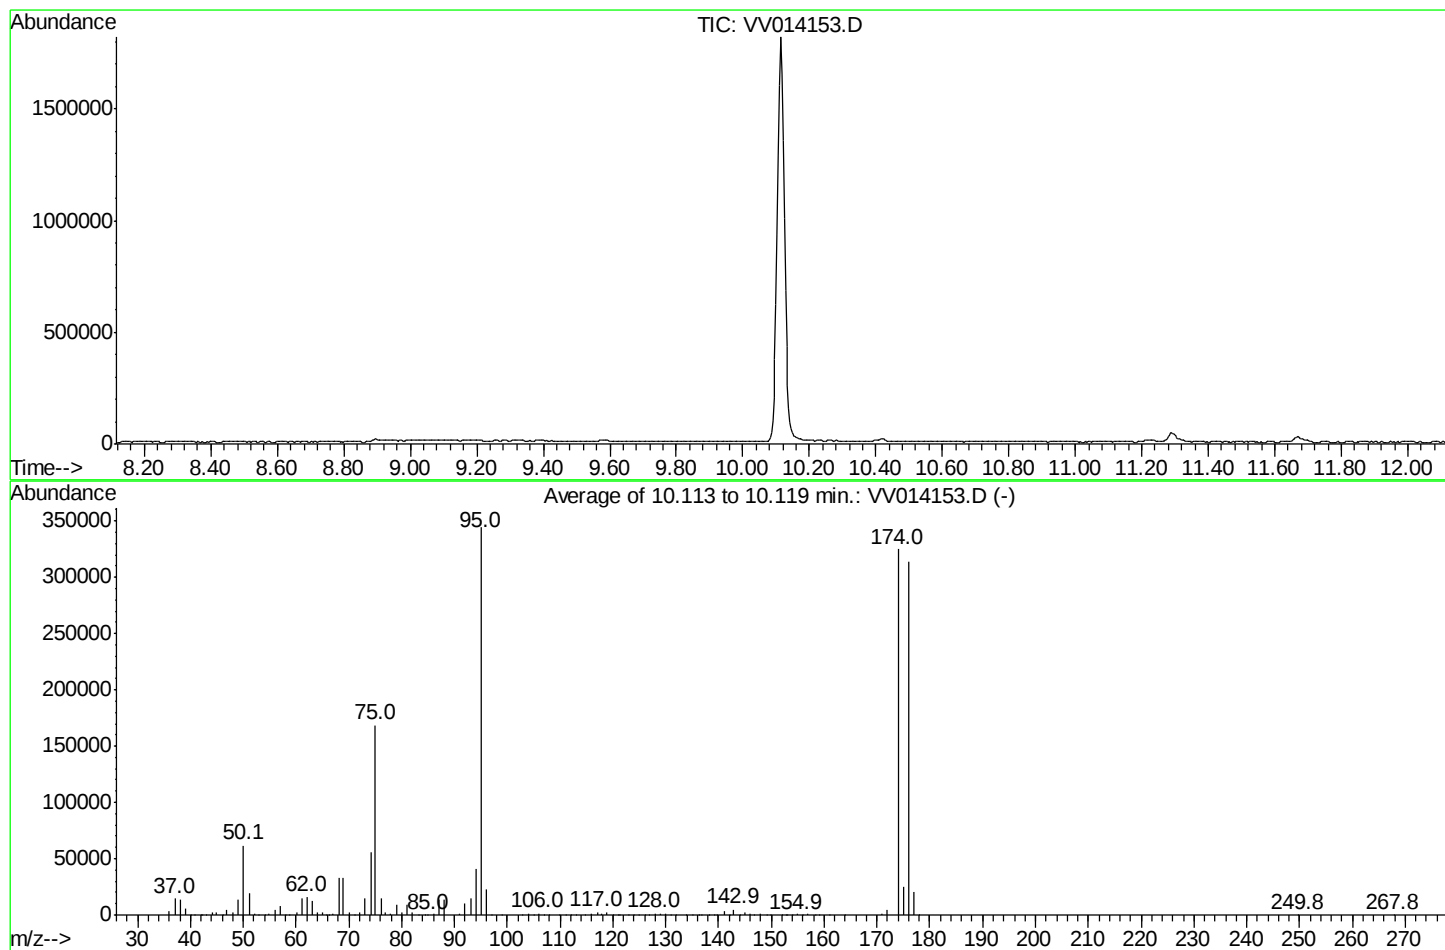

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2791

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	61538	PASS
75	95	30	80	49.0	168576	PASS
95	95	100	100	100.0	344320	PASS
96	95	5	9	6.6	22720	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.4	325034	PASS
175	174	5	9	7.7	25149	PASS
176	174	95	101	96.5	313664	PASS
177	176	5	9	6.4	19976	PASS

m/z	Abundance
36.00	6714.0
37.10	16255.0
38.10	14992.0
39.10	6861.0
40.10	1208.0
40.90	341.0
41.90	182.0
43.00	261.0
44.10	2442.0
45.00	2720.0
46.20	538.0
47.00	5273.0
48.00	1901.0
49.10	14505.0
50.10	63656.0
51.10	20304.0
52.10	932.0
53.10	431.0
54.00	259.0
55.00	915.0
56.00	4603.0
57.00	8451.0
58.00	275.0
58.80	265.0
60.10	3009.0
61.10	15977.0
62.00	17560.0
63.00	13294.0
64.10	2234.0
65.00	3057.0
65.90	383.0
66.30	275.0
66.90	1163.0
68.00	33088.0
69.00	34728.0
70.00	2780.0
71.00	346.0
72.00	1800.0
73.00	16456.0
74.10	57376.0
75.00	174976.0
76.10	15123.0
76.90	2281.0
77.90	1257.0
79.00	9444.0
80.00	2692.0
81.00	9772.0
81.90	2293.0
83.10	208.0
84.40	151.0
86.10	738.0
87.00	14579.0
88.00	12993.0
90.90	1133.0
92.00	10216.0
93.10	15376.0
94.00	42536.0
95.00	351488.0
96.00	23960.0
97.10	656.0
99.00	165.0
102.90	266.0
103.90	1524.0
105.00	661.0
105.90	1300.0
106.90	393.0
108.00	229.0
109.80	200.0
111.10	230.0
112.00	329.0
112.90	219.0
114.80	334.0
116.00	1466.0
117.00	2659.0
117.90	1222.0
118.90	2140.0
121.00	111.0
122.90	208.0
123.90	241.0
124.90	180.0
126.10	159.0
126.80	147.0
128.00	1275.0
128.90	661.0
130.00	1255.0
131.00	555.0
131.90	149.0
133.80	135.0
134.90	600.0
136.20	146.0
136.90	609.0
139.00	235.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

139.80	299.0
141.00	3307.0
142.10	508.0
142.90	5549.0
143.90	334.0
144.90	2096.0
145.90	545.0
146.80	359.0
147.90	932.0
149.10	339.0
149.80	362.0
151.90	153.0
152.70	249.0
153.80	130.0
154.90	1081.0
155.90	308.0
157.00	679.0
158.20	173.0
159.00	524.0
161.00	439.0
171.00	938.0
172.00	4576.0
174.00	326464.0
175.00	25336.0
176.00	315200.0
177.00	20208.0
178.00	587.0
249.80	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
36.00	6815.0
37.10	15395.0
38.10	15212.0
39.10	6410.0
40.10	1150.0
40.90	317.0
42.10	145.0
43.00	247.0
44.10	2420.0
45.10	2829.0
46.00	483.0
47.00	4794.0
48.00	1829.0
49.00	14393.0
50.10	63760.0
51.10	19848.0
52.10	995.0
53.00	378.0
54.10	234.0
55.00	879.0
56.00	4429.0
57.00	8092.0
58.00	376.0
58.70	203.0
60.00	2963.0
61.10	15157.0
62.10	16952.0
63.00	12988.0
64.10	2241.0
65.00	2880.0
65.90	396.0
67.00	978.0
68.00	33720.0
69.00	34616.0
70.00	2855.0
71.00	274.0
72.10	1772.0
73.00	15803.0
74.10	58120.0
75.00	174464.0
76.10	15090.0
77.00	2421.0
77.80	1407.0
79.00	9401.0
80.00	2676.0
81.00	9519.0
81.90	2088.0
83.10	232.0
84.40	128.0
85.00	107.0
86.00	763.0
87.00	14933.0
88.00	13910.0
90.90	1273.0
92.00	10676.0
93.10	15188.0
94.00	42008.0
95.00	356160.0
96.10	23744.0
97.10	616.0
98.90	117.0
102.90	253.0
104.00	1486.0
105.00	630.0
105.90	1380.0
106.90	338.0
108.00	115.0
109.80	191.0
109.90	187.0
111.10	295.0
112.00	390.0
112.90	270.0
114.80	354.0
116.00	1510.0
117.00	2430.0
118.00	1311.0
118.90	2136.0
121.20	104.0
123.00	242.0
123.90	284.0
124.90	167.0
126.10	175.0
126.90	187.0
127.90	1393.0
128.90	676.0
129.90	1197.0
130.90	599.0
131.90	189.0
134.90	594.0
136.10	167.0
136.80	577.0
138.10	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

139.10	180.0
139.80	276.0
141.00	3334.0
142.90	5296.0
143.90	272.0
145.00	1923.0
145.80	659.0
146.80	341.0
147.90	930.0
149.10	329.0
149.80	332.0
151.90	135.0
152.60	282.0
153.90	164.0
154.90	1018.0
155.90	279.0
156.90	705.0
159.00	576.0
160.90	515.0
164.00	124.0
171.00	928.0
172.00	4712.0
174.00	337344.0
175.00	26032.0
176.00	324672.0
177.00	20528.0
178.00	549.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
36.00	6536.0
37.10	13071.0
38.10	14251.0
39.10	5688.0
40.10	1040.0
40.80	261.0
42.20	136.0
43.00	259.0
44.10	2264.0
45.10	2640.0
45.90	552.0
47.00	3793.0
48.00	1636.0
49.00	12288.0
50.10	57200.0
51.10	17536.0
52.10	921.0
53.00	352.0
54.20	261.0
55.00	785.0
56.00	3900.0
57.00	7110.0
58.00	438.0
58.60	132.0
60.10	2681.0
61.10	13248.0
62.10	14860.0
63.00	11707.0
64.00	2134.0
65.00	2599.0
65.80	384.0
67.10	872.0
68.10	30784.0
69.00	30792.0
70.00	2416.0
70.90	201.0
72.10	1689.0
73.10	13638.0
74.10	52440.0
75.00	156288.0
76.10	13149.0
77.00	2060.0
77.80	1434.0
79.00	8510.0
80.00	2380.0
81.00	8702.0
82.00	1743.0
83.10	213.0
86.00	716.0
87.00	13203.0
88.00	13436.0
91.00	1253.0
92.00	9694.0
93.00	13413.0
94.00	37640.0
95.00	325312.0
96.10	20456.0
97.10	502.0
102.90	212.0
104.00	1334.0
105.00	526.0
106.00	1338.0
106.90	301.0
109.80	187.0
111.00	315.0
112.00	363.0
112.90	307.0
114.80	408.0
116.00	1237.0
117.00	2053.0
118.00	1181.0
118.90	1860.0
120.10	105.0
121.20	105.0
123.00	263.0
123.80	241.0
124.80	145.0
126.10	163.0
126.90	166.0
127.90	1296.0
129.00	680.0
129.80	1141.0
130.90	524.0
131.90	203.0
133.90	104.0
135.00	524.0
136.10	158.0
136.80	524.0
139.70	215.0
141.10	3176.0
142.10	447.0
142.90	4518.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

144.00	213.0
145.00	1609.0
145.80	646.0
146.80	277.0
147.90	814.0
149.10	251.0
149.80	320.0
151.90	127.0
152.60	230.0
153.00	166.0
153.90	200.0
154.90	907.0
156.00	244.0
156.90	664.0
158.30	183.0
159.00	485.0
160.90	528.0
164.00	140.0
171.00	788.0
172.00	4219.0
174.00	311296.0
175.00	24080.0
176.00	301120.0
177.00	19192.0
178.00	422.0
267.80	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
36.00	3536.0
37.00	535.0
38.00	1337.0
39.20	216.0
39.90	983.0
40.90	162.0
42.40	162.0
43.30	171.0
43.90	586.0
45.00	140.0
45.50	119.0
46.80	110.0
47.50	167.0
50.70	178.0
53.00	113.0
53.80	113.0
54.80	130.0
55.90	155.0
58.60	118.0
60.10	125.0
61.40	109.0
73.20	147.0
74.40	114.0
75.60	102.0
77.80	148.0
79.00	132.0
91.10	165.0
92.20	108.0
118.70	109.0
130.50	102.0
135.40	115.0
139.40	101.0
154.20	107.0
173.20	150.0
234.70	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44