

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122320\
 Data File : VV019818.D
 Acq On : 23 Dec 2020 17:46
 Operator : SY/MD
 Sample : L5173-16 100X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4S9

Quant Time: Dec 24 00:01:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 23 22:04:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.62	114	695722	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.86	117	650184	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.26	152	312460	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	220050	44.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.22%
7) Chloroethane-d5	1.57	69	189631	48.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.38%
11) 1,1-Dichloroethene-d2	2.11	63	329994	35.64	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.28%
21) 2-Butanone-d5	3.89	46	357131	131.70	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	131.70%#
24) Chloroform-d	4.35	84	420901	46.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.62%
26) 1,2-Dichloroethane-d4	5.04	65	292733	49.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.64%
32) Benzene-d6	5.05	84	841479	48.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.06%
36) 1,2-Dichloropropane-d6	6.07	67	268482	49.43	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.86%
41) Toluene-d8	7.32	98	724256	46.39	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.78%
43) trans-1,3-Dichloropropene-	7.63	79	122205	39.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.10%
47) 2-Hexanone-d5	8.09	63	214992	100.84	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.84%
57) 1,1,2,2-Tetrachloroethane-	10.22	84	330220	44.94	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.88%
64) 1,2-Dichlorobenzene-d4	11.63	152	265629	45.48	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.96%


Target Compounds					Ovalue
34) Trichloroethene	5.92	95	85282	16.990 ug/L	98
46) Tetrachloroethene	7.98	164	1299046	374.003 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122320\
Data File : VV019818.D
Acq On : 23 Dec 2020 17:46
Operator : SY/MD
Sample : L5173-16 100X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4S9

Quant Time: Dec 24 00:01:14 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 23 22:04:07 2020
Response via : Initial Calibration

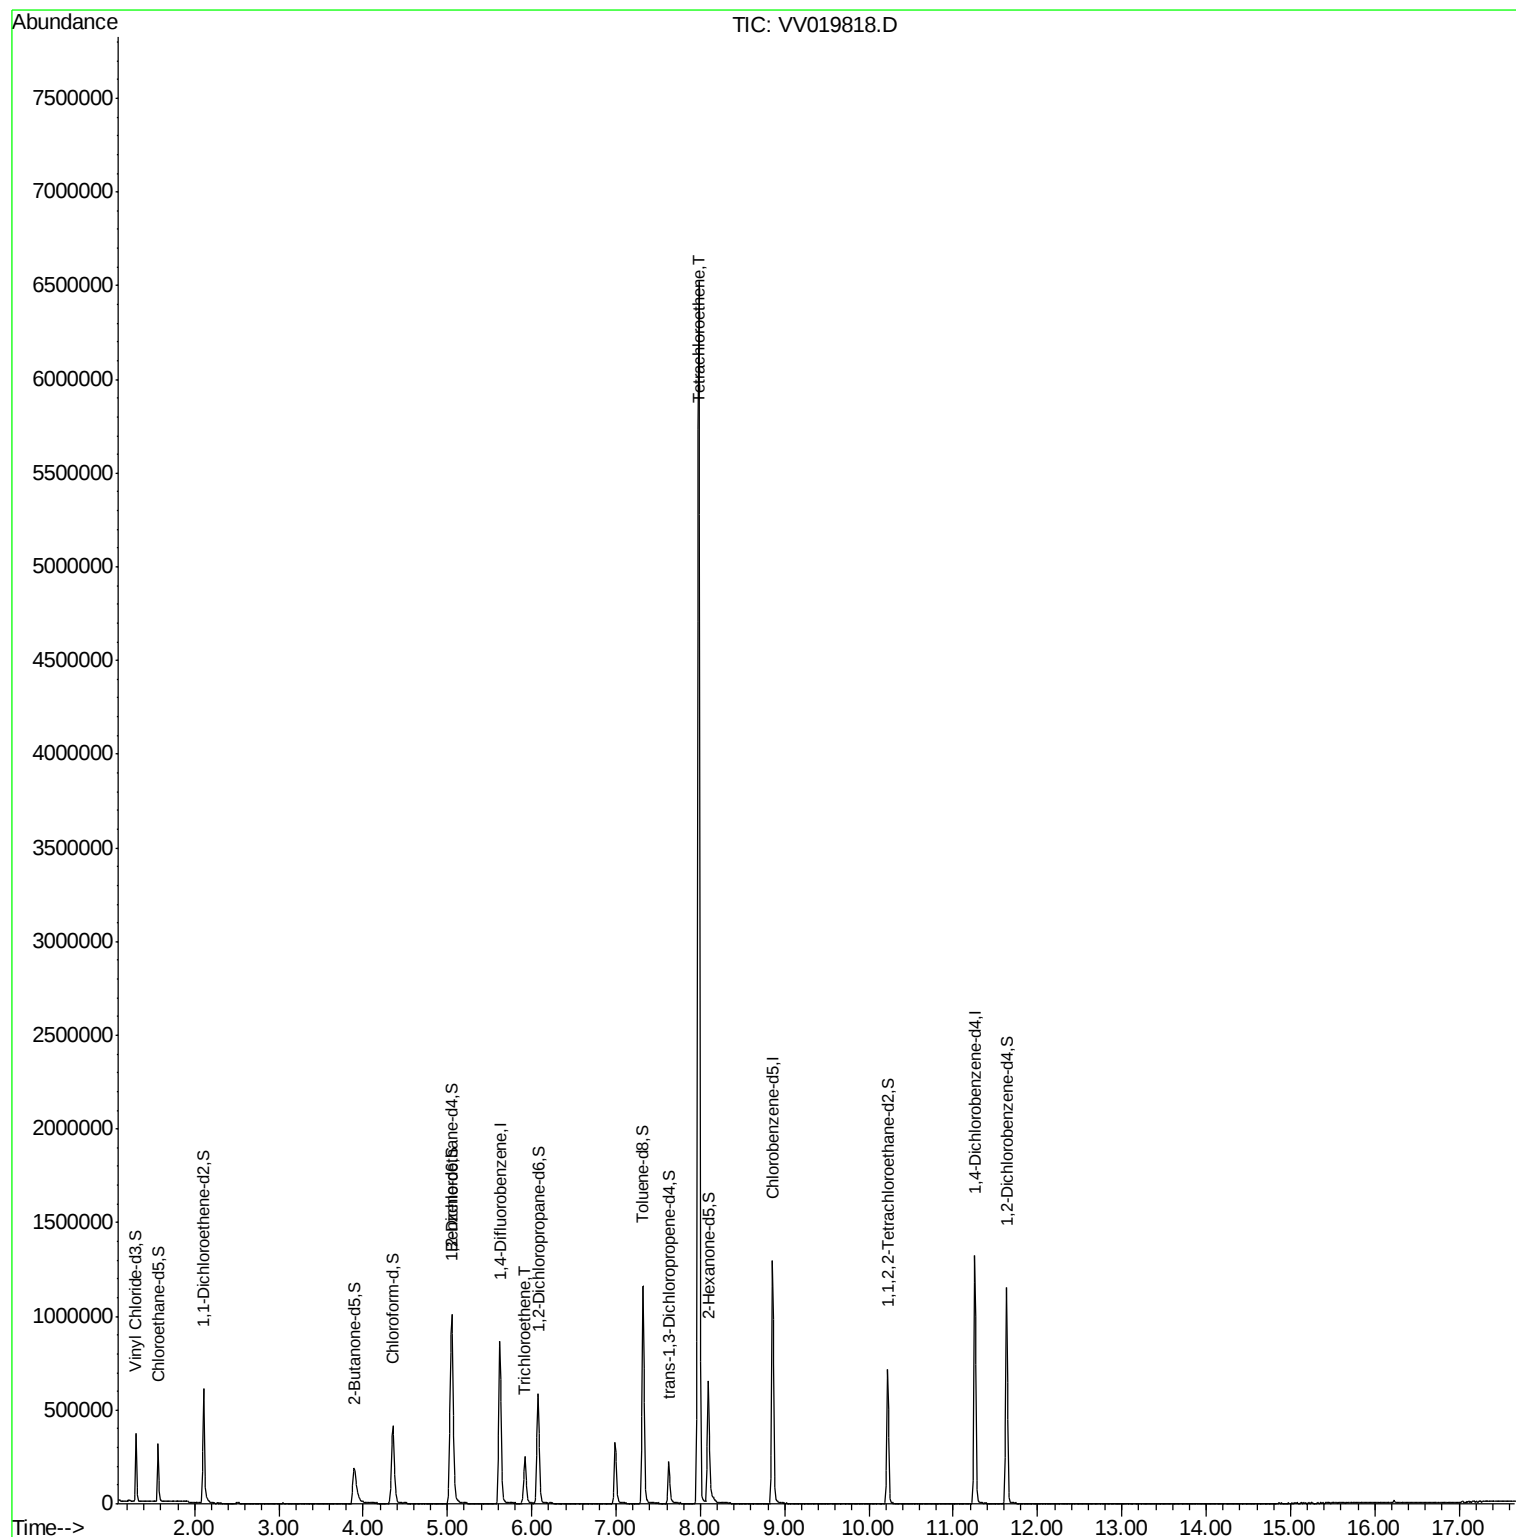

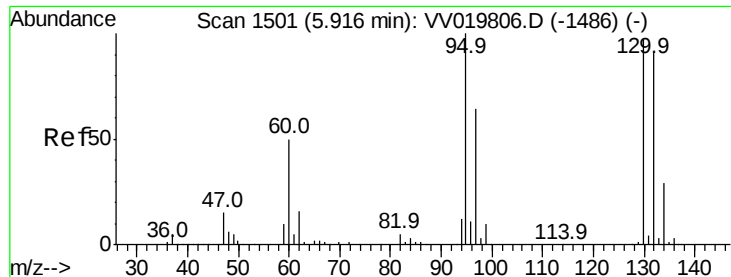

#34

Trichloroethene

Concen: 16.990 ug/L

RT: 5.92 min Scan# 1502

Delta R.T. 0.00 min

Lab File: VV019818.D

Acq: 23 Dec 2020 17:46

Instrument :

MSVOA_V

ClientSampleId :

BG4S9

Tot Ion: 95 Resp: 85282





Ion Ratio Lower Upper

95 100

97 65.5 44.4 82.4

132 95.0 64.3 119.3

130 97.0 67.8 125.8

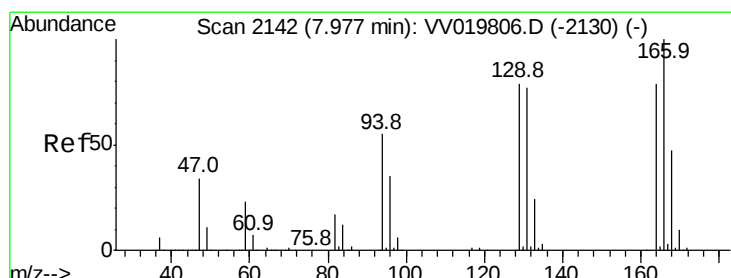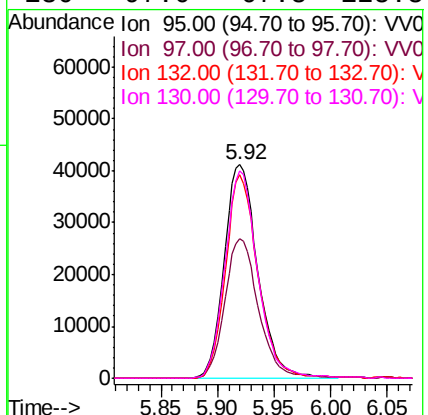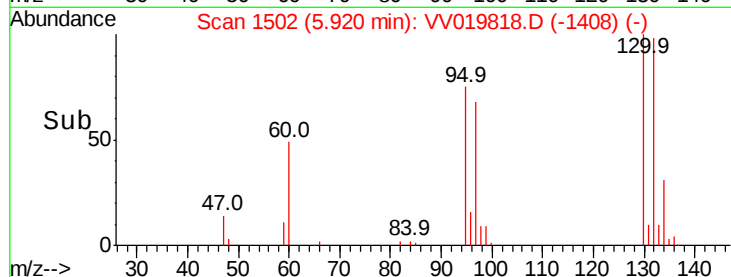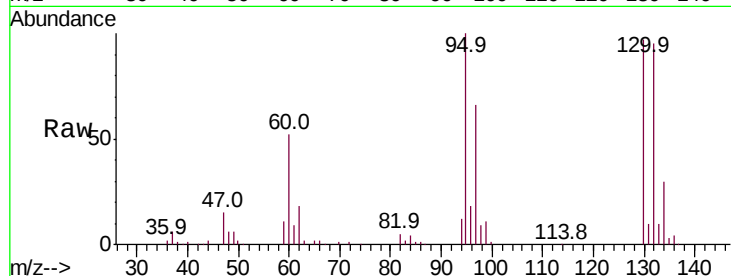

#46

Tetrachloroethene

Concen: 374.003 ug/L

RT: 7.98 min Scan# 2143

Delta R.T. 0.00 min

Lab File: VV019818.D

Acq: 23 Dec 2020 17:46

Tgt Ion:164 Resp: 1299046

Ion Ratio Lower Upper

164 100

129 102.9 70.6 131.0

131 98.7 68.0 126.4

166 127.7 86.9 161.5

