

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122320\
 Data File : VV019812.D
 Acq On : 23 Dec 2020 15:21
 Operator : SY/MD
 Sample : L5206-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4P3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	84	rVB	371119	367424	14.88%	1.977%
2	1.569	142	149	161	rVB	290418	327549	13.27%	1.762%
3	2.110	307	317	336	rBV	581307	881333	35.70%	4.741%
4	2.579	461	463	468	rBV3	644	386	0.02%	0.002%
5	2.865	550	552	555	rVB4	711	361	0.01%	0.002%
6	3.048	599	609	616	rBV5	3428	6166	0.25%	0.033%
7	3.219	659	662	666	rBV5	530	386	0.02%	0.002%
8	3.312	687	691	696	rVB3	511	528	0.02%	0.003%
9	3.364	701	707	708	rBV3	949	589	0.02%	0.003%
10	3.389	712	715	716	rBV2	305	162	0.01%	0.001%
11	3.405	716	720	721	rBV	741	472	0.02%	0.003%
12	3.482	738	744	746	rBV4	842	989	0.04%	0.005%
13	3.518	754	755	757	rBV	343	92	0.00%	0.000%
14	3.527	757	758	760	rVB	486	120	0.00%	0.001%
15	3.540	760	762	764	rBV2	661	318	0.01%	0.002%
16	3.576	771	773	775	rBV2	347	168	0.01%	0.001%
17	3.585	775	776	778	rVB	315	93	0.00%	0.001%
18	3.627	785	789	791	rBV3	766	599	0.02%	0.003%
19	3.672	799	803	805	rBV4	974	853	0.03%	0.005%
20	3.852	855	859	861	rBV3	1322	969	0.04%	0.005%
21	3.891	861	871	910	rVV2	165846	498497	20.19%	2.682%
22	4.354	1001	1015	1037	rBV	389932	944508	38.26%	5.081%
23	4.907	1185	1187	1189	rBV3	535	362	0.01%	0.002%
24	4.981	1208	1210	1214	rBV4	898	616	0.02%	0.003%
25	5.052	1214	1232	1261	rBV2	963616	2468639	100.00%	13.280%
26	5.399	1337	1340	1342	rBV4	1051	778	0.03%	0.004%
27	5.492	1366	1369	1371	rBV3	1203	685	0.03%	0.004%
28	5.621	1396	1409	1437	rBV	758618	1525252	61.79%	8.205%
29	5.910	1489	1499	1518	rVB3	45496	94188	3.82%	0.507%
30	6.074	1537	1550	1581	rBV	554297	1123782	45.52%	6.045%
31	6.508	1684	1685	1686	rBV	695	238	0.01%	0.001%
32	6.781	1768	1770	1773	rBV3	535	318	0.01%	0.002%
33	6.823	1780	1783	1785	rBV4	745	551	0.02%	0.003%
34	6.852	1791	1792	1794	rBV	467	180	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122320\
 Data File : VV019812.D
 Acq On : 23 Dec 2020 15:21
 Operator : SY/MD
 Sample : L5206-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4P3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.868	1794	1797	1798	rBV	758	373	0.02%	0.002%
36	6.920	1810	1813	1816	rBV3	725	368	0.01%	0.002%
37	6.942	1816	1820	1822	rBV4	802	561	0.02%	0.003%
38	6.990	1823	1835	1856	rBV	309483	564326	22.86%	3.036%
39	7.322	1925	1938	1972	rBV	1121845	1929531	78.16%	10.380%
40	7.627	2021	2033	2056	rBV	214168	378609	15.34%	2.037%
41	7.936	2125	2129	2130	rBV3	1581	857	0.03%	0.005%
42	8.051	2163	2165	2167	rBV2	677	363	0.01%	0.002%
43	8.093	2167	2178	2213	rBV2	539747	1067286	43.23%	5.741%
44	8.698	2363	2366	2369	rBV4	788	629	0.03%	0.003%
45	8.746	2379	2381	2385	rBV4	552	356	0.01%	0.002%
46	8.794	2394	2396	2400	rVB3	715	444	0.02%	0.002%
47	8.858	2403	2416	2439	rBV	1141272	1846920	74.82%	9.935%
48	9.244	2534	2536	2537	rBV2	451	184	0.01%	0.001%
49	9.312	2555	2557	2558	rBV2	516	201	0.01%	0.001%
50	9.338	2563	2565	2569	rBV2	914	634	0.03%	0.003%
51	9.373	2575	2576	2579	rVB3	700	306	0.01%	0.002%
52	9.399	2582	2584	2586	rVB2	604	201	0.01%	0.001%
53	9.412	2586	2588	2590	rBV2	626	257	0.01%	0.001%
54	9.450	2598	2600	2601	rBV2	741	312	0.01%	0.002%
55	9.476	2606	2608	2610	rVB	531	200	0.01%	0.001%
56	9.492	2610	2613	2615	rBV3	738	412	0.02%	0.002%
57	9.511	2617	2619	2621	rBV2	690	331	0.01%	0.002%
58	9.550	2626	2631	2638	rVV7	1551	1805	0.07%	0.010%
59	9.637	2656	2658	2665	rVB4	1042	931	0.04%	0.005%
60	9.666	2665	2667	2669	rBV2	621	403	0.02%	0.002%
61	9.717	2681	2683	2684	rBV2	695	313	0.01%	0.002%
62	9.791	2703	2706	2709	rBV3	762	463	0.02%	0.002%
63	9.829	2709	2718	2722	rBV7	1767	2798	0.11%	0.015%
64	10.048	2783	2786	2790	rBV2	768	502	0.02%	0.003%
65	10.161	2819	2821	2823	rBV3	470	282	0.01%	0.002%
66	10.222	2828	2840	2857	rVV	615052	978845	39.65%	5.266%
67	10.479	2917	2920	2923	rBV3	614	466	0.02%	0.003%
68	10.547	2939	2941	2943	rBV2	669	372	0.02%	0.002%
69	10.756	3003	3006	3007	rBV3	354	175	0.01%	0.001%
70	10.817	3021	3025	3026	rBV3	660	389	0.02%	0.002%
71	10.855	3033	3037	3038	rBV3	440	271	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122320\
 Data File : VV019812.D
 Acq On : 23 Dec 2020 15:21
 Operator : SY/MD
 Sample : L5206-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4P3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.993	3077	3080	3081	rBV2	816	378	0.02%	0.002%
73	11.257	3150	3162	3194	rBV	1185976	1826481	73.99%	9.825%
74	11.633	3266	3279	3297	rBV	1104280	1720588	69.70%	9.256%
75	11.907	3362	3364	3366	rBV3	929	579	0.02%	0.003%
76	11.952	3376	3378	3384	rVB4	1354	1192	0.05%	0.006%
77	12.064	3411	3413	3418	rBV3	855	868	0.04%	0.005%
78	12.254	3467	3472	3474	rBV3	1774	1544	0.06%	0.008%
79	12.357	3499	3504	3506	rBV3	3524	3459	0.14%	0.019%
80	12.800	3640	3642	3646	rVB4	980	534	0.02%	0.003%
81	12.839	3651	3654	3656	rBV4	659	487	0.02%	0.003%
82	13.003	3703	3705	3710	rBV3	887	807	0.03%	0.004%
83	13.141	3745	3748	3749	rBV2	1176	766	0.03%	0.004%
84	13.614	3892	3895	3897	rBV3	745	348	0.01%	0.002%
85	13.669	3910	3912	3913	rBV3	675	250	0.01%	0.001%
86	13.833	3962	3963	3967	rBV4	918	476	0.02%	0.003%
87	14.267	4094	4098	4099	rBV2	1080	769	0.03%	0.004%


Sum of corrected areas: 18589353

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122320\
Data File : VV019812.D
Acq On : 23 Dec 2020 15:21
Operator : SY/MD
Sample : L5206-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4P3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

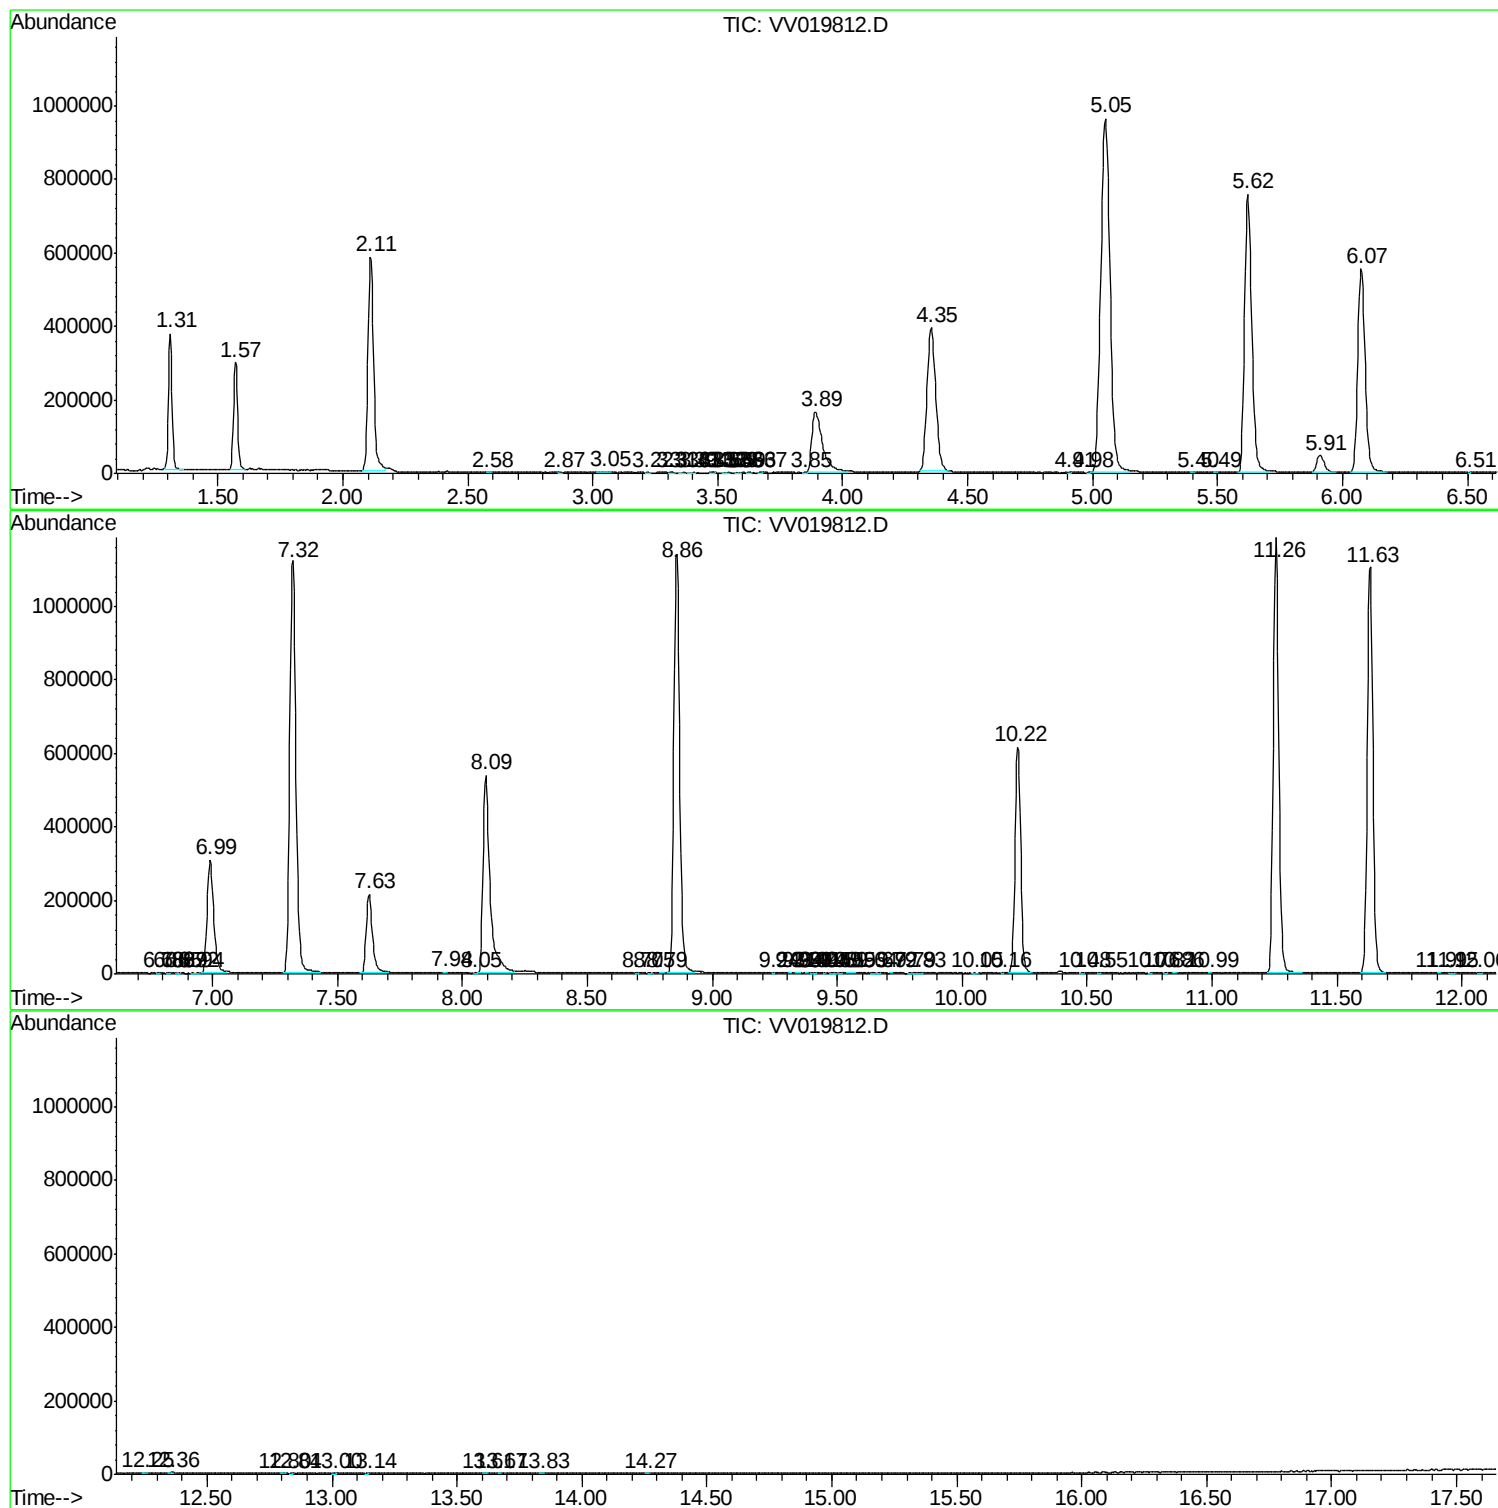

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV122320\
Data File : VV019812.D
Acq On : 23 Dec 2020 15:21
Operator : SY/MD
Sample : L5206-03
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4P3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV122320\
Data File : VV019812.D
Acq On : 23 Dec 2020 15:21
Operator : SY/MD
Sample : L5206-03
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4P3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc