


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV122320\
 Data File : VV019805.D
 Acq On : 23 Dec 2020 09:00
 Operator : SY/MD
 Sample : BFB72
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB72

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 23 22:04:07 2020

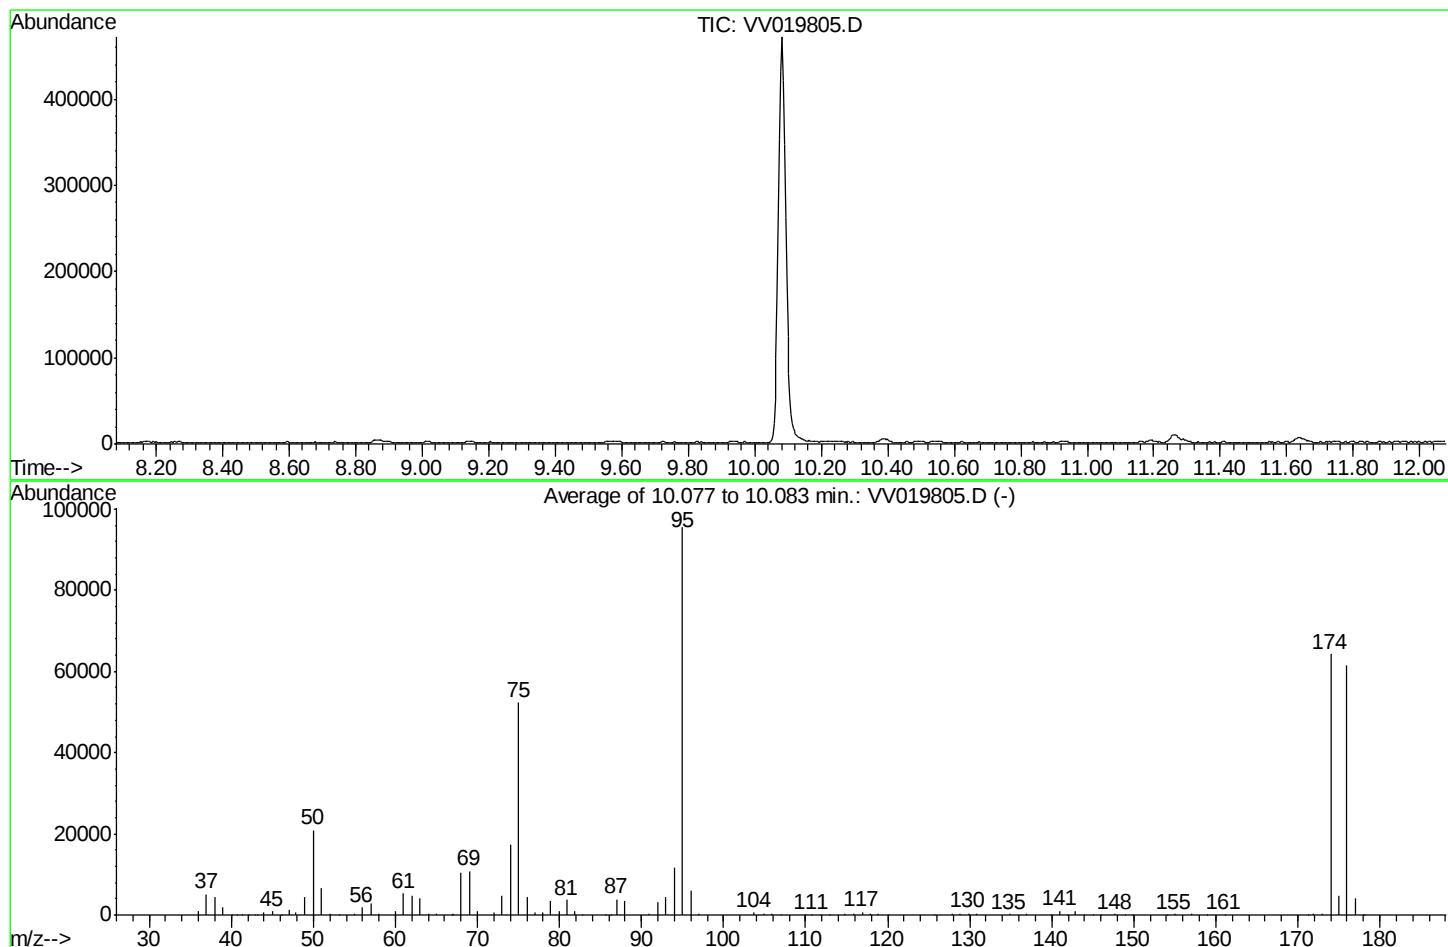

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	20893	PASS
75	95	30	80	54.8	52341	PASS
95	95	100	100	100.0	95530	PASS
96	95	5	9	6.4	6145	PASS
173	174	0.00	2	0.3	174	PASS
174	95	50	120	67.2	64208	PASS
175	174	5	9	7.3	4707	PASS
176	174	95	101	95.6	61378	PASS
177	176	5	9	6.7	4141	PASS

m/z	Abundance
36.00	1031.0
37.00	5022.0
38.00	4172.0
39.00	1779.0
40.00	460.0
40.70	105.0
42.00	107.0
42.80	131.0
43.90	1357.0
45.00	875.0
46.10	156.0
47.00	1247.0
47.90	573.0
49.00	4244.0
50.00	20328.0
51.00	6437.0
52.00	393.0
53.10	135.0
55.00	344.0
55.90	1661.0
57.00	2767.0
57.90	175.0
59.90	910.0
61.00	5076.0
62.00	4487.0
63.00	3900.0
64.00	369.0
65.00	367.0
67.10	271.0
68.00	10251.0
69.00	9992.0
70.00	820.0
72.00	521.0
73.00	4467.0
74.00	16520.0
75.00	49896.0
76.00	4097.0
76.90	716.0
78.00	460.0
78.90	3390.0
79.90	958.0
80.90	3491.0
81.90	859.0
82.80	114.0
85.70	165.0
87.00	3899.0
88.00	3409.0
91.00	450.0
92.00	2946.0
93.00	4330.0
94.00	11382.0
95.00	90256.0
96.00	5789.0
97.00	173.0
103.80	473.0
104.80	236.0
105.90	390.0
107.00	138.0
110.80	165.0
111.80	126.0
112.90	157.0
114.80	269.0
115.80	363.0
116.90	681.0
117.80	456.0
118.70	341.0
127.80	316.0
128.80	238.0
129.90	440.0
130.80	157.0
134.90	228.0
136.80	162.0
141.00	1069.0
142.90	1102.0
143.90	123.0
145.10	110.0
145.90	104.0
147.70	167.0
148.80	139.0
155.00	279.0
157.00	177.0
158.80	102.0
171.80	309.0
172.90	523.0
174.00	58744.0
175.00	4548.0
176.00	56176.0
177.00	3928.0
177.90	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.00	1014.0
37.00	5404.0
38.00	4592.0
39.00	2061.0
40.00	474.0
41.20	107.0
42.80	110.0
43.90	1467.0
45.00	932.0
46.10	164.0
47.00	1236.0
47.90	647.0
49.00	4622.0
50.00	21616.0
51.00	6780.0
52.00	415.0
53.10	143.0
55.00	414.0
56.00	1925.0
57.00	2911.0
57.90	195.0
60.00	1060.0
61.00	5520.0
62.00	4998.0
63.00	4167.0
64.00	405.0
65.00	320.0
67.10	253.0
68.00	10874.0
69.00	11289.0
70.00	1037.0
72.00	609.0
73.00	4787.0
74.00	18088.0
75.00	54336.0
76.00	4463.0
76.90	750.0
77.90	520.0
78.90	3532.0
79.90	969.0
80.90	3831.0
81.90	965.0
85.60	102.0
87.00	3965.0
87.90	3645.0
90.90	440.0
92.00	3222.0
93.00	4499.0
94.00	12001.0
95.00	98480.0
96.00	6315.0
97.00	193.0
103.70	529.0
104.90	206.0
105.90	444.0
106.90	168.0
109.90	112.0
110.80	154.0
111.80	157.0
113.00	177.0
114.80	244.0
115.90	358.0
116.90	772.0
117.90	456.0
118.80	435.0
127.90	338.0
128.80	319.0
129.90	395.0
130.80	226.0
134.90	279.0
136.90	181.0
139.90	102.0
141.00	1091.0
141.90	120.0
142.90	1007.0
143.90	132.0
145.10	125.0
147.70	255.0
148.90	134.0
154.10	107.0
155.00	296.0
157.00	224.0
158.80	158.0
161.10	106.0
171.20	123.0
171.90	366.0
174.00	66208.0
175.00	4850.0
176.00	63432.0
177.00	4240.0
177.90	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
36.00	985.0
37.00	5229.0
38.00	4705.0
39.00	2162.0
40.00	461.0
41.30	108.0
42.90	109.0
43.10	110.0
43.90	1415.0
45.00	970.0
46.00	166.0
47.00	1211.0
47.90	633.0
49.00	4585.0
50.00	20736.0
51.00	6464.0
52.00	356.0
53.10	102.0
54.90	396.0
56.00	1956.0
57.00	2913.0
58.00	166.0
60.00	1040.0
61.00	5420.0
62.00	5138.0
63.00	4132.0
64.00	412.0
64.90	272.0
66.80	292.0
68.00	10475.0
69.00	11191.0
70.00	1093.0
71.90	616.0
73.00	4677.0
74.00	17720.0
75.00	52792.0
76.00	4349.0
77.00	634.0
78.00	513.0
78.90	3349.0
79.90	864.0
80.90	3740.0
81.90	955.0
86.20	225.0
87.00	3730.0
87.90	3758.0
90.90	385.0
91.90	3022.0
93.00	4121.0
94.00	11601.0
95.00	97856.0
96.00	6331.0
97.00	185.0
103.70	524.0
105.00	189.0
105.80	497.0
106.90	157.0
109.90	112.0
110.60	147.0
111.80	141.0
113.00	149.0
114.80	135.0
115.90	326.0
116.90	796.0
117.90	358.0
118.80	541.0
120.10	107.0
125.70	129.0
127.90	314.0
128.90	314.0
129.90	279.0
130.80	231.0
134.80	290.0
136.90	176.0
139.80	145.0
141.00	988.0
141.90	142.0
142.90	928.0
145.00	141.0
147.70	292.0
149.00	133.0
149.90	122.0
155.00	255.0
157.00	244.0
158.90	172.0
161.10	114.0
172.00	440.0
174.00	67672.0
175.00	4723.0
176.00	64528.0
177.00	4256.0
178.10	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

Scan 2784 (10.042 min): VV019805.D
BFB72

m/z	Abundance
36.90	104.0
37.50	119.0
38.80	151.0
40.00	440.0
42.80	114.0
43.90	896.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72