

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
 Data File : VV029778.D
 Acq On : 23 Dec 2022 10:19
 Operator : SY/MD
 Sample : VV1223WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK315

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	246963	243677	14.71%	1.869%
2	1.561	154	162	174	rBV	213061	237522	14.34%	1.822%
3	2.104	320	331	345	rBV	399746	572937	34.59%	4.395%
4	2.285	383	387	389	rBV2	817	762	0.05%	0.006%
5	2.339	401	404	406	rBV	292	210	0.01%	0.002%
6	2.368	411	413	414	rBV	328	181	0.01%	0.001%
7	2.503	445	455	464	rBV2	4086	6428	0.39%	0.049%
8	2.664	503	505	509	rVB2	267	189	0.01%	0.001%
9	2.686	509	512	517	rBV2	251	229	0.01%	0.002%
10	2.712	517	520	529	rVB3	420	477	0.03%	0.004%
11	2.754	529	533	536	rBV3	392	344	0.02%	0.003%
12	3.101	637	641	644	rVV2	294	240	0.01%	0.002%
13	3.133	647	651	654	rVB2	425	260	0.02%	0.002%
14	3.285	694	698	701	rBV2	283	202	0.01%	0.002%
15	3.352	717	719	723	rVB2	353	222	0.01%	0.002%
16	3.436	743	745	750	rVV2	340	267	0.02%	0.002%
17	3.468	753	755	763	rVB2	294	251	0.02%	0.002%
18	3.600	792	796	803	rVB2	385	469	0.03%	0.004%
19	3.635	803	807	809	rBV2	345	231	0.01%	0.002%
20	3.870	870	880	925	rBV	119657	341794	20.64%	2.622%
21	4.336	1008	1025	1056	rBV	246410	628668	37.96%	4.822%
22	4.635	1114	1118	1120	rVB4	406	235	0.01%	0.002%
23	4.706	1137	1140	1142	rBV2	355	225	0.01%	0.002%
24	4.915	1202	1205	1211	rVB2	211	229	0.01%	0.002%
25	4.950	1211	1216	1217	rBV2	256	181	0.01%	0.001%
26	5.037	1226	1243	1300	rVV2	626717	1656158	100.00%	12.704%
27	5.609	1405	1421	1448	rBV	509116	1045474	63.13%	8.019%
28	5.828	1486	1489	1491	rVB3	355	216	0.01%	0.002%
29	5.902	1501	1512	1528	rVB5	4913	10670	0.64%	0.082%
30	6.059	1545	1561	1596	rBV	351614	734469	44.35%	5.634%
31	6.384	1657	1662	1667	rVB	184	198	0.01%	0.002%
32	6.474	1687	1690	1694	rVB2	330	265	0.02%	0.002%
33	6.558	1711	1716	1718	rBV2	202	209	0.01%	0.002%
34	6.628	1727	1738	1745	rBV7	1615	3731	0.23%	0.029%
35	6.783	1783	1786	1793	rBV2	212	240	0.01%	0.002%
36	6.879	1813	1816	1818	rBV	324	217	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
 Data File : VV029778.D
 Acq On : 23 Dec 2022 10:19
 Operator : SY/MD
 Sample : VV1223WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK315

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.979	1834	1847	1880	rBV	178979	338141	20.42%	2.594%
38	7.153	1893	1901	1902	rBV5	1180	1441	0.09%	0.011%
39	7.230	1922	1925	1929	rBV3	440	350	0.02%	0.003%
40	7.307	1933	1949	1987	rBV	763633	1348925	81.45%	10.347%
41	7.612	2033	2044	2072	rBV	124921	220777	13.33%	1.694%
42	7.808	2102	2105	2110	rVB3	431	311	0.02%	0.002%
43	7.837	2110	2114	2118	rVB3	789	562	0.03%	0.004%
44	7.866	2118	2123	2124	rBV2	294	218	0.01%	0.002%
45	7.915	2134	2138	2139	rBV	370	210	0.01%	0.002%
46	8.037	2173	2176	2180	rVB2	414	324	0.02%	0.002%
47	8.082	2180	2190	2226	rBV	440591	811121	48.98%	6.222%
48	8.381	2280	2283	2286	rBV2	539	277	0.02%	0.002%
49	8.416	2292	2294	2301	rVB5	455	424	0.03%	0.003%
50	8.477	2311	2313	2316	rVB2	368	208	0.01%	0.002%
51	8.506	2316	2322	2325	rBV4	373	326	0.02%	0.003%
52	8.558	2336	2338	2344	rVB2	460	366	0.02%	0.003%
53	8.615	2352	2356	2361	rBV2	311	368	0.02%	0.003%
54	8.725	2388	2390	2395	rVB2	356	233	0.01%	0.002%
55	8.754	2395	2399	2402	rBV	300	269	0.02%	0.002%
56	8.844	2414	2427	2455	rBV	768134	1297120	78.32%	9.950%
57	9.194	2533	2536	2537	rBV2	347	185	0.01%	0.001%
58	9.332	2576	2579	2584	rVB2	316	274	0.02%	0.002%
59	9.394	2595	2598	2605	rVV	251	261	0.02%	0.002%
60	9.587	2655	2658	2661	rVB2	469	301	0.02%	0.002%
61	9.712	2695	2697	2702	rVB2	271	180	0.01%	0.001%
62	9.741	2702	2706	2711	rVB2	306	267	0.02%	0.002%
63	9.821	2726	2731	2732	rBV3	216	180	0.01%	0.001%
64	9.985	2778	2782	2785	rVB2	357	245	0.01%	0.002%
65	10.162	2828	2837	2840	rBV3	9994	13711	0.83%	0.105%
66	10.204	2840	2850	2869	rVB	534070	833511	50.33%	6.394%
67	10.377	2898	2904	2909	rVB4	488	624	0.04%	0.005%
68	10.532	2945	2952	2953	rBV3	631	569	0.03%	0.004%
69	10.567	2956	2963	2974	rVB2	5582	8955	0.54%	0.069%
70	10.728	3011	3013	3017	rVB2	356	201	0.01%	0.002%
71	10.747	3017	3019	3022	rBV	508	258	0.02%	0.002%
72	10.786	3028	3031	3035	rBV2	450	415	0.03%	0.003%
73	10.844	3045	3049	3052	rVB3	374	305	0.02%	0.002%
74	10.898	3062	3066	3074	rBV2	600	733	0.04%	0.006%
75	11.130	3132	3138	3142	rBV2	402	453	0.03%	0.003%
76	11.175	3144	3152	3159	rBV5	1145	1817	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
 Data File : VV029778.D
 Acq On : 23 Dec 2022 10:19
 Operator : SY/MD
 Sample : VV1223WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK315

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.236	3159	3171	3190	rBV	893998	1394108	84.18%	10.694%
78	11.464	3237	3242	3246	rVB2	463	474	0.03%	0.004%
79	11.490	3246	3250	3254	rBV2	389	332	0.02%	0.003%
80	11.516	3256	3258	3266	rVB3	342	370	0.02%	0.003%
81	11.554	3266	3270	3273	rBV2	488	324	0.02%	0.002%
82	11.612	3273	3288	3311	rBV	765064	1223356	73.87%	9.384%
83	11.924	3383	3385	3390	rVB	419	354	0.02%	0.003%
84	11.975	3396	3401	3404	rVB2	240	230	0.01%	0.002%
85	12.001	3404	3409	3413	rBV3	412	403	0.02%	0.003%
86	12.078	3431	3433	3437	rBV	292	214	0.01%	0.002%
87	12.194	3462	3469	3473	rBV3	320	499	0.03%	0.004%
88	12.291	3497	3499	3501	rBV	382	187	0.01%	0.001%
89	12.455	3548	3550	3555	rVB3	314	237	0.01%	0.002%
90	12.635	3601	3606	3613	rVB4	1907	2316	0.14%	0.018%
91	12.670	3613	3617	3619	rBV3	337	273	0.02%	0.002%
92	12.766	3643	3647	3650	rBV	377	347	0.02%	0.003%
93	12.831	3666	3667	3672	rBV2	320	224	0.01%	0.002%
94	13.017	3722	3725	3730	rBV4	409	311	0.02%	0.002%
95	13.056	3735	3737	3740	rBV2	492	287	0.02%	0.002%
96	13.252	3790	3798	3807	rVB5	3172	4831	0.29%	0.037%
97	13.445	3855	3858	3861	rBV3	450	425	0.03%	0.003%
98	13.493	3864	3873	3889	rVB	17197	27973	1.69%	0.215%
99	13.731	3941	3947	3956	rVB5	2706	4556	0.28%	0.035%
100	14.692	4244	4246	4249	rBV	727	364	0.02%	0.003%




Sum of corrected areas: 13036688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029778.D
Acq On : 23 Dec 2022 10:19
Operator : SY/MD
Sample : VV1223WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

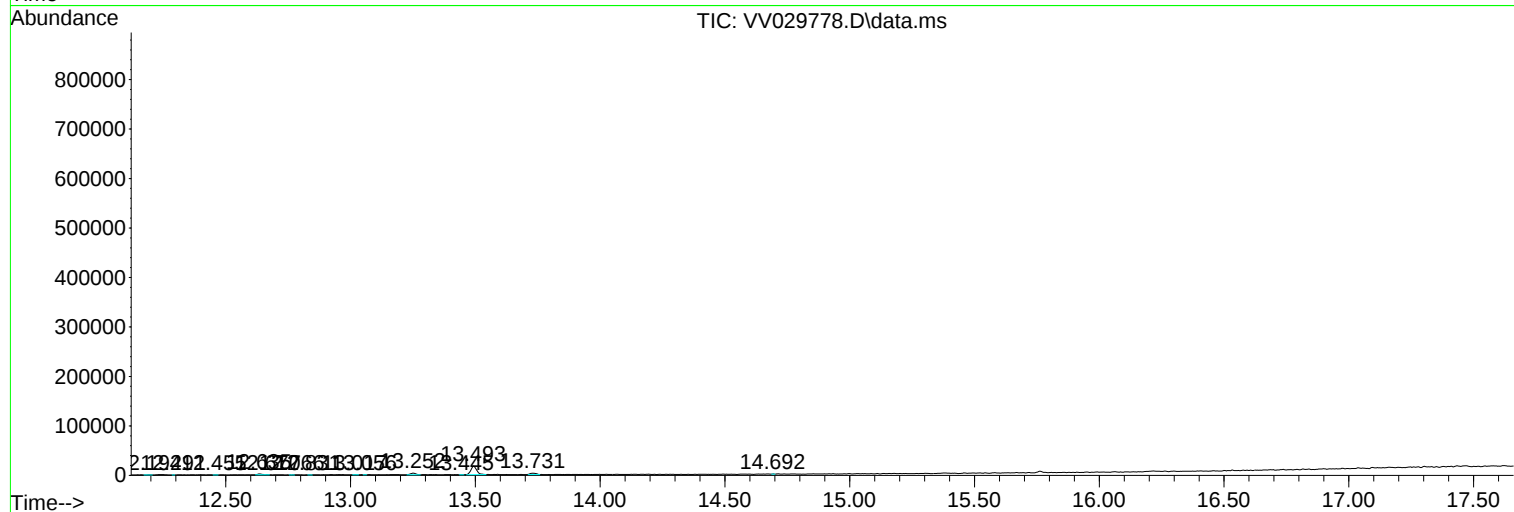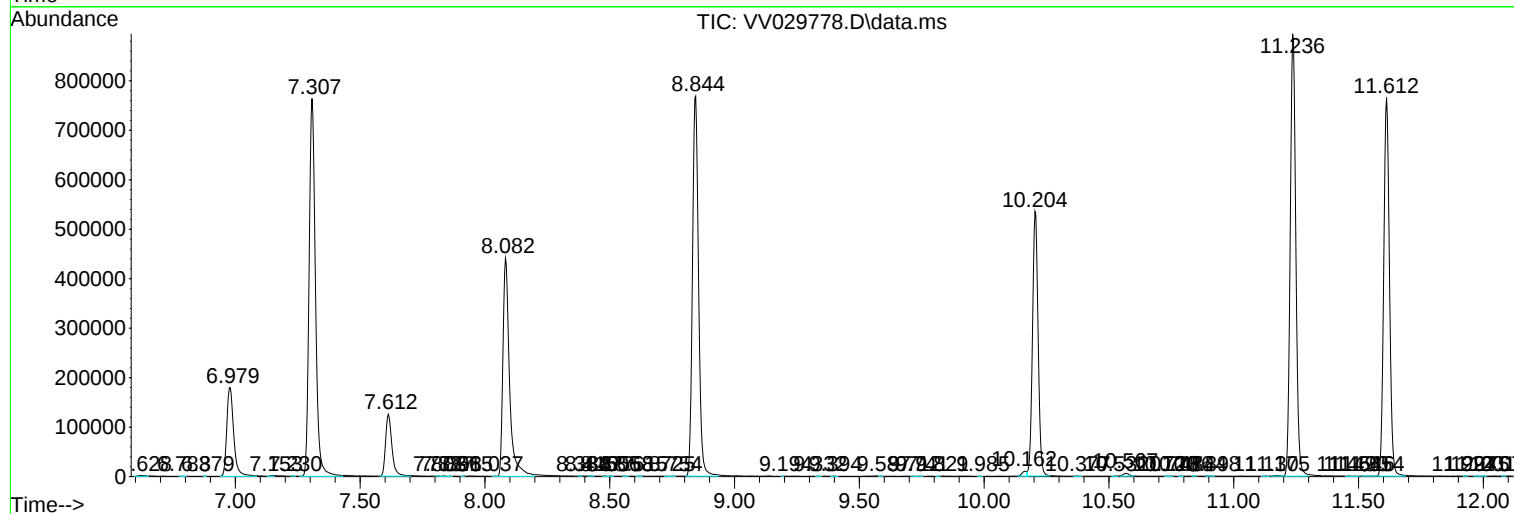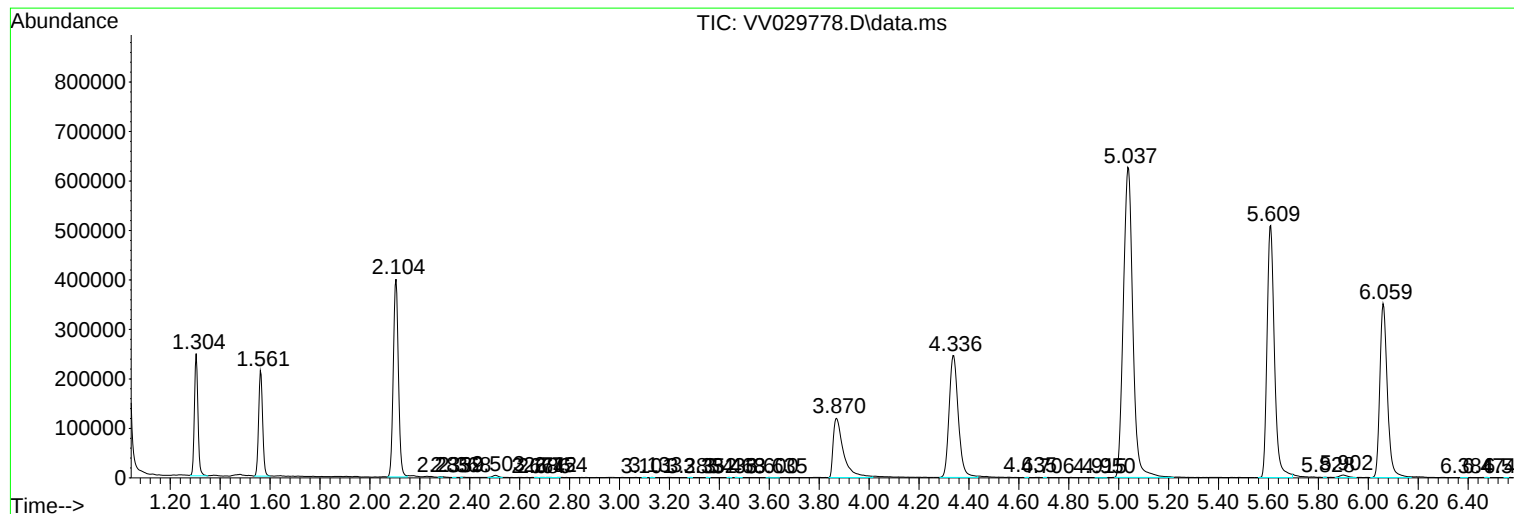

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029778.D
Acq On : 23 Dec 2022 10:19
Operator : SY/MD
Sample : VV1223WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029778.D
Acq On : 23 Dec 2022 10:19
Operator : SY/MD
Sample : VV1223WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK315

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc