

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
 Data File : VV029779.D
 Acq On : 23 Dec 2022 10:42
 Operator : SY/MD
 Sample : N6193-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	97	rVB	210209	207609	14.51%	1.848%
2	1.561	154	162	172	rBV	182901	200022	13.98%	1.780%
3	2.101	319	330	343	rBV	339852	482492	33.73%	4.294%
4	2.500	446	454	468	rVB2	3819	6580	0.46%	0.059%
5	2.609	485	488	493	rBV3	486	493	0.03%	0.004%
6	2.670	505	507	511	rBV2	309	196	0.01%	0.002%
7	2.799	545	547	549	rBV	239	138	0.01%	0.001%
8	2.992	605	607	611	rVB2	223	120	0.01%	0.001%
9	3.015	611	614	616	rBV	162	99	0.01%	0.001%
10	3.265	689	692	694	rBV	210	129	0.01%	0.001%
11	3.275	694	695	700	rVB2	274	167	0.01%	0.001%
12	3.301	700	703	707	rBV2	234	190	0.01%	0.002%
13	3.336	711	714	715	rBV2	177	100	0.01%	0.001%
14	3.359	718	721	722	rBV	178	113	0.01%	0.001%
15	3.523	766	772	778	rBV	154	239	0.02%	0.002%
16	3.561	781	784	791	rVV2	244	237	0.02%	0.002%
17	3.693	822	825	829	rVB2	122	88	0.01%	0.001%
18	3.715	829	832	834	rBV	237	163	0.01%	0.001%
19	3.764	844	847	851	rBV2	190	191	0.01%	0.002%
20	3.867	870	879	910	rBV	112747	301692	21.09%	2.685%
21	4.336	1010	1025	1056	rBV	215044	537781	37.60%	4.787%
22	4.596	1103	1106	1110	rBV2	347	279	0.02%	0.002%
23	4.677	1126	1131	1133	rBV	286	234	0.02%	0.002%
24	4.715	1141	1143	1146	rVB	215	118	0.01%	0.001%
25	4.741	1149	1151	1154	rBV	276	191	0.01%	0.002%
26	4.773	1159	1161	1165	rVV2	255	148	0.01%	0.001%
27	4.799	1165	1169	1175	rVB2	351	284	0.02%	0.003%
28	4.828	1175	1178	1181	rBV2	300	132	0.01%	0.001%
29	4.931	1208	1210	1211	rBV	211	76	0.01%	0.001%
30	5.037	1220	1243	1293	rBV2	542688	1430454	100.00%	12.732%
31	5.275	1315	1317	1323	rVB3	308	220	0.02%	0.002%
32	5.397	1351	1355	1364	rVB3	462	596	0.04%	0.005%
33	5.436	1364	1367	1372	rVB2	539	430	0.03%	0.004%
34	5.465	1372	1376	1380	rBV2	472	505	0.04%	0.004%
35	5.519	1390	1393	1396	rVB	207	140	0.01%	0.001%
36	5.539	1397	1399	1401	rBV	163	63	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122322\
 Data File : VW029779.D
 Acq On : 23 Dec 2022 10:42
 Operator : SY/MD
 Sample : N6193-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.606	1404	1420	1464	rBV	425130	891252	62.31%	7.933%
38	5.895	1500	1510	1524	rVB4	4498	9953	0.70%	0.089%
39	5.950	1524	1527	1530	rBV2	251	194	0.01%	0.002%
40	6.059	1547	1561	1594	rBV	303668	634683	44.37%	5.649%
41	6.346	1647	1650	1654	rBV	363	203	0.01%	0.002%
42	6.368	1654	1657	1664	rVB	253	198	0.01%	0.002%
43	6.442	1678	1680	1685	rBV2	104	71	0.00%	0.001%
44	6.506	1697	1700	1702	rBV	190	102	0.01%	0.001%
45	6.574	1718	1721	1728	rVB2	271	231	0.02%	0.002%
46	6.612	1728	1733	1734	rBV	1371	1058	0.07%	0.009%
47	6.754	1773	1777	1778	rBV	209	97	0.01%	0.001%
48	6.776	1781	1784	1787	rVV2	248	166	0.01%	0.001%
49	6.931	1830	1832	1833	rVB2	163	63	0.00%	0.001%
50	6.976	1833	1846	1879	rBV	157039	295670	20.67%	2.632%
51	7.111	1886	1888	1891	rBV2	267	165	0.01%	0.001%
52	7.146	1894	1899	1900	rBV3	987	784	0.05%	0.007%
53	7.243	1925	1929	1932	rVB2	432	327	0.02%	0.003%
54	7.307	1936	1949	1991	rBV	639186	1147255	80.20%	10.211%
55	7.612	2034	2044	2070	rBV	110641	194305	13.58%	1.729%
56	7.770	2091	2093	2095	rBV2	309	164	0.01%	0.001%
57	7.841	2112	2115	2120	rBV2	354	329	0.02%	0.003%
58	7.866	2121	2123	2128	rVB3	442	298	0.02%	0.003%
59	8.011	2166	2168	2170	rBV2	214	112	0.01%	0.001%
60	8.082	2180	2190	2226	rBV	388797	717535	50.16%	6.386%
61	8.545	2332	2334	2335	rBV	288	111	0.01%	0.001%
62	8.587	2344	2347	2349	rBV2	274	157	0.01%	0.001%
63	8.641	2362	2364	2367	rBV	335	153	0.01%	0.001%
64	8.673	2372	2374	2381	rBV2	428	313	0.02%	0.003%
65	8.786	2406	2409	2411	rBV	248	155	0.01%	0.001%
66	8.844	2414	2427	2450	rBV	675741	1108065	77.46%	9.862%
67	9.079	2497	2500	2504	rBV2	396	265	0.02%	0.002%
68	9.207	2538	2540	2543	rVB3	324	121	0.01%	0.001%
69	9.464	2618	2620	2624	rVB2	214	99	0.01%	0.001%
70	9.493	2627	2629	2632	rBV2	222	112	0.01%	0.001%
71	9.587	2656	2658	2660	rBV2	139	61	0.00%	0.001%
72	9.609	2660	2665	2669	rBV3	249	287	0.02%	0.003%
73	9.673	2682	2685	2686	rBV	185	111	0.01%	0.001%
74	9.718	2697	2699	2701	rBV2	215	108	0.01%	0.001%
75	9.879	2745	2749	2755	rVB2	359	348	0.02%	0.003%
76	9.918	2758	2761	2766	rBV3	560	430	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
 Data File : VV029779.D
 Acq On : 23 Dec 2022 10:42
 Operator : SY/MD
 Sample : N6193-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.050	2797	2802	2805	rVB	274	182	0.01%	0.002%
78	10.088	2812	2814	2817	rVB	282	145	0.01%	0.001%
79	10.120	2822	2824	2826	rVB	279	117	0.01%	0.001%
80	10.162	2828	2837	2840	rBV2	8583	11353	0.79%	0.101%
81	10.204	2841	2850	2869	rVB	476093	736073	51.46%	6.551%
82	10.397	2908	2910	2911	rBV	303	119	0.01%	0.001%
83	10.529	2948	2951	2954	rBV	665	471	0.03%	0.004%
84	10.567	2955	2963	2976	rVB2	5000	8326	0.58%	0.074%
85	10.686	2998	3000	3001	rBV2	206	71	0.00%	0.001%
86	10.779	3026	3029	3030	rBV	171	86	0.01%	0.001%
87	10.789	3030	3032	3036	rVV3	253	163	0.01%	0.001%
88	10.828	3042	3044	3045	rBV	383	122	0.01%	0.001%
89	11.027	3104	3106	3107	rBV	237	108	0.01%	0.001%
90	11.095	3125	3127	3128	rBV	287	129	0.01%	0.001%
91	11.175	3147	3152	3160	rVB4	1289	1563	0.11%	0.014%
92	11.236	3160	3171	3202	rBV	773764	1198377	83.78%	10.666%
93	11.522	3258	3260	3261	rBV	268	91	0.01%	0.001%
94	11.612	3275	3288	3318	rBV	688597	1086597	75.96%	9.671%
95	11.918	3380	3383	3384	rBV	374	211	0.01%	0.002%
96	12.197	3467	3470	3475	rBV2	413	293	0.02%	0.003%
97	12.519	3567	3570	3574	rBV2	633	543	0.04%	0.005%
98	12.593	3590	3593	3599	rBV3	545	477	0.03%	0.004%
99	13.168	3768	3772	3777	rBV2	599	541	0.04%	0.005%
100	13.493	3866	3873	3884	rBV	6914	10281	0.72%	0.092%




Sum of corrected areas: 11235259

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029779.D
Acq On : 23 Dec 2022 10:42
Operator : SY/MD
Sample : N6193-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

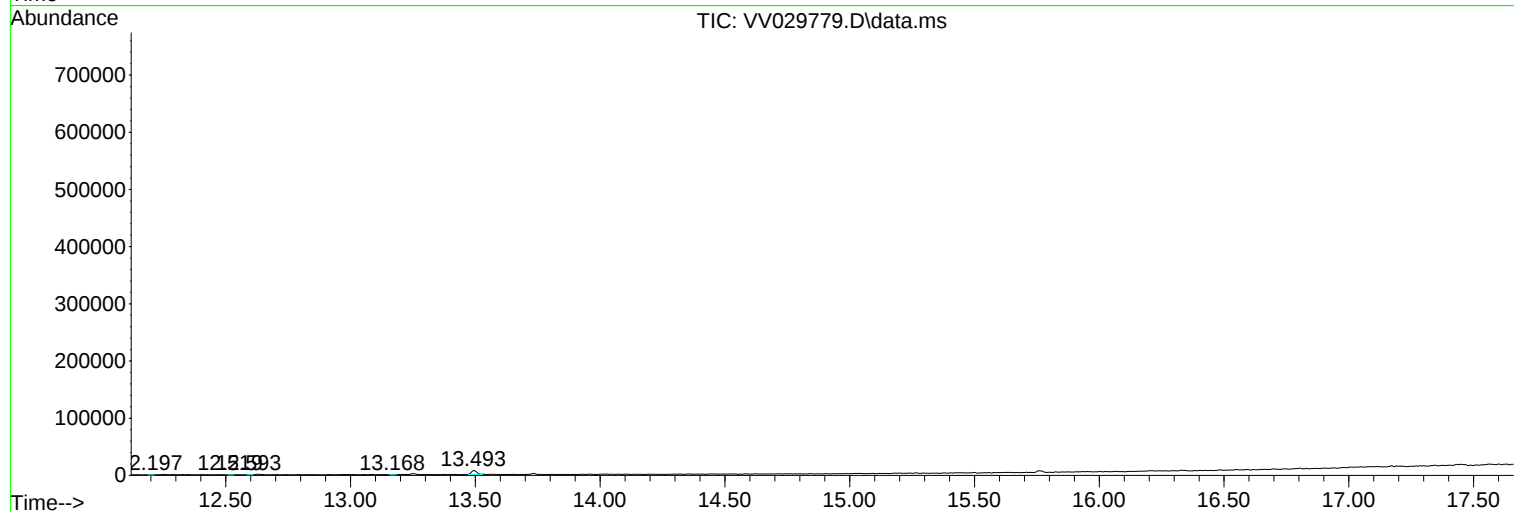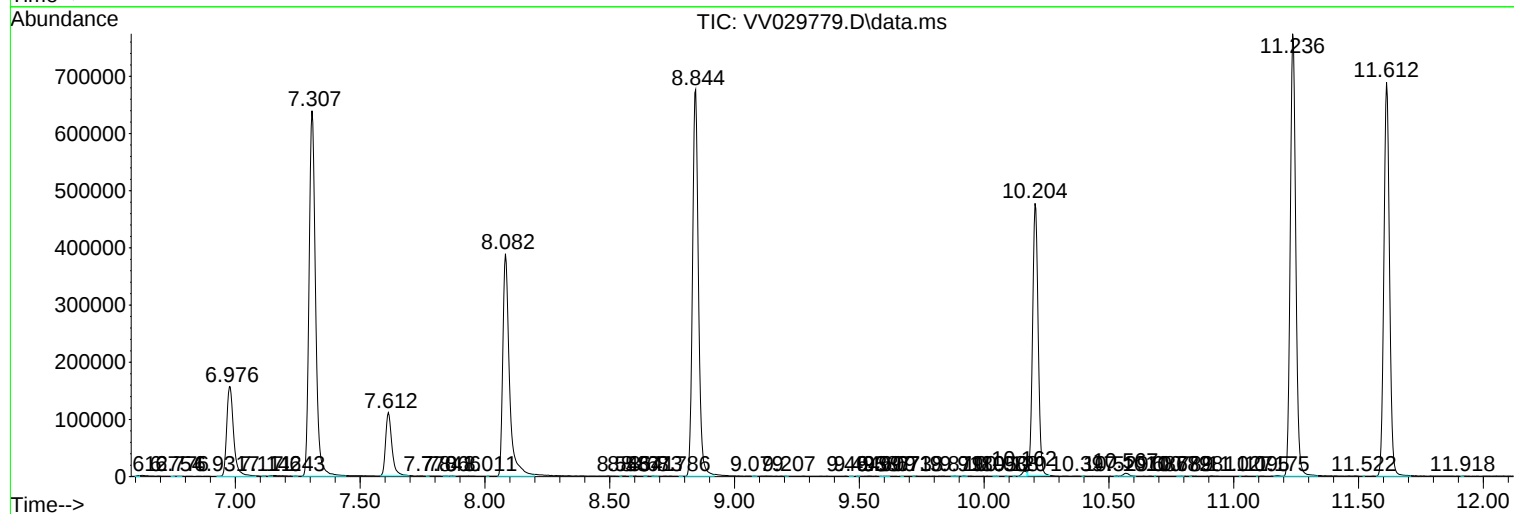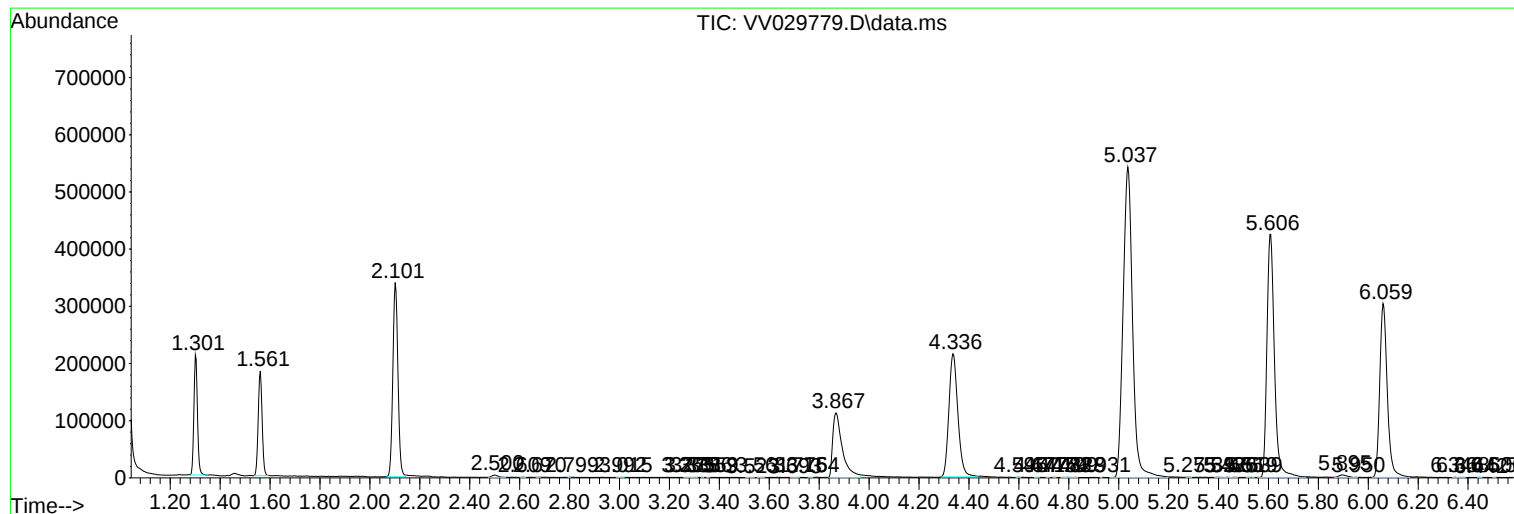

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029779.D
Acq On : 23 Dec 2022 10:42
Operator : SY/MD
Sample : N6193-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029779.D
Acq On : 23 Dec 2022 10:42
Operator : SY/MD
Sample : N6193-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc