

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122322\
 Data File : VW029780.D
 Acq On : 23 Dec 2022 11:11
 Operator : SY/MD
 Sample : N6195-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VW029780.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	262823	260378	14.83%	1.887%
2	1.561	154	162	176	rVB	225814	251386	14.32%	1.821%
3	2.015	296	303	305	rBV4	626	782	0.04%	0.006%
4	2.101	319	330	343	rBV	425908	611627	34.83%	4.432%
5	2.275	379	384	395	rVB3	4309	7846	0.45%	0.057%
6	2.384	416	418	421	rBV2	573	337	0.02%	0.002%
7	2.500	444	454	463	rBV4	2280	3532	0.20%	0.026%
8	2.622	486	492	494	rBV3	228	218	0.01%	0.002%
9	2.777	537	540	548	rVB2	230	269	0.02%	0.002%
10	3.027	615	618	623	rVB2	297	274	0.02%	0.002%
11	3.082	633	635	640	rVV2	357	274	0.02%	0.002%
12	3.130	647	650	657	rVB	232	221	0.01%	0.002%
13	3.230	677	681	684	rBV2	299	223	0.01%	0.002%
14	3.564	778	785	789	rBV2	218	287	0.02%	0.002%
15	3.706	825	829	833	rVB2	291	260	0.01%	0.002%
16	3.786	848	854	857	rBV3	389	450	0.03%	0.003%
17	3.805	857	860	866	rVB3	276	287	0.02%	0.002%
18	3.867	869	879	910	rBV	123749	338196	19.26%	2.450%
19	4.211	984	986	991	rVB3	481	345	0.02%	0.002%
20	4.333	1008	1024	1057	rBV2	262277	673048	38.33%	4.877%
21	4.561	1091	1095	1098	rBV2	242	224	0.01%	0.002%
22	4.722	1142	1145	1150	rVB3	360	306	0.02%	0.002%
23	4.825	1173	1177	1182	rVB2	268	231	0.01%	0.002%
24	5.034	1223	1242	1294	rBV2	663693	1755890	100.00%	12.723%
25	5.249	1306	1309	1311	rBV3	481	274	0.02%	0.002%
26	5.304	1323	1326	1331	rBV	272	234	0.01%	0.002%
27	5.352	1336	1341	1344	rBV2	470	412	0.02%	0.003%
28	5.400	1353	1356	1364	rVB3	496	494	0.03%	0.004%
29	5.606	1406	1420	1460	rBV	540278	1118174	63.68%	8.102%
30	5.802	1478	1481	1486	rBV3	347	290	0.02%	0.002%
31	5.847	1493	1495	1500	rVB3	391	245	0.01%	0.002%
32	5.892	1500	1509	1524	rBV5	4578	10097	0.58%	0.073%
33	6.059	1545	1561	1585	rBV	372915	774177	44.09%	5.610%
34	6.616	1724	1734	1736	rBV4	1735	2261	0.13%	0.016%
35	6.725	1767	1768	1775	rVB	267	206	0.01%	0.001%
36	6.873	1810	1814	1818	rVB2	379	330	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122322\
 Data File : VW029780.D
 Acq On : 23 Dec 2022 11:11
 Operator : SY/MD
 Sample : N6195-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.924	1827	1830	1833	rBV3	292	210	0.01%	0.002%
38	6.976	1833	1846	1869	rBV	194876	354907	20.21%	2.572%
39	7.149	1893	1900	1903	rBV5	973	1319	0.08%	0.010%
40	7.307	1936	1949	1988	rBV	806761	1439635	81.99%	10.431%
41	7.609	2031	2043	2076	rBV	135300	241627	13.76%	1.751%
42	7.876	2123	2126	2129	rBV2	284	273	0.02%	0.002%
43	7.931	2135	2143	2155	rVB3	2851	4713	0.27%	0.034%
44	8.082	2179	2190	2231	rBV	429343	799849	45.55%	5.796%
45	8.474	2309	2312	2314	rBV2	360	233	0.01%	0.002%
46	8.616	2353	2356	2359	rVB2	403	261	0.01%	0.002%
47	8.683	2374	2377	2381	rVB2	520	329	0.02%	0.002%
48	8.796	2409	2412	2414	rBV4	455	296	0.02%	0.002%
49	8.841	2414	2426	2451	rBV	837377	1371472	78.11%	9.937%
50	8.998	2473	2475	2484	rVB5	612	790	0.04%	0.006%
51	9.133	2516	2517	2524	rVV4	712	511	0.03%	0.004%
52	9.169	2524	2528	2531	rVB2	281	260	0.01%	0.002%
53	9.320	2570	2575	2580	rBV3	257	338	0.02%	0.002%
54	9.413	2601	2604	2607	rVB2	334	274	0.02%	0.002%
55	9.677	2683	2686	2690	rVB2	329	212	0.01%	0.002%
56	9.718	2690	2699	2701	rBV2	240	301	0.02%	0.002%
57	9.834	2732	2735	2741	rVB3	283	264	0.02%	0.002%
58	10.030	2793	2796	2802	rVB2	294	242	0.01%	0.002%
59	10.066	2804	2807	2814	rBV3	348	256	0.01%	0.002%
60	10.098	2814	2817	2821	rVB	365	236	0.01%	0.002%
61	10.162	2821	2837	2839	rBV2	11388	14355	0.82%	0.104%
62	10.204	2840	2850	2874	rVB	547131	865278	49.28%	6.270%
63	10.374	2895	2903	2910	rVB4	3599	5757	0.33%	0.042%
64	10.529	2950	2951	2954	rVB3	515	232	0.01%	0.002%
65	10.567	2954	2963	2980	rVB3	6741	10963	0.62%	0.079%
66	10.715	3007	3009	3012	rBV2	429	332	0.02%	0.002%
67	10.783	3024	3030	3033	rBV2	346	312	0.02%	0.002%
68	10.834	3038	3046	3048	rBV3	400	472	0.03%	0.003%
69	10.931	3074	3076	3083	rVB3	334	284	0.02%	0.002%
70	11.075	3119	3121	3126	rVB2	350	241	0.01%	0.002%
71	11.172	3144	3151	3158	rBV4	629	847	0.05%	0.006%
72	11.236	3158	3171	3200	rBV	959002	1497562	85.29%	10.851%
73	11.429	3228	3231	3233	rBV3	362	218	0.01%	0.002%
74	11.471	3242	3244	3250	rVB4	409	308	0.02%	0.002%
75	11.554	3263	3270	3275	rBV4	1421	1810	0.10%	0.013%
76	11.612	3275	3288	3313	rVV	858965	1353136	77.06%	9.805%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122322\
 Data File : VW029780.D
 Acq On : 23 Dec 2022 11:11
 Operator : SY/MD
 Sample : N6195-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.802	3340	3347	3349	rBV4	569	601	0.03%	0.004%
78	11.837	3353	3358	3361	rBV4	331	321	0.02%	0.002%
79	11.892	3371	3375	3379	rBV2	254	215	0.01%	0.002%
80	11.985	3402	3404	3409	rBV3	234	214	0.01%	0.002%
81	12.014	3411	3413	3416	rVV2	437	215	0.01%	0.002%
82	12.104	3438	3441	3445	rVB2	329	257	0.01%	0.002%
83	12.127	3445	3448	3454	rVB3	390	425	0.02%	0.003%
84	12.239	3479	3483	3492	rVB4	811	1028	0.06%	0.007%
85	12.320	3504	3508	3510	rBV3	414	296	0.02%	0.002%
86	12.345	3510	3516	3519	rVV3	703	705	0.04%	0.005%
87	12.628	3601	3604	3612	rVB4	773	974	0.06%	0.007%
88	12.721	3630	3633	3637	rVV3	459	334	0.02%	0.002%
89	12.808	3657	3660	3662	rBV	345	232	0.01%	0.002%
90	12.924	3693	3696	3699	rBV4	615	382	0.02%	0.003%
91	13.104	3750	3752	3755	rVB2	659	325	0.02%	0.002%
92	13.120	3755	3757	3760	rBV3	344	221	0.01%	0.002%
93	13.139	3760	3763	3766	rBV4	342	207	0.01%	0.001%
94	13.426	3848	3852	3853	rBV2	532	372	0.02%	0.003%
95	13.455	3858	3861	3862	rBV2	474	300	0.02%	0.002%
96	13.493	3870	3873	3884	rVB3	3790	4804	0.27%	0.035%
97	13.612	3908	3910	3913	rBV3	337	235	0.01%	0.002%
98	13.731	3942	3947	3958	rVB6	1484	2428	0.14%	0.018%
99	13.773	3958	3960	3966	rBV4	541	552	0.03%	0.004%
100	14.194	4088	4091	4094	rBV2	571	466	0.03%	0.003%


Sum of corrected areas: 13801109

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029780.D
Acq On : 23 Dec 2022 11:11
Operator : SY/MD
Sample : N6195-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

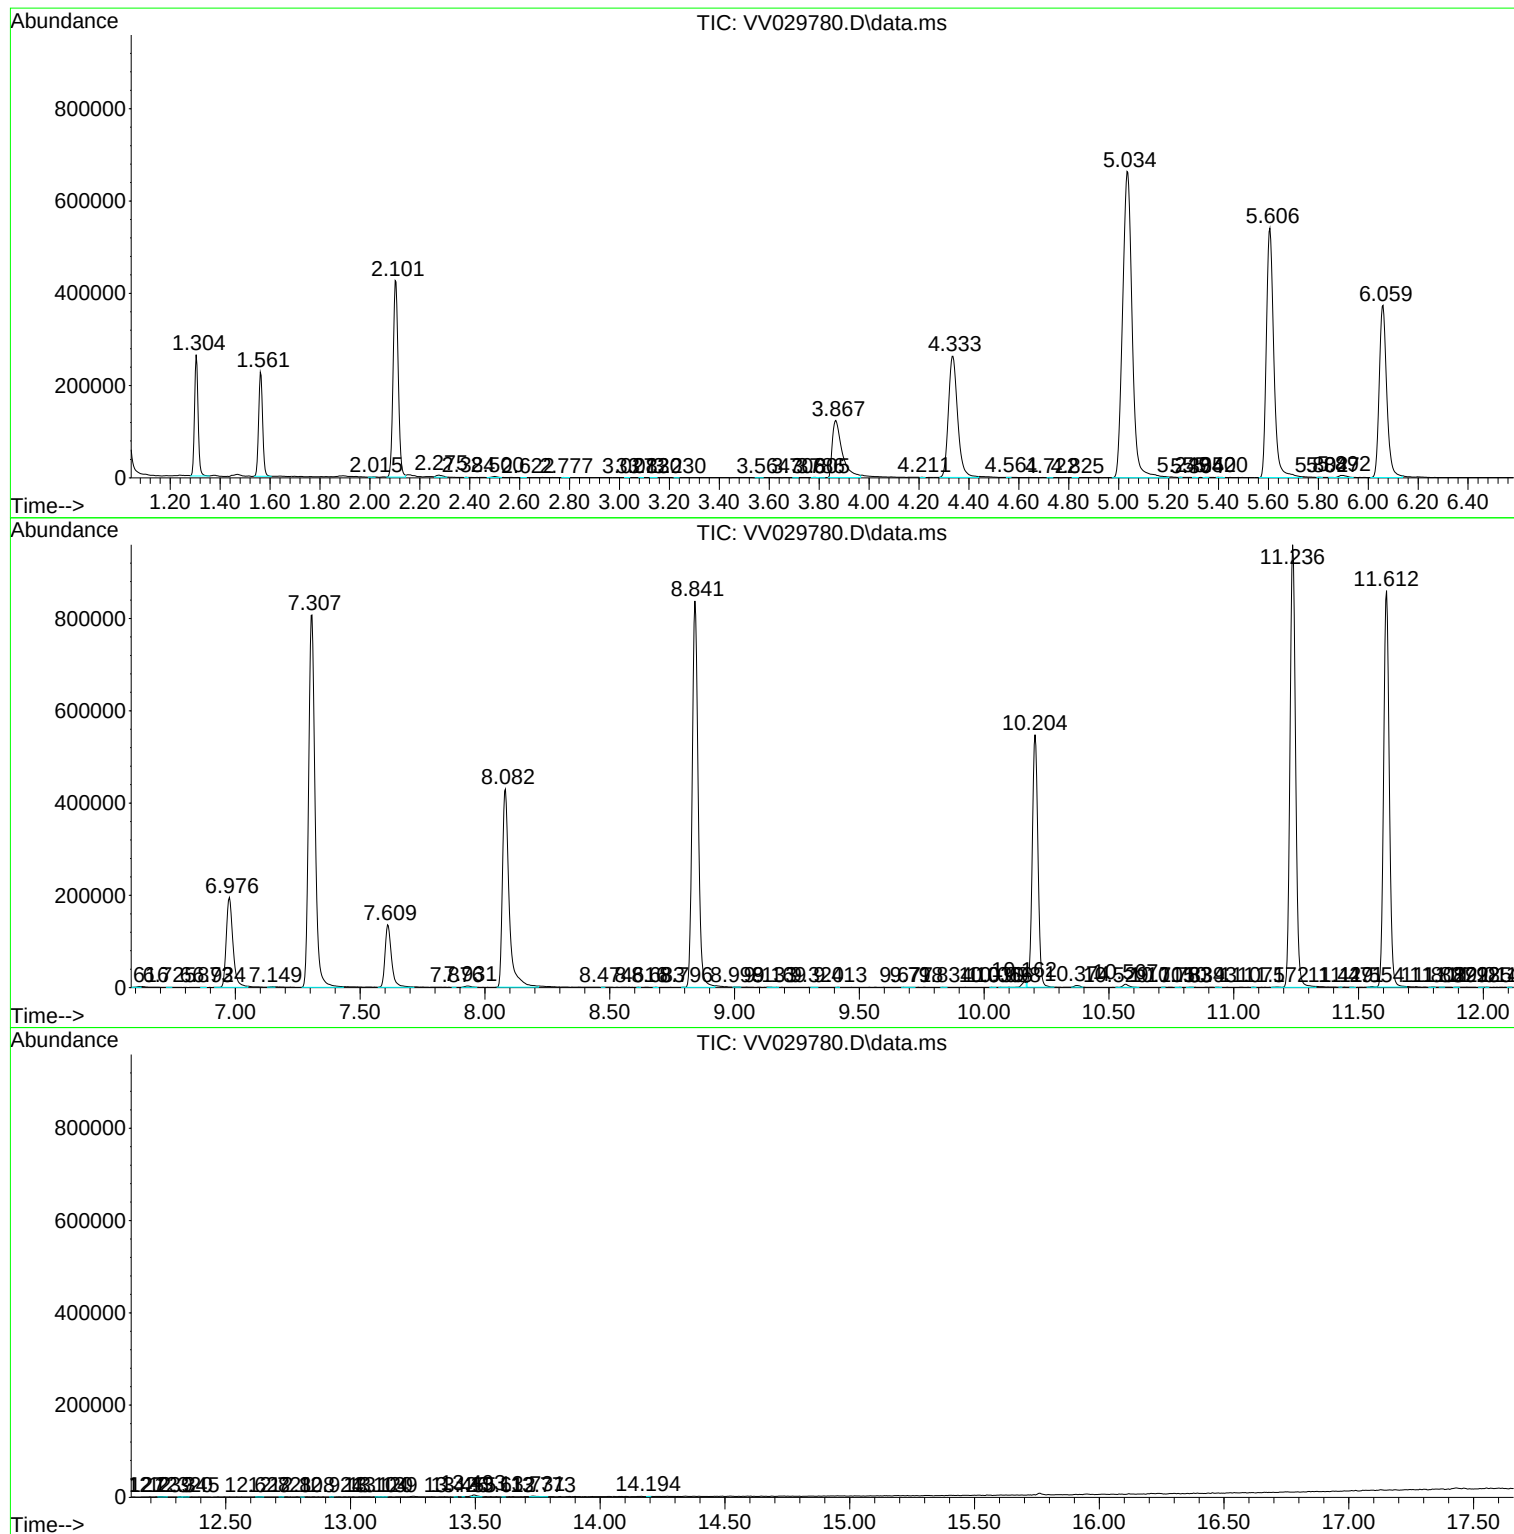

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029780.D
Acq On : 23 Dec 2022 11:11
Operator : SY/MD
Sample : N6195-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029780.D
Acq On : 23 Dec 2022 11:11
Operator : SY/MD
Sample : N6195-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc