

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
 Data File : VV029781.D
 Acq On : 23 Dec 2022 11:36
 Operator : SY/MD
 Sample : N6195-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029781.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	246093	245035	14.86%	1.875%
2	1.564	154	163	175	rBV	211049	239790	14.54%	1.835%
3	1.982	290	293	298	rBV3	697	646	0.04%	0.005%
4	2.105	319	331	347	rBV	412847	588993	35.72%	4.507%
5	2.288	384	388	390	rBV2	592	507	0.03%	0.004%
6	2.503	446	455	468	rVB2	5734	9236	0.56%	0.071%
7	2.857	560	565	568	rBV2	447	350	0.02%	0.003%
8	3.220	675	678	686	rVB2	196	198	0.01%	0.002%
9	3.452	745	750	755	rBV2	432	391	0.02%	0.003%
10	3.551	778	781	783	rBV	298	197	0.01%	0.002%
11	3.751	840	843	847	rVB	269	220	0.01%	0.002%
12	3.780	847	852	855	rBV3	469	403	0.02%	0.003%
13	3.867	869	879	909	rBV	116859	313660	19.02%	2.400%
14	4.275	1002	1006	1008	rBV3	300	291	0.02%	0.002%
15	4.339	1008	1026	1059	rBV	251058	636900	38.63%	4.874%
16	4.809	1168	1172	1178	rVB2	263	325	0.02%	0.002%
17	5.037	1226	1243	1287	rBV2	625135	1648894	100.00%	12.618%
18	5.474	1374	1379	1381	rBV2	257	253	0.02%	0.002%
19	5.606	1406	1420	1460	rBV	514594	1068838	64.82%	8.179%
20	5.780	1472	1474	1477	rVB2	524	271	0.02%	0.002%
21	5.899	1502	1511	1524	rBV4	4649	9275	0.56%	0.071%
22	6.059	1547	1561	1591	rBV	351590	734419	44.54%	5.620%
23	6.500	1692	1698	1702	rBV2	250	267	0.02%	0.002%
24	6.616	1726	1734	1735	rBV4	1357	1406	0.09%	0.011%
25	6.725	1763	1768	1773	rVB	370	345	0.02%	0.003%
26	6.754	1773	1777	1780	rBV2	290	220	0.01%	0.002%
27	6.873	1810	1814	1817	rBV2	421	283	0.02%	0.002%
28	6.976	1834	1846	1870	rBV	182919	336479	20.41%	2.575%
29	7.146	1894	1899	1902	rBV3	899	923	0.06%	0.007%
30	7.233	1924	1926	1933	rVB3	791	673	0.04%	0.005%
31	7.307	1936	1949	1983	rBV	781916	1366637	82.88%	10.458%
32	7.612	2032	2044	2066	rBV	128718	224760	13.63%	1.720%
33	7.931	2134	2143	2146	rBV5	899	1179	0.07%	0.009%
34	7.998	2160	2164	2168	rVB3	231	223	0.01%	0.002%
35	8.021	2168	2171	2176	rVB2	304	246	0.01%	0.002%
36	8.082	2179	2190	2222	rBV	405351	744857	45.17%	5.700%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122322\
 Data File : VW029781.D
 Acq On : 23 Dec 2022 11:36
 Operator : SY/MD
 Sample : N6195-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	8.317	2259	2263	2267	rVB4	665	707	0.04%	0.005%
38	8.349	2267	2273	2276	rBV6	605	540	0.03%	0.004%
39	8.365	2276	2278	2284	rVB4	362	287	0.02%	0.002%
40	8.513	2322	2324	2327	rBV	367	224	0.01%	0.002%
41	8.635	2359	2362	2366	rVB4	282	244	0.01%	0.002%
42	8.841	2414	2426	2456	rBV	793892	1314603	79.73%	10.060%
43	9.040	2486	2488	2491	rVB2	464	197	0.01%	0.002%
44	9.066	2491	2496	2497	rBV3	252	238	0.01%	0.002%
45	9.159	2521	2525	2528	rVB2	377	272	0.02%	0.002%
46	9.198	2535	2537	2543	rVB2	300	227	0.01%	0.002%
47	9.265	2552	2558	2561	rBV3	282	322	0.02%	0.002%
48	9.371	2588	2591	2595	rBV2	286	206	0.01%	0.002%
49	9.416	2601	2605	2609	rVB2	324	211	0.01%	0.002%
50	9.448	2613	2615	2621	rBV2	323	282	0.02%	0.002%
51	9.538	2636	2643	2646	rBV3	460	494	0.03%	0.004%
52	9.561	2646	2650	2654	rVB3	422	287	0.02%	0.002%
53	9.583	2654	2657	2659	rBV2	361	234	0.01%	0.002%
54	9.628	2667	2671	2677	rBV3	282	273	0.02%	0.002%
55	9.689	2687	2690	2695	rBV2	246	210	0.01%	0.002%
56	9.712	2695	2697	2700	rBV	324	213	0.01%	0.002%
57	9.805	2723	2726	2730	rVV2	303	217	0.01%	0.002%
58	9.853	2737	2741	2745	rVB3	293	262	0.02%	0.002%
59	9.886	2745	2751	2754	rBV	379	413	0.03%	0.003%
60	9.927	2761	2764	2768	rVB2	244	216	0.01%	0.002%
61	9.992	2778	2784	2788	rBV2	314	380	0.02%	0.003%
62	10.050	2798	2802	2805	rVB3	277	227	0.01%	0.002%
63	10.072	2805	2809	2814	rVB2	402	268	0.02%	0.002%
64	10.098	2814	2817	2820	rBV	393	320	0.02%	0.002%
65	10.162	2828	2837	2840	rBV2	9592	13137	0.80%	0.101%
66	10.204	2840	2850	2875	rVB	526290	824465	50.00%	6.309%
67	10.339	2887	2892	2893	rBV	377	371	0.02%	0.003%
68	10.368	2895	2901	2903	rBV2	836	727	0.04%	0.006%
69	10.532	2948	2952	2954	rBV3	321	285	0.02%	0.002%
70	10.567	2955	2963	2976	rVB	5856	9534	0.58%	0.073%
71	10.680	2992	2998	3000	rBV2	307	221	0.01%	0.002%
72	10.760	3017	3023	3027	rVB2	347	344	0.02%	0.003%
73	10.908	3063	3069	3071	rVV3	442	397	0.02%	0.003%
74	10.985	3089	3093	3100	rVB2	306	333	0.02%	0.003%
75	11.175	3148	3152	3157	rVB2	631	576	0.03%	0.004%
76	11.236	3157	3171	3204	rBV	911828	1430089	86.73%	10.943%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
 Data File : VV029781.D
 Acq On : 23 Dec 2022 11:36
 Operator : SY/MD
 Sample : N6195-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.416	3225	3227	3233	rVB3	439	315	0.02%	0.002%
78	11.490	3246	3250	3253	rVB3	406	296	0.02%	0.002%
79	11.535	3262	3264	3267	rBV	295	199	0.01%	0.002%
80	11.612	3276	3288	3324	rBV	802516	1275499	77.35%	9.760%
81	11.873	3365	3369	3373	rBV2	358	406	0.02%	0.003%
82	11.898	3375	3377	3382	rVB2	350	259	0.02%	0.002%
83	11.988	3402	3405	3407	rBV	447	222	0.01%	0.002%
84	12.091	3435	3437	3442	rBV	330	316	0.02%	0.002%
85	12.230	3476	3480	3481	rBV2	621	443	0.03%	0.003%
86	12.336	3510	3513	3515	rBV2	462	259	0.02%	0.002%
87	12.464	3550	3553	3557	rBV4	484	278	0.02%	0.002%
88	12.635	3601	3606	3610	rBV3	951	1002	0.06%	0.008%
89	12.689	3619	3623	3626	rBV2	530	389	0.02%	0.003%
90	12.760	3642	3645	3648	rVB3	351	205	0.01%	0.002%
91	12.799	3653	3657	3660	rBV3	391	334	0.02%	0.003%
92	12.824	3661	3665	3666	rBV	354	239	0.01%	0.002%
93	12.863	3674	3677	3680	rBV2	528	276	0.02%	0.002%
94	12.931	3694	3698	3701	rBV2	374	284	0.02%	0.002%
95	13.406	3843	3846	3853	rBV4	400	504	0.03%	0.004%
96	13.496	3867	3874	3883	rBV2	2428	3614	0.22%	0.028%
97	13.728	3944	3946	3947	rBV	659	306	0.02%	0.002%
98	14.030	4037	4040	4042	rBV3	749	555	0.03%	0.004%
99	14.612	4218	4221	4224	rBV2	625	561	0.03%	0.004%
100	14.651	4230	4233	4235	rBV3	865	575	0.03%	0.004%




Sum of corrected areas: 13067979

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029781.D
Acq On : 23 Dec 2022 11:36
Operator : SY/MD
Sample : N6195-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

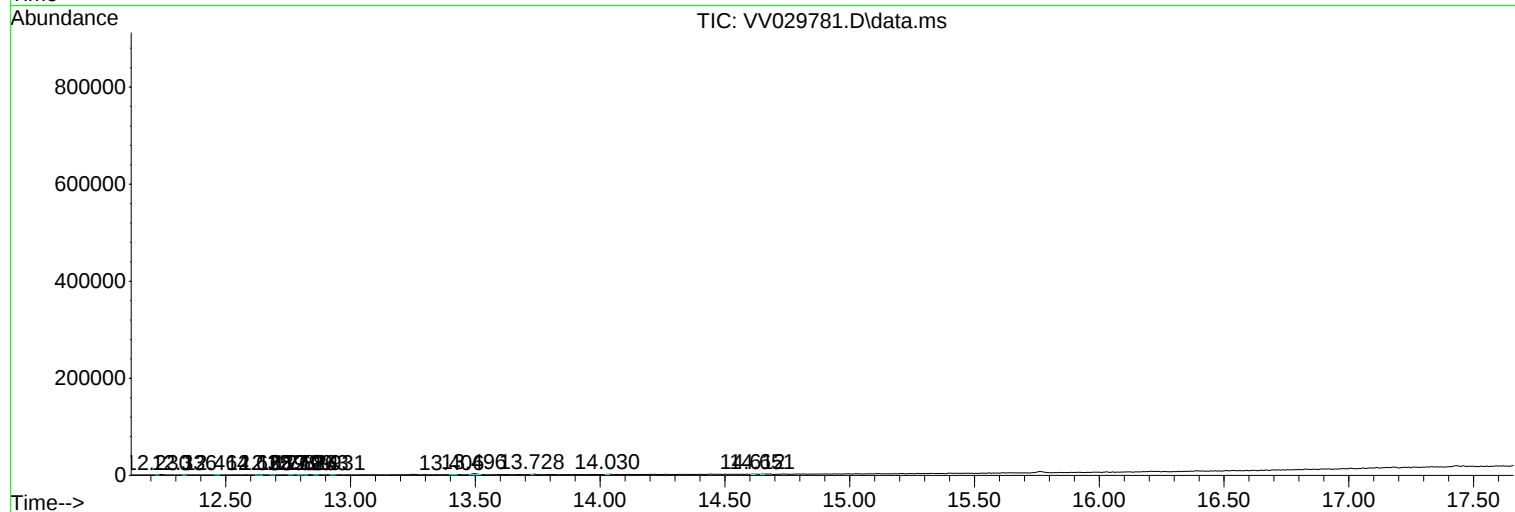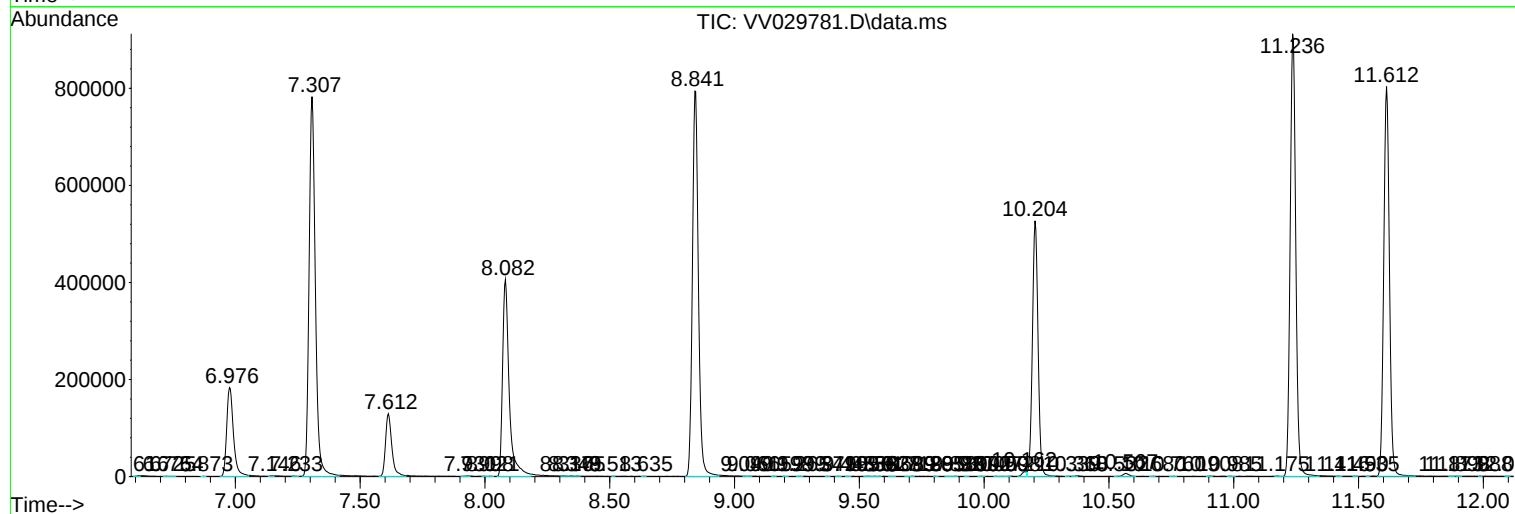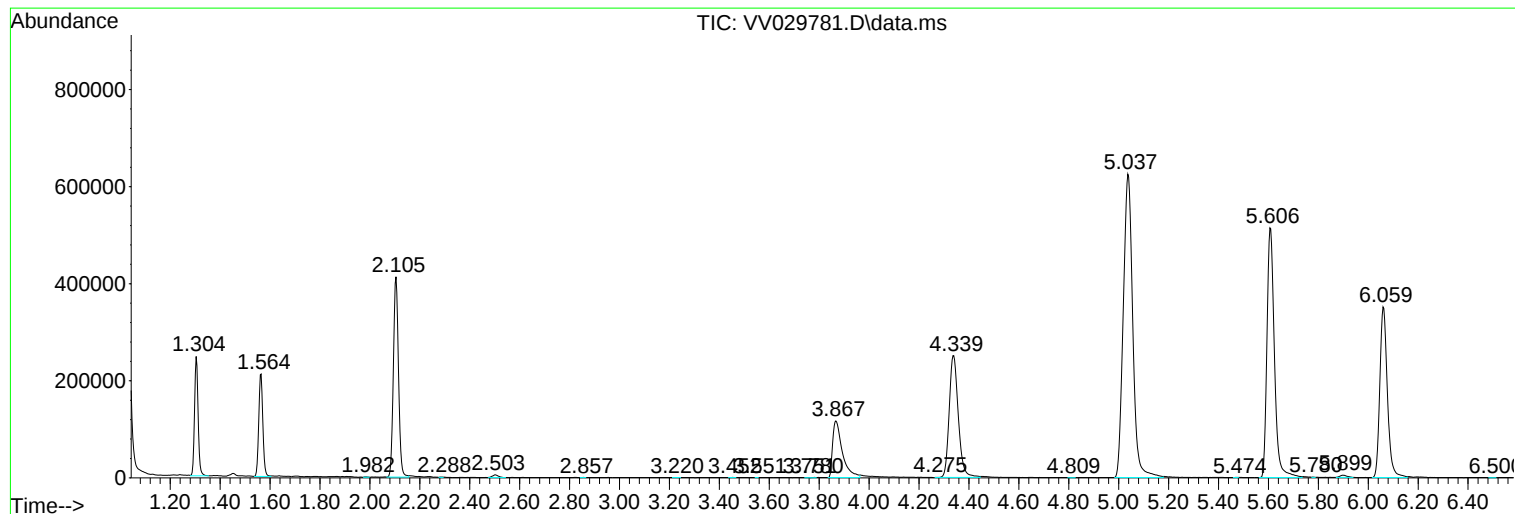

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029781.D
Acq On : 23 Dec 2022 11:36
Operator : SY/MD
Sample : N6195-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029781.D
Acq On : 23 Dec 2022 11:36
Operator : SY/MD
Sample : N6195-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc