

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122322\
 Data File : VW029782.D
 Acq On : 23 Dec 2022 12:03
 Operator : SY/MD
 Sample : N6171-08ME
 Misc : 4.96g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBQC6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029782.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	141061	182699	11.34%	1.372%
2	1.767	220	226	235	rVB2	38076	48623	3.02%	0.365%
3	2.085	315	325	341	rVB	328764	465685	28.90%	3.498%
4	3.011	610	613	615	rBV3	457	348	0.02%	0.003%
5	3.031	617	619	626	rVV3	354	250	0.02%	0.002%
6	3.072	630	632	636	rBV2	279	114	0.01%	0.001%
7	3.275	693	695	697	rBV	195	92	0.01%	0.001%
8	3.423	738	741	742	rBV	236	120	0.01%	0.001%
9	3.622	800	803	805	rBV	331	210	0.01%	0.002%
10	3.690	822	824	825	rBV	104	43	0.00%	0.000%
11	3.709	825	830	831	rBV	344	224	0.01%	0.002%
12	3.879	873	883	942	rBV2	82136	293783	18.23%	2.207%
13	4.330	1007	1023	1056	rBV	226005	576205	35.76%	4.328%
14	4.709	1138	1141	1144	rBV2	334	286	0.02%	0.002%
15	4.722	1144	1145	1146	rBV2	175	50	0.00%	0.000%
16	4.748	1151	1153	1155	rBV	149	75	0.00%	0.001%
17	4.783	1161	1164	1168	rBV	221	219	0.01%	0.002%
18	4.802	1168	1170	1175	rVB2	256	178	0.01%	0.001%
19	4.831	1177	1179	1182	rBV2	161	83	0.01%	0.001%
20	4.876	1190	1193	1195	rBV	110	74	0.00%	0.001%
21	4.947	1213	1215	1218	rVB	188	59	0.00%	0.000%
22	4.960	1218	1219	1220	rVB	111	21	0.00%	0.000%
23	5.030	1220	1241	1275	rBV2	584510	1458230	90.50%	10.954%
24	5.333	1333	1335	1338	rBV2	284	211	0.01%	0.002%
25	5.371	1345	1347	1349	rBV2	274	136	0.01%	0.001%
26	5.410	1357	1359	1361	rBV2	291	163	0.01%	0.001%
27	5.439	1364	1368	1371	rBV2	220	223	0.01%	0.002%
28	5.513	1388	1391	1396	rBV2	315	243	0.02%	0.002%
29	5.603	1406	1419	1450	rBV	586114	1200989	74.54%	9.022%
30	5.899	1500	1511	1523	rVB10	5562	13109	0.81%	0.098%
31	5.998	1536	1542	1547	rBV5	823	1160	0.07%	0.009%
32	6.056	1547	1560	1585	rBV	315126	655542	40.68%	4.924%
33	6.265	1624	1625	1626	rBV	134	45	0.00%	0.000%
34	6.284	1630	1631	1632	rBV	195	60	0.00%	0.000%
35	6.323	1641	1643	1644	rVB	193	54	0.00%	0.000%
36	6.333	1644	1646	1650	rBV	147	82	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122322\
 Data File : VW029782.D
 Acq On : 23 Dec 2022 12:03
 Operator : SY/MD
 Sample : N6171-08ME
 Misc : 4.96g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBQC6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.349	1650	1651	1652	rVB	88	18	0.00%	0.000%
38	6.484	1689	1693	1696	rBV2	295	240	0.01%	0.002%
39	6.497	1696	1697	1700	rVB	177	50	0.00%	0.000%
40	6.516	1700	1703	1705	rBV	193	133	0.01%	0.001%
41	6.571	1718	1720	1723	rVB2	361	168	0.01%	0.001%
42	6.590	1723	1726	1730	rBV2	247	212	0.01%	0.002%
43	6.609	1730	1732	1735	rBV	147	97	0.01%	0.001%
44	6.786	1784	1787	1789	rBV	326	251	0.02%	0.002%
45	6.976	1833	1846	1871	rBV	169701	321349	19.94%	2.414%
46	7.304	1936	1948	1979	rBV	663128	1174205	72.87%	8.821%
47	7.612	2033	2044	2067	rBV	114101	213712	13.26%	1.605%
48	7.825	2107	2110	2111	rBV2	498	282	0.02%	0.002%
49	7.963	2139	2153	2174	rBV	858209	1425876	88.49%	10.711%
50	8.091	2182	2193	2194	rBV	207714	270322	16.78%	2.031%
51	8.468	2308	2310	2312	rBV2	475	289	0.02%	0.002%
52	8.567	2338	2341	2344	rBV2	425	340	0.02%	0.003%
53	8.616	2354	2356	2358	rBV	172	99	0.01%	0.001%
54	8.661	2368	2370	2374	rVB2	663	359	0.02%	0.003%
55	8.683	2374	2377	2378	rBV	260	114	0.01%	0.001%
56	8.735	2388	2393	2398	rBV5	503	653	0.04%	0.005%
57	8.796	2410	2412	2414	rBV2	245	87	0.01%	0.001%
58	8.841	2414	2426	2457	rBV	851122	1446590	89.78%	10.867%
59	9.239	2549	2550	2551	rBV	198	56	0.00%	0.000%
60	9.265	2557	2558	2561	rBV	215	96	0.01%	0.001%
61	9.316	2571	2574	2575	rBV2	264	150	0.01%	0.001%
62	9.445	2611	2614	2615	rBV	278	137	0.01%	0.001%
63	9.480	2622	2625	2627	rVB2	316	203	0.01%	0.002%
64	9.493	2627	2629	2631	rBV	64	27	0.00%	0.000%
65	9.509	2631	2634	2636	rBV	173	94	0.01%	0.001%
66	9.522	2636	2638	2641	rBV2	275	207	0.01%	0.002%
67	9.606	2661	2664	2665	rBV	218	135	0.01%	0.001%
68	9.725	2698	2701	2705	rBV2	344	277	0.02%	0.002%
69	9.776	2714	2717	2720	rVB2	363	146	0.01%	0.001%
70	9.789	2720	2721	2726	rBV2	302	279	0.02%	0.002%
71	9.857	2736	2742	2745	rBV2	238	303	0.02%	0.002%
72	9.889	2750	2752	2753	rBV2	267	104	0.01%	0.001%
73	9.918	2759	2761	2763	rVB	312	103	0.01%	0.001%
74	10.008	2782	2789	2791	rBV3	420	476	0.03%	0.004%
75	10.165	2826	2838	2840	rBV4	7101	9397	0.58%	0.071%
76	10.210	2841	2852	2870	rVB	447757	770905	47.84%	5.791%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
 Data File : VV029782.D
 Acq On : 23 Dec 2022 12:03
 Operator : SY/MD
 Sample : N6171-08ME
 Misc : 4.96g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBQC6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

77	10.416	2913	2916	2922	rVB3	546	423	0.03%	0.003%
78	10.484	2935	2937	2941	rVB2	462	252	0.02%	0.002%
79	10.535	2946	2953	2956	rBV4	469	638	0.04%	0.005%
80	10.570	2957	2964	2979	rVB4	4190	7526	0.47%	0.057%
81	10.625	2979	2981	2984	rBV	275	197	0.01%	0.001%
82	10.722	3006	3011	3014	rBV3	291	304	0.02%	0.002%
83	10.876	3056	3059	3061	rBV2	219	121	0.01%	0.001%
84	11.175	3148	3152	3154	rBV2	497	360	0.02%	0.003%
85	11.239	3159	3172	3195	rBV	1012569	1611277	100.00%	12.104%
86	11.615	3277	3289	3313	rVB	721271	1151345	71.46%	8.649%
87	12.011	3409	3412	3416	rBV3	424	334	0.02%	0.003%
88	13.596	3903	3905	3911	rBV4	716	690	0.04%	0.005%
89	13.676	3928	3930	3934	rBV4	577	296	0.02%	0.002%


Sum of corrected areas: 13311992

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029782.D
Acq On : 23 Dec 2022 12:03
Operator : SY/MD
Sample : N6171-08ME
Misc : 4.96g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBQC6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

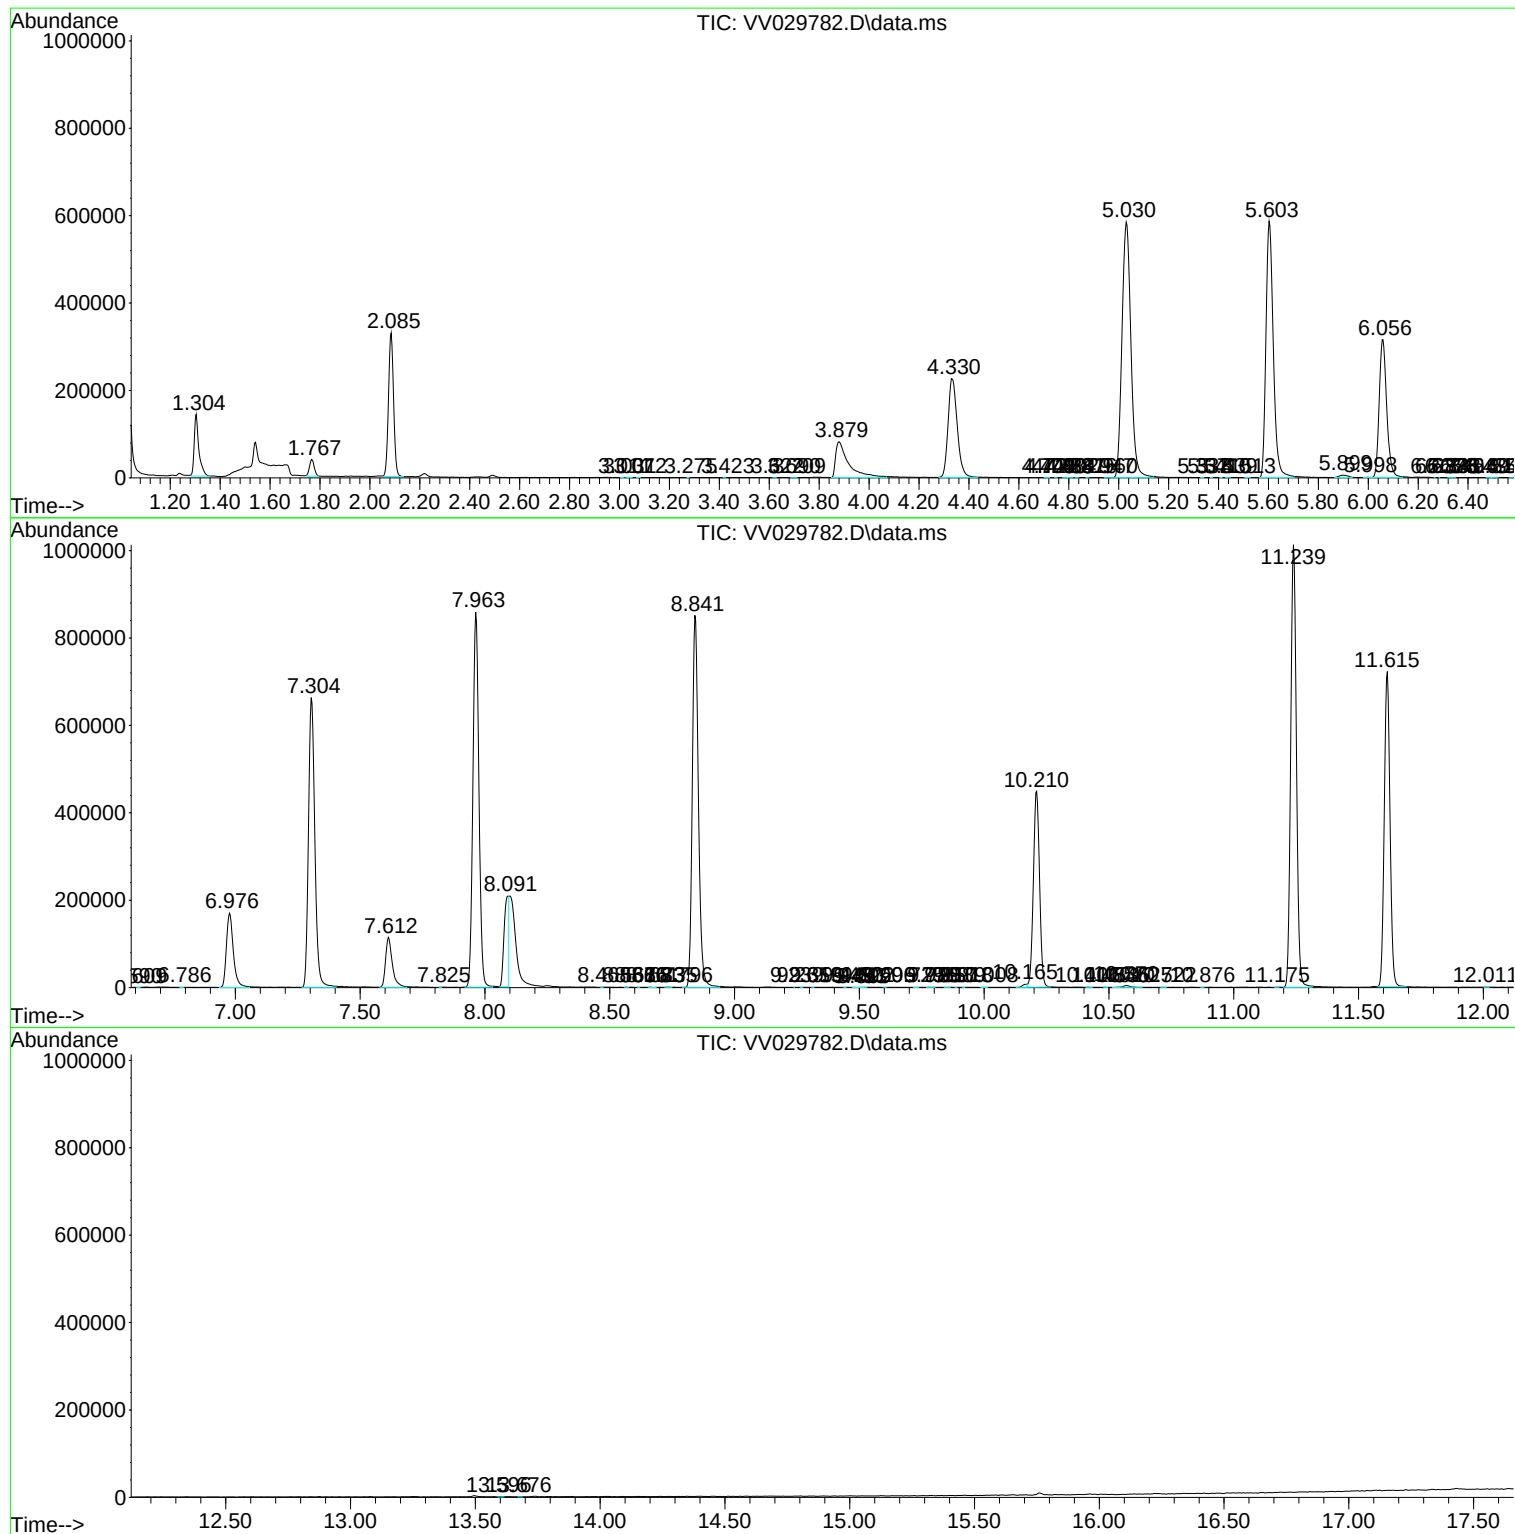

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029782.D
Acq On : 23 Dec 2022 12:03
Operator : SY/MD
Sample : N6171-08ME
Misc : 4.96g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBQC6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029782.D
Acq On : 23 Dec 2022 12:03
Operator : SY/MD
Sample : N6171-08ME
Misc : 4.96g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBQC6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc