
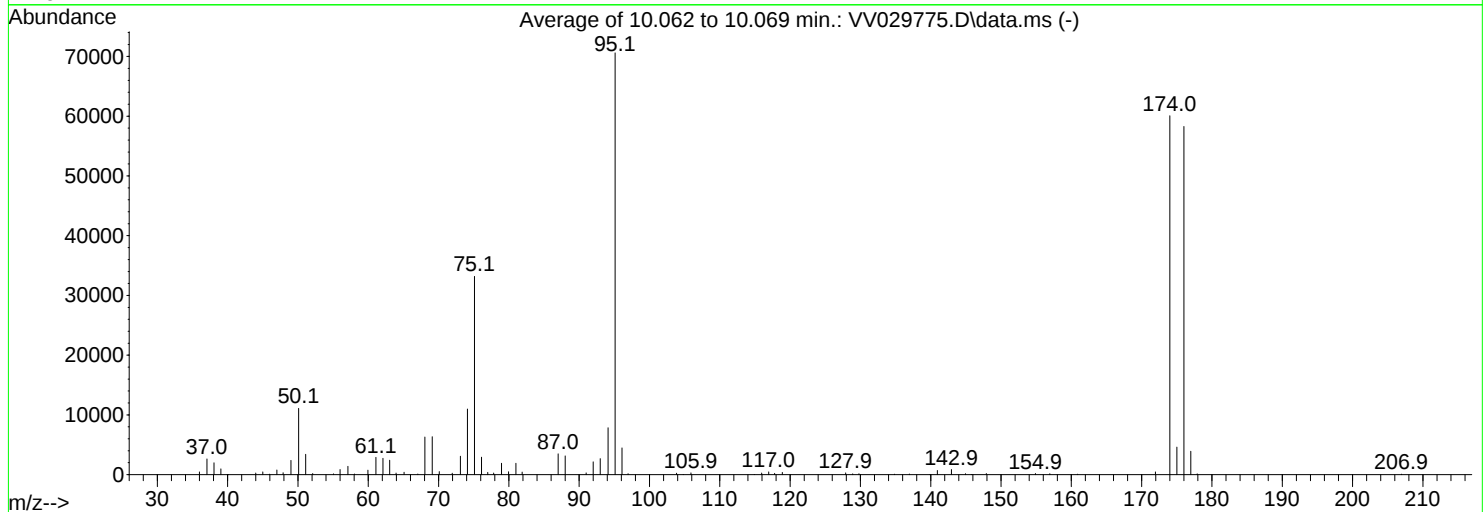


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122322\
Data File : VV029775.D
Acq On : 23 Dec 2022 08:54
Operator : SY/MD
Sample : BFB360
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB360

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Title : VOC Analysis
Last Update : Sat Dec 24 01:45:32 2022

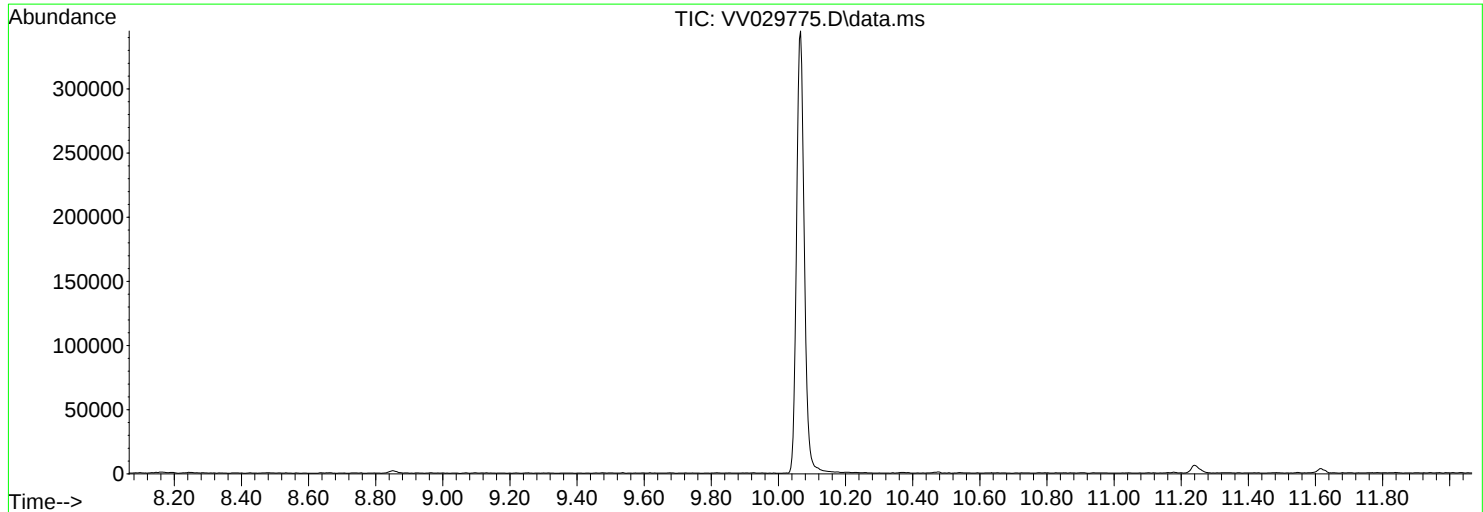

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	11101	PASS
75	95	30	80	47.0	33184	PASS
95	95	100	100	100.0	70603	PASS
96	95	5	9	6.3	4483	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.1	60085	PASS
175	174	5	9	7.7	4612	PASS
176	174	95	105	97.0	58291	PASS
177	176	5	10	6.7	3918	PASS

m/z	Abundance
40.00	280.0
44.00	401.0

Instrument :
MSVOA_V
ClientSampleId :
BFB360

m/z	Abundance
36.00	471.0
37.00	2674.0
38.10	2083.0
39.10	945.0
40.00	284.0
44.10	670.0
45.00	519.0
46.00	115.0
47.00	772.0
47.90	341.0
49.00	2328.0
50.10	11329.0
51.10	3562.0
52.10	192.0
55.00	116.0
56.00	921.0
57.10	1400.0
58.00	124.0
59.90	740.0
61.10	2999.0
62.10	2774.0
63.10	2420.0
64.00	260.0
65.10	401.0
67.10	206.0
68.00	6272.0
69.10	6539.0
70.10	513.0
72.10	286.0
73.10	2970.0
74.10	11482.0
75.10	33640.0
76.10	3110.0
77.00	394.0
77.90	297.0
79.00	1886.0
80.00	459.0
81.00	2014.0
81.90	440.0
87.00	3523.0
88.00	3028.0
91.00	356.0
92.00	2217.0
93.00	2821.0
94.10	7911.0
95.10	72312.0
96.10	4732.0
96.90	154.0
103.90	279.0
104.80	109.0
105.90	264.0
114.90	102.0
115.90	292.0
116.90	497.0
117.80	201.0
118.90	419.0
127.90	232.0
128.90	150.0
129.80	196.0
137.00	125.0
139.90	102.0
141.00	709.0
142.90	913.0
145.00	158.0
145.80	108.0
147.80	181.0
154.90	171.0
156.90	158.0
171.90	392.0
174.00	60648.0
175.00	4761.0
176.00	57432.0
177.00	4080.0
177.90	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB360

m/z	Abundance
36.00	465.0
37.10	2759.0
38.10	2058.0
39.10	1016.0
40.00	289.0
44.00	650.0
45.00	479.0
45.90	109.0
47.00	814.0
47.90	331.0
49.00	2442.0
50.10	11528.0
51.10	3501.0
52.10	189.0
55.00	134.0
56.00	894.0
57.10	1439.0
58.00	130.0
60.00	781.0
61.10	2990.0
62.10	2840.0
63.00	2528.0
63.90	268.0
65.10	400.0
68.00	6555.0
69.10	6572.0
70.10	527.0
71.90	242.0
73.10	3205.0
74.10	11371.0
75.10	34200.0
76.10	3010.0
77.00	378.0
77.80	269.0
79.00	1948.0
79.90	498.0
81.00	1949.0
81.90	450.0
87.00	3577.0
88.00	3274.0
91.00	319.0
92.00	2270.0
93.00	2730.0
94.10	8131.0
95.10	72784.0
96.10	4559.0
97.00	151.0
103.90	248.0
105.90	294.0
115.90	276.0
116.90	463.0
117.80	228.0
118.90	388.0
127.90	313.0
128.90	134.0
129.80	164.0
134.90	104.0
136.90	120.0
140.90	723.0
142.90	910.0
144.90	160.0
147.90	185.0
154.90	195.0
156.90	166.0
160.90	127.0
172.00	462.0
174.00	62024.0
175.00	4745.0
176.00	60384.0
177.00	4066.0
177.90	141.0
206.90	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB360

m/z	Abundance
36.00	427.0
37.10	2446.0
38.00	1827.0
39.00	915.0
39.90	290.0
44.00	662.0
45.00	411.0
47.00	787.0
47.90	288.0
49.00	2350.0
50.10	10445.0
51.10	3176.0
52.10	173.0
55.10	154.0
56.00	797.0
57.10	1338.0
58.10	103.0
60.00	764.0
61.10	2660.0
62.10	2560.0
63.10	2284.0
63.90	265.0
65.10	389.0
67.00	163.0
68.10	6063.0
69.10	5902.0
70.10	503.0
71.90	227.0
73.10	3074.0
74.10	10117.0
75.10	31712.0
76.10	2666.0
77.00	361.0
77.80	214.0
78.90	1888.0
80.00	464.0
81.00	1741.0
81.90	412.0
87.00	3337.0
88.00	3102.0
91.00	250.0
92.00	1990.0
93.00	2456.0
94.10	7487.0
95.10	66712.0
96.10	4157.0
97.00	178.0
103.80	238.0
105.90	295.0
116.00	222.0
117.00	393.0
117.80	243.0
118.90	350.0
127.90	340.0
128.90	115.0
129.80	161.0
134.80	130.0
136.90	116.0
140.90	702.0
143.00	791.0
144.90	151.0
146.00	113.0
148.00	180.0
154.90	163.0
157.00	159.0
160.90	156.0
172.00	503.0
174.00	57584.0
175.00	4331.0
176.00	57056.0
177.00	3609.0
177.90	107.0
207.00	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB360