

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122421\
 Data File : VV024161.D
 Acq On : 24 Dec 2021 15:49
 Operator : SY/MD
 Sample : VV1223WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 24 16:07:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122421.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 24 15:33:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	7658	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	7502	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.261	152	4104	0.500	ug/L	0.02
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	5495	0.576	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	116.000%
4) 1,2-Dichloroethane-d4	5.042	65	3493	0.538	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	108.000%
7) 1,2-Dichloropropane-d6	6.068	67	4094	0.566	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	114.000%
8) Toluene-d8	7.317	98	10769	0.528	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	106.000%
10) 1,1,2,2-Tetrachloroeth...	10.216	84	2522	0.550	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	110.000%
Target Compounds						
					Qvalue	
6) Trichloroethene	5.925	95	76	0.011	ug/L #	80
9) 1,2-Dibromoethane	8.415	107	63	0.014	ug/L #	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122421\
Data File : VV024161.D
Acq On : 24 Dec 2021 15:49
Operator : SY/MD
Sample : VV1223WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 24 16:07:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122421.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 24 15:33:30 2021
Response via : Initial Calibration

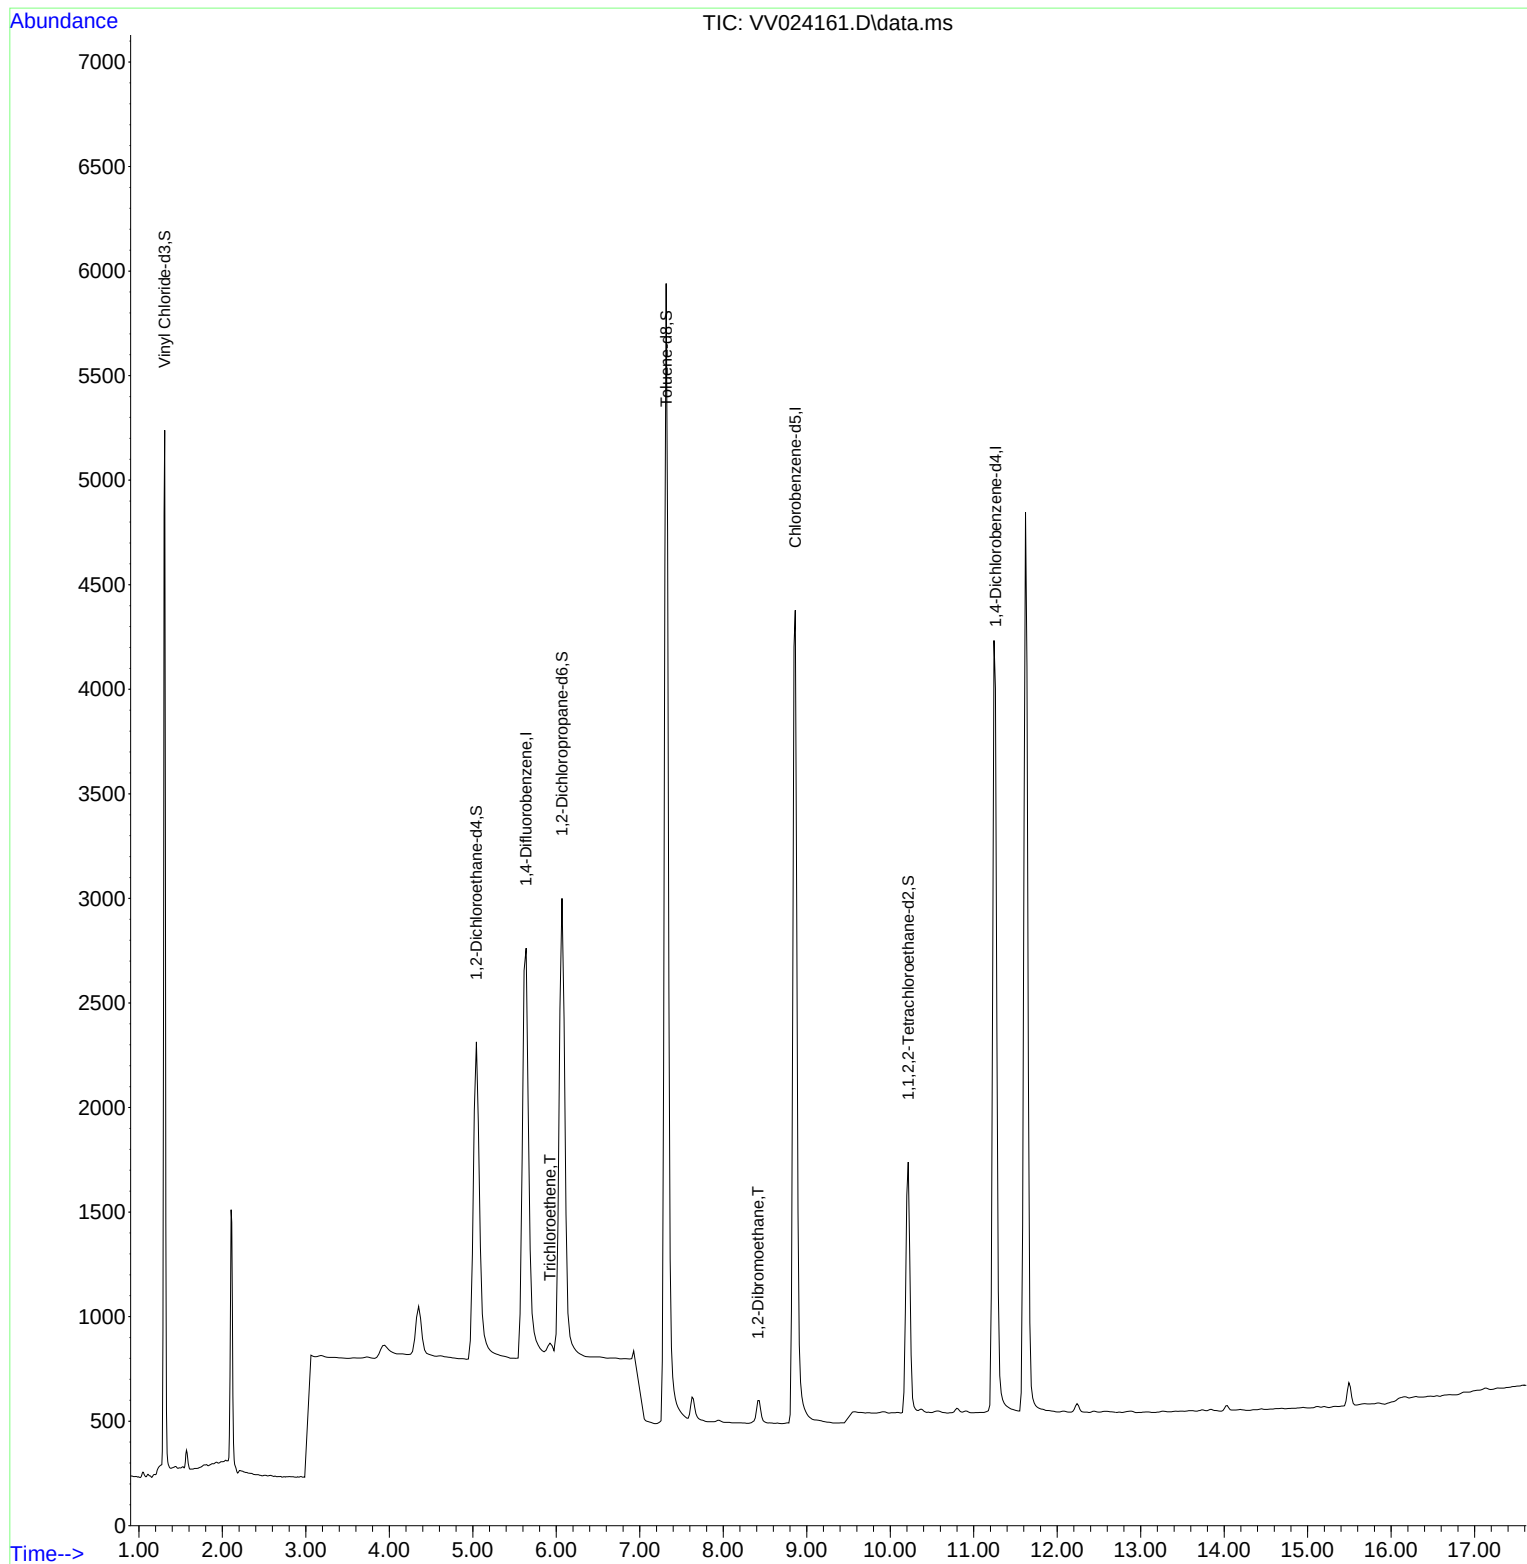

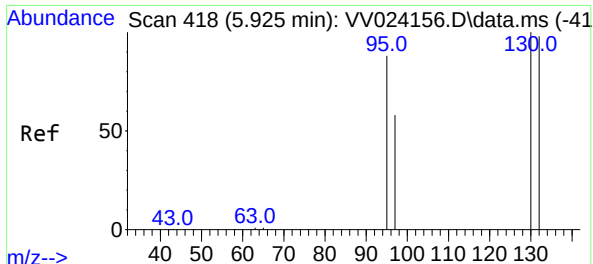




#6
 Trichloroethene
 Concen: 0.011 ug/L
 RT: 5.925 min Scan# 418
 Delta R.T. 0.000 min
 Lab File: VV024161.D
 Acq: 24 Dec 2021 15:49

Instrument :
 MSVOA_V
 ClientSampleId :

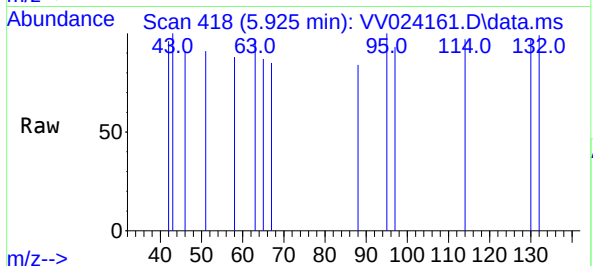

Tgt Ion: 95 Resp: 76

Ion	Ratio	Lower	Upper
95	100		
97	92.5	47.9	89.1#
132	98.5	79.9	148.3
130	97.0	82.4	153.0

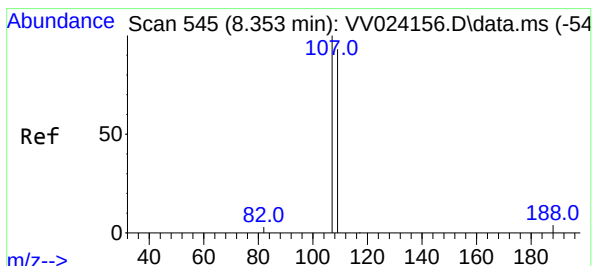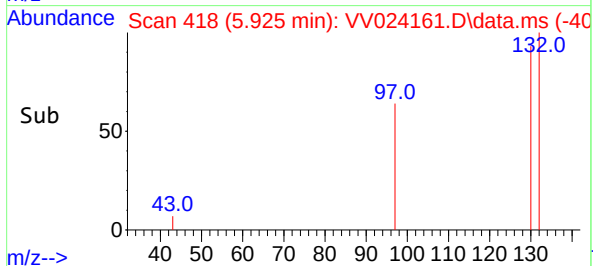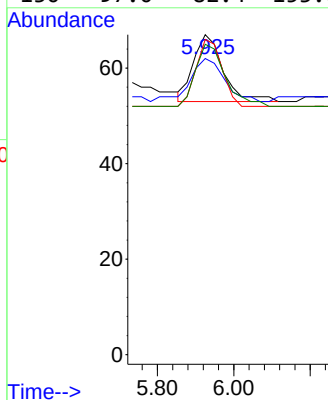

#9
 1,2-Dibromoethane
 Concen: 0.014 ug/L
 RT: 8.415 min Scan# 549
 Delta R.T. 0.062 min
 Lab File: VV024161.D
 Acq: 24 Dec 2021 15:49

Tgt Ion: 107 Resp: 63

Ion	Ratio	Lower	Upper
107	100		
109	87.1	64.7	120.1
188	82.3	10.0	15.0#

