

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122421\
 Data File : VV024169.D
 Acq On : 24 Dec 2021 19:23
 Operator : SY/MD
 Sample : M5152-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 24 21:47:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122421.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 24 15:33:30 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	9734	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	9437	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.244	152	5027	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	4653	0.384	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	76.000%		
4) 1,2-Dichloroethane-d4	5.042	65	3881	0.470	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	94.000%		
7) 1,2-Dichloropropane-d6	6.068	67	4540	0.499	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	100.000%		
8) Toluene-d8	7.317	98	11665	0.454	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	90.000%		
10) 1,1,2,2-Tetrachloroeth...	10.216	84	2808	0.487	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	98.000%		
Target Compounds						
13) 1,2-Dibromo-3-chloropr...	12.238	75	117	0.141	ug/L	Qvalue # 45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122421\
Data File : VV024169.D
Acq On : 24 Dec 2021 19:23
Operator : SY/MD
Sample : M5152-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 24 21:47:50 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122421.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 24 15:33:30 2021
Response via : Initial Calibration

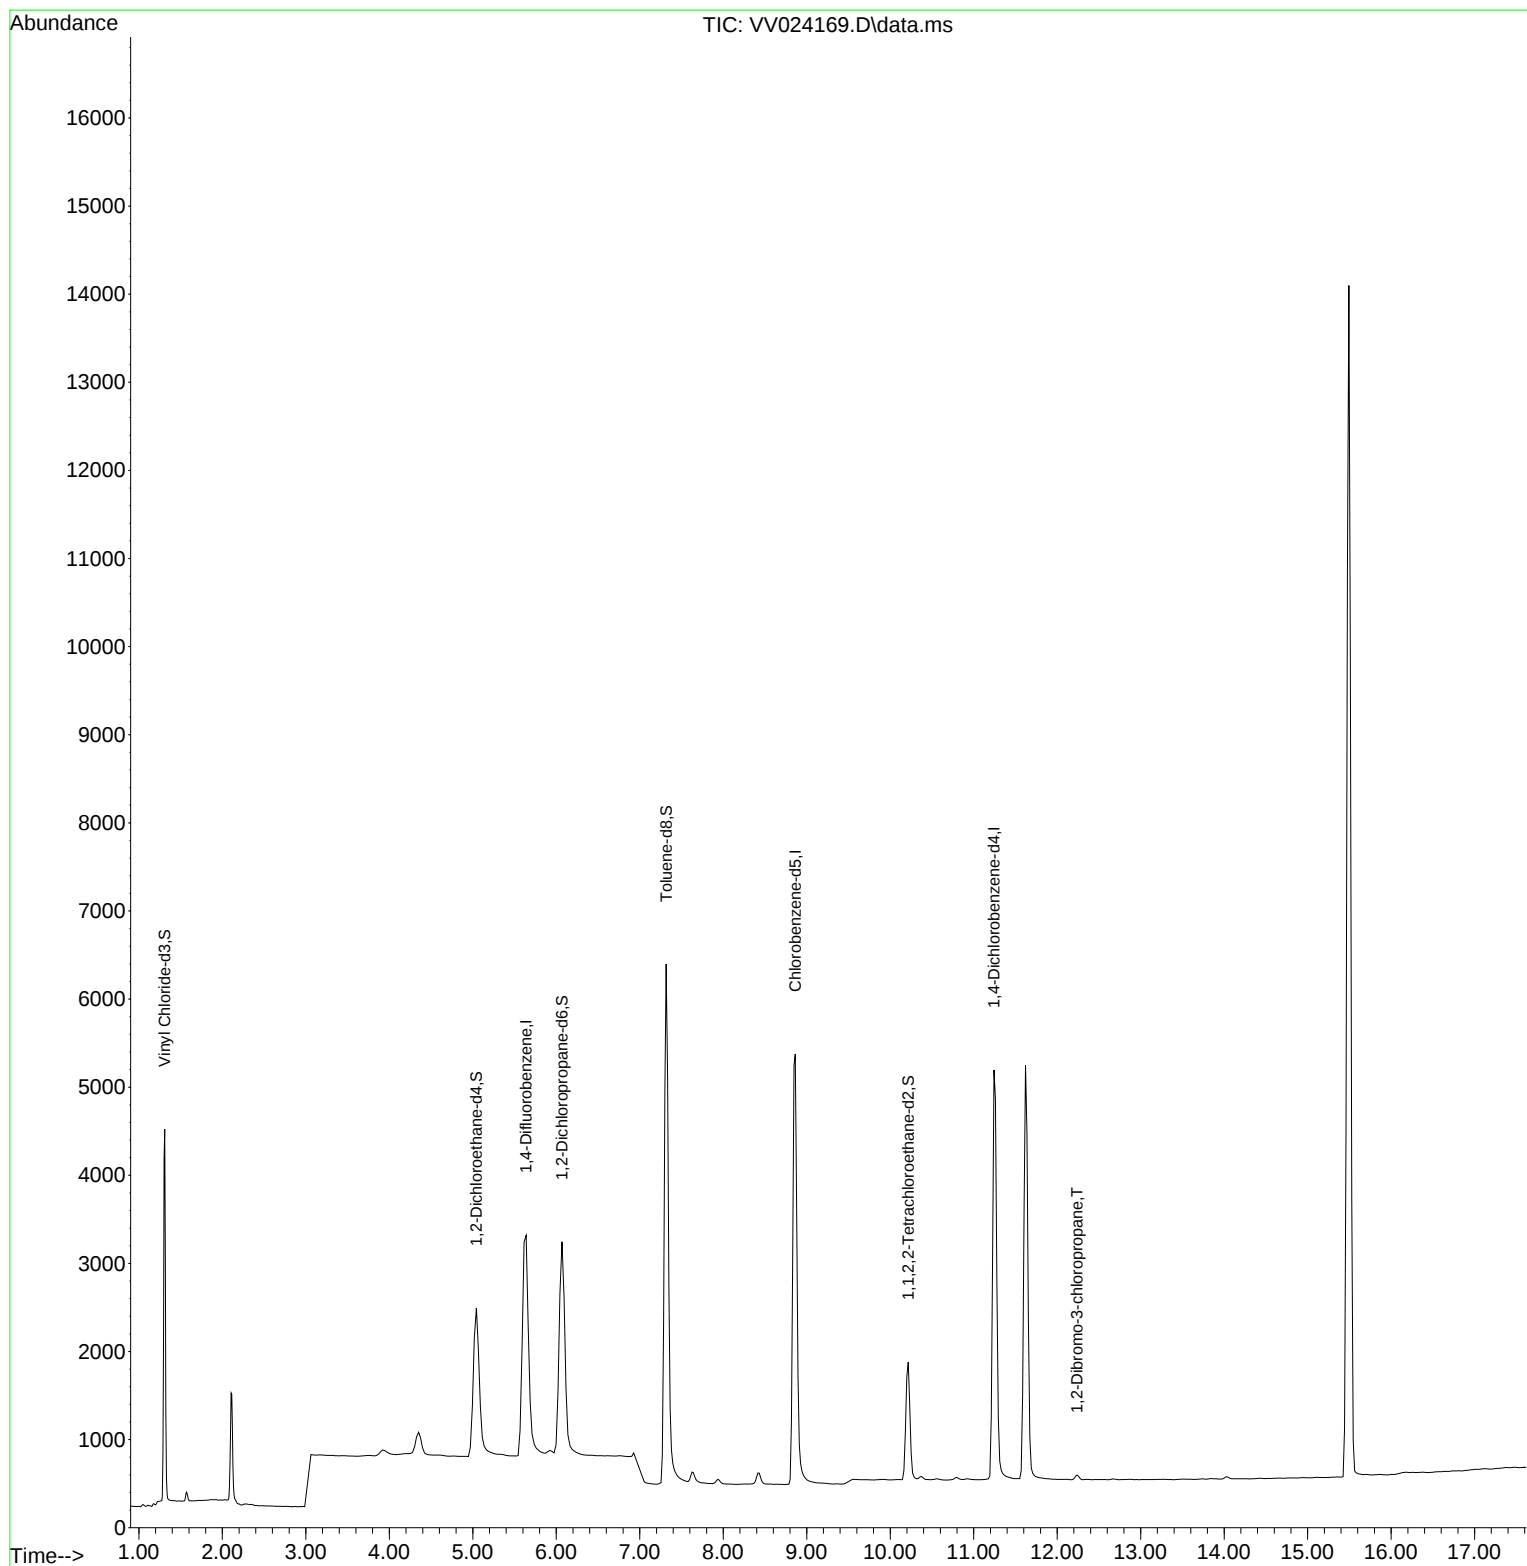

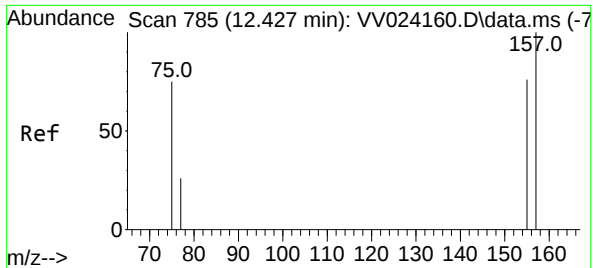

#13
 1,2-Dibromo-3-chloropropane
 Concen: 0.141 ug/L
 RT: 12.238 min Scan# 71
 Delta R.T. -0.188 min
 Lab File: VV024169.D
 Acq: 24 Dec 2021 19:23

Instrument :
 MSVOA_V
 ClientSampleId :

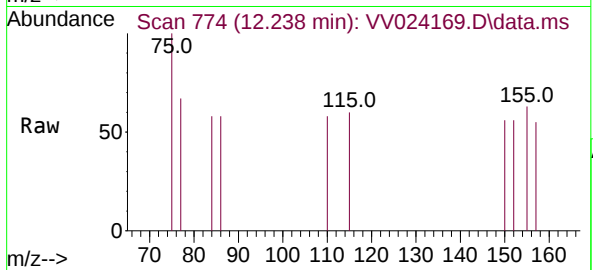

Tgt Ion:	75	Resp:	117
Ion	Ratio	Lower	Upper
75	100		
157	54.7	102.9	154.3#
155	63.2	87.6	131.4#

