
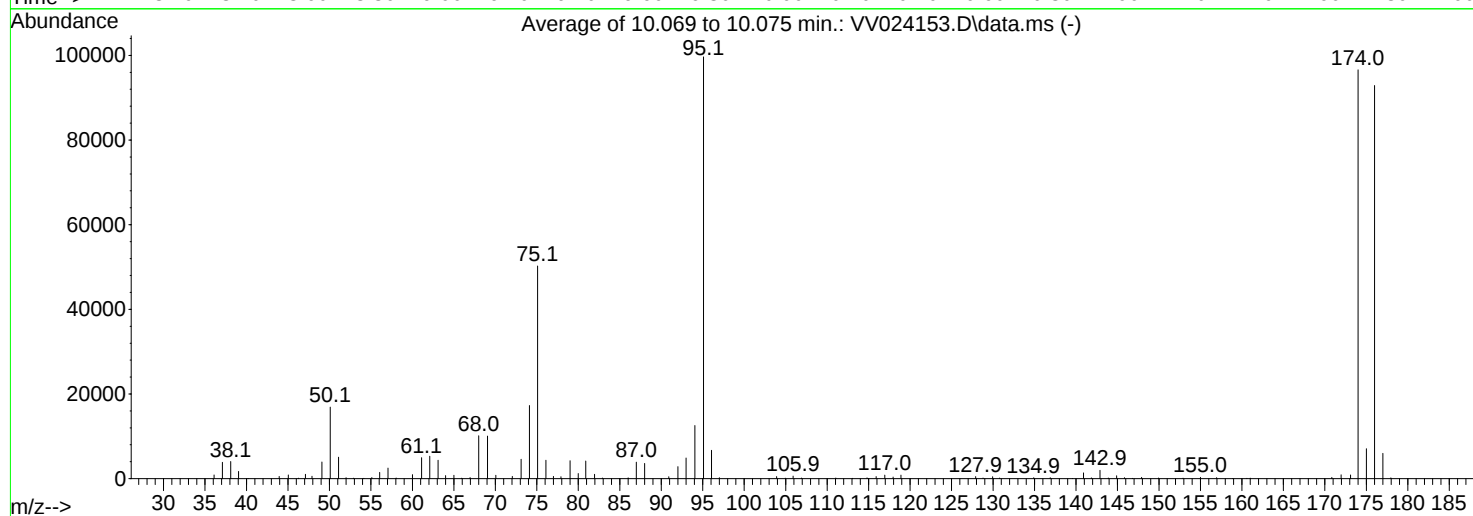


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122421\
 Data File : VV024153.D
 Acq On : 24 Dec 2021 09:02
 Operator : SY/MD
 Sample : BFB210
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB210

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM122421.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Dec 24 15:33:30 2021

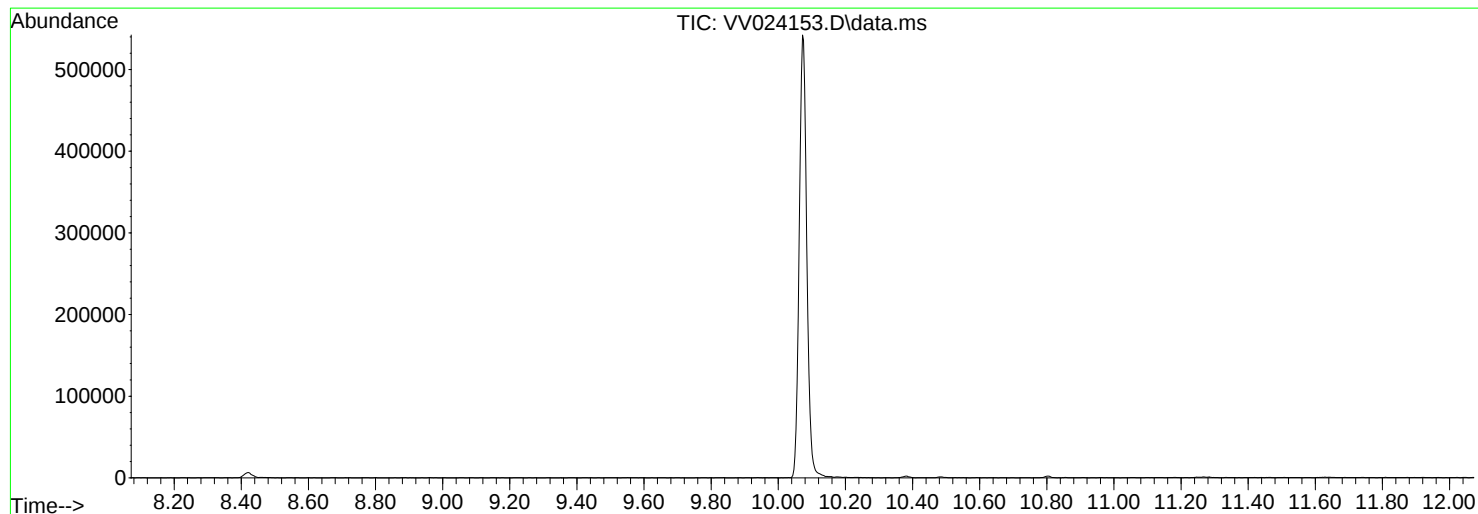

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	16913	PASS
75	95	30	80	50.4	50253	PASS
95	95	100	100	100.0	99664	PASS
96	95	5	9	6.7	6687	PASS
173	174	0.00	2	0.9	860	PASS
174	95	50	120	96.9	96600	PASS
175	174	5	9	7.3	7066	PASS
176	174	95	101	96.2	92893	PASS
177	176	5	9	6.4	5964	PASS

Scan 2796 (10.030 min): VV024153.D\data.ms
BFB210

m/z	Abundance
36.70	106.0
39.90	106.0
43.90	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
36.10	854.0
37.10	3690.0
38.10	3652.0
39.10	1590.0
40.00	143.0
44.00	622.0
45.10	843.0
46.30	110.0
47.10	979.0
47.90	529.0
49.10	3654.0
50.10	16116.0
51.10	4851.0
52.00	234.0
52.90	108.0
54.10	104.0
55.10	310.0
56.10	1494.0
57.10	2352.0
58.10	180.0
60.00	981.0
61.10	4747.0
62.10	4832.0
63.10	4035.0
64.00	705.0
65.00	713.0
65.90	109.0
67.00	243.0
68.00	9746.0
69.10	9325.0
70.10	816.0
72.10	503.0
73.10	4438.0
74.10	16126.0
75.10	46664.0
76.10	4122.0
77.00	608.0
77.90	496.0
79.00	3949.0
80.00	1228.0
80.90	3838.0
82.00	990.0
82.90	145.0
85.90	184.0
87.00	3749.0
88.00	3661.0
90.90	453.0
92.00	2708.0
93.00	4642.0
94.00	12020.0
95.10	94672.0
96.00	6529.0
97.00	190.0
103.90	442.0
104.90	110.0
105.90	563.0
106.90	151.0
111.10	153.0
114.80	170.0
115.90	418.0
117.00	875.0
118.00	305.0
118.90	754.0
127.90	492.0
128.80	140.0
130.00	460.0
130.80	141.0
134.90	218.0
136.90	201.0
139.60	109.0
140.90	1213.0
141.90	198.0
142.90	1899.0
143.90	127.0
144.90	604.0
145.90	166.0
147.90	334.0
150.00	120.0
152.90	125.0
155.10	285.0
156.90	181.0
158.90	103.0
160.60	102.0
161.00	104.0
170.80	290.0
172.00	855.0
173.10	1237.0
174.00	90312.0
175.00	6591.0
176.00	85944.0
177.00	5622.0
177.90	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
36.10	873.0
37.10	3948.0
38.10	4310.0
39.00	1789.0
44.00	696.0
45.00	883.0
46.20	159.0
47.10	972.0
47.90	624.0
49.10	4042.0
50.10	17040.0
51.10	5138.0
52.00	219.0
52.90	109.0
55.10	268.0
56.00	1416.0
57.00	2563.0
58.00	137.0
60.00	942.0
61.10	4951.0
62.10	5551.0
63.10	4549.0
64.00	706.0
65.00	801.0
66.00	102.0
66.90	272.0
68.00	10132.0
69.00	10375.0
70.00	801.0
72.00	551.0
73.10	4573.0
74.10	17824.0
75.10	52056.0
76.10	4424.0
77.00	442.0
77.90	374.0
79.00	4388.0
80.00	1194.0
80.90	4335.0
81.90	1029.0
82.90	136.0
86.10	188.0
87.00	3951.0
88.00	3360.0
90.90	461.0
92.00	2850.0
93.00	4980.0
94.10	12635.0
95.10	101264.0
96.10	6604.0
97.00	257.0
103.90	559.0
105.00	138.0
105.90	612.0
106.90	164.0
111.00	148.0
113.00	117.0
114.80	166.0
115.90	541.0
116.90	784.0
118.00	439.0
118.90	890.0
127.90	436.0
128.80	191.0
129.90	458.0
130.80	142.0
134.90	258.0
136.90	235.0
140.90	1438.0
141.80	213.0
142.90	2005.0
143.90	140.0
144.90	755.0
145.80	262.0
146.80	134.0
147.90	284.0
149.90	173.0
152.90	125.0
154.90	324.0
157.00	234.0
161.00	144.0
170.90	315.0
171.90	954.0
174.00	99592.0
175.00	7336.0
176.00	96704.0
177.00	6092.0
178.00	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
36.10	918.0
37.10	3990.0
38.10	4139.0
39.10	1718.0
40.20	111.0
44.00	705.0
45.00	946.0
46.20	126.0
47.10	1103.0
47.90	606.0
49.10	4084.0
50.10	17584.0
51.10	5254.0
52.00	219.0
52.90	114.0
54.20	108.0
55.10	271.0
56.10	1513.0
57.00	2534.0
58.00	174.0
60.00	968.0
61.10	5173.0
62.10	5476.0
63.10	4500.0
64.00	749.0
65.00	833.0
66.00	110.0
66.90	263.0
68.00	10470.0
69.00	10478.0
70.10	821.0
72.00	526.0
73.10	4672.0
74.10	17936.0
75.10	52040.0
76.10	4493.0
77.00	553.0
77.90	461.0
79.00	4347.0
80.00	1263.0
80.90	4329.0
81.90	1083.0
82.90	132.0
86.00	165.0
87.00	4041.0
88.00	3726.0
90.90	502.0
92.00	2936.0
93.00	5073.0
94.10	12974.0
95.10	103056.0
96.00	6929.0
97.00	244.0
103.90	522.0
105.00	124.0
105.90	638.0
106.90	164.0
111.00	155.0
113.10	102.0
114.80	185.0
115.90	525.0
116.90	874.0
117.90	382.0
118.90	878.0
127.90	502.0
128.80	149.0
129.90	465.0
130.80	162.0
134.90	255.0
136.90	225.0
140.90	1468.0
141.80	203.0
142.90	2046.0
143.90	144.0
144.90	734.0
145.80	234.0
146.80	103.0
147.90	339.0
149.90	154.0
152.90	134.0
155.00	313.0
157.00	222.0
160.60	119.0
161.00	137.0
170.80	331.0
172.00	909.0
173.10	1344.0
174.00	99896.0
175.00	7272.0
176.00	96032.0
177.00	6179.0
178.00	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210