

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122719\
 Data File : VV014205.D
 Acq On : 27 Dec 2019 21:07
 Operator : SY/MD
 Sample : VIBLK35
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK35

Quant Time: Dec 28 17:33:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Dec 28 01:05:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	884496	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	808105	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	377683	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	180116	4.34	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.80%
7) Chloroethane-d5	1.58	69	165220	4.79	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.80%
11) 1,1-Dichloroethene-d2	2.13	63	240106	3.23	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.60%
20) 2-Butanone-d5	3.92	46	581433	56.50	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.00%
24) Chloroform-d	4.40	84	427964	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.40%
26) 1,2-Dichloroethane-d4	5.08	65	219153	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.40%
32) Benzene-d6	5.10	84	905428	4.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.00%
36) 1,2-Dichloropropane-d6	6.12	67	280535	4.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.00%
41) Toluene-d8	7.36	98	825183	4.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.00%
43) trans-1,3-Dichloropropene-	7.66	79	117126	3.92	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.40%
46) 2-Hexanone-d5	8.13	63	524304	46.24	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.48%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	202441	4.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	280664	4.15	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	83.00%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	12679	0.193 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV122719\
Data File : VV014205.D
Acq On : 27 Dec 2019 21:07
Operator : SY/MD
Sample : VIBLK35
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK35

Quant Time: Dec 28 17:33:21 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Dec 28 01:05:52 2019
Response via : Initial Calibration

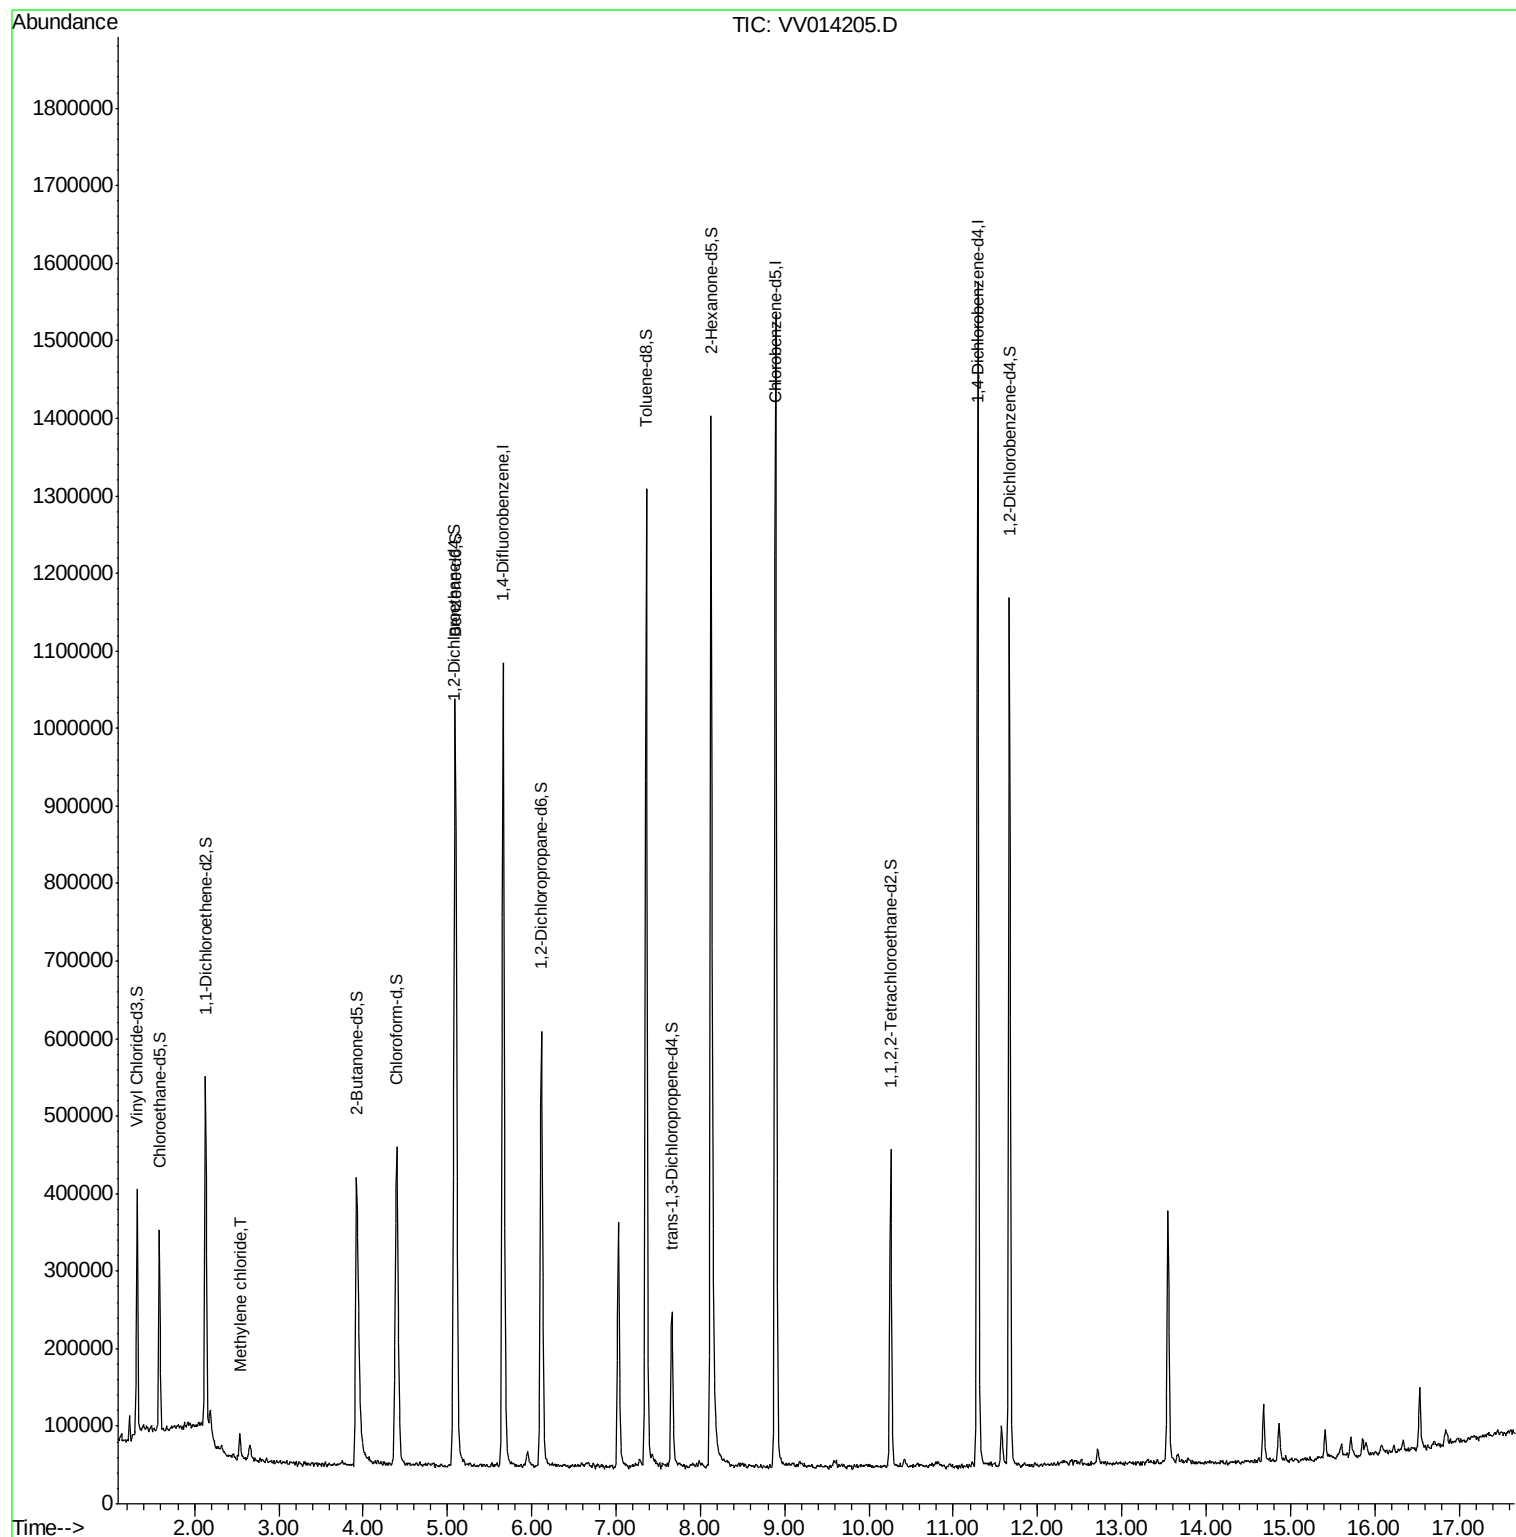

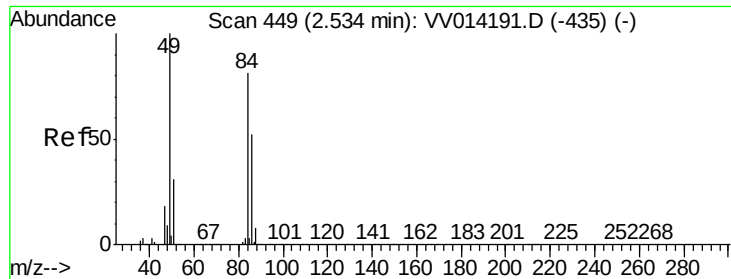

#16
 Methvlene chloride
 Concen: 0.193 ug/L
 RT: 2.54 min Scan# 450
 Delta R.T. 0.00 min
 Lab File: VV014205.D
 Acq: 27 Dec 2019 21:07

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK35

Tot Ion	Ratio	Lower	Upper
84	100		
86	70.2	43.1	80.1
49	117.8	82.1	152.5

