

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122721\
 Data File : VW024186.D
 Acq On : 27 Dec 2021 17:51
 Operator : SY/MD
 Sample : M5126-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J19

Quant Time: Dec 28 05:51:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Dec 28 05:23:55 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	149947	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	153521	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	78442	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	41591	3.688	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	73.800%	
7) Chloroethane-d5	1.568	69	36515	3.882	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	77.600%	
11) 1,1-Dichloroethene-d2	2.108	63	62826	2.292	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	45.800%#	
20) 2-Butanone-d5	3.905	46	66103	52.764	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	105.520%	
24) Chloroform-d	4.349	84	94530	3.948	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	79.000%	
26) 1,2-Dichloroethane-d4	5.034	65	46323	4.322	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.400%	
32) Benzene-d6	5.050	84	183062	4.416	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.400%	
36) 1,2-Dichloropropane-d6	6.069	67	53536	4.714	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	94.200%	
41) Toluene-d8	7.317	98	162989	3.989	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.800%	
43) trans-1,3-Dichloroprop...	7.625	79	18411	3.829	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	76.600%	
46) 2-Hexanone-d5	8.088	63	78533	48.572	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	97.140%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	35618	4.594	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	65711	4.819	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.400%	
Target Compounds						
42) Toluene	7.394	91	11672	0.130	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024186.D
Acq On : 27 Dec 2021 17:51
Operator : SY/MD
Sample : M5126-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J19

Quant Time: Dec 28 05:51:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Dec 28 05:23:55 2021
Response via : Initial Calibration

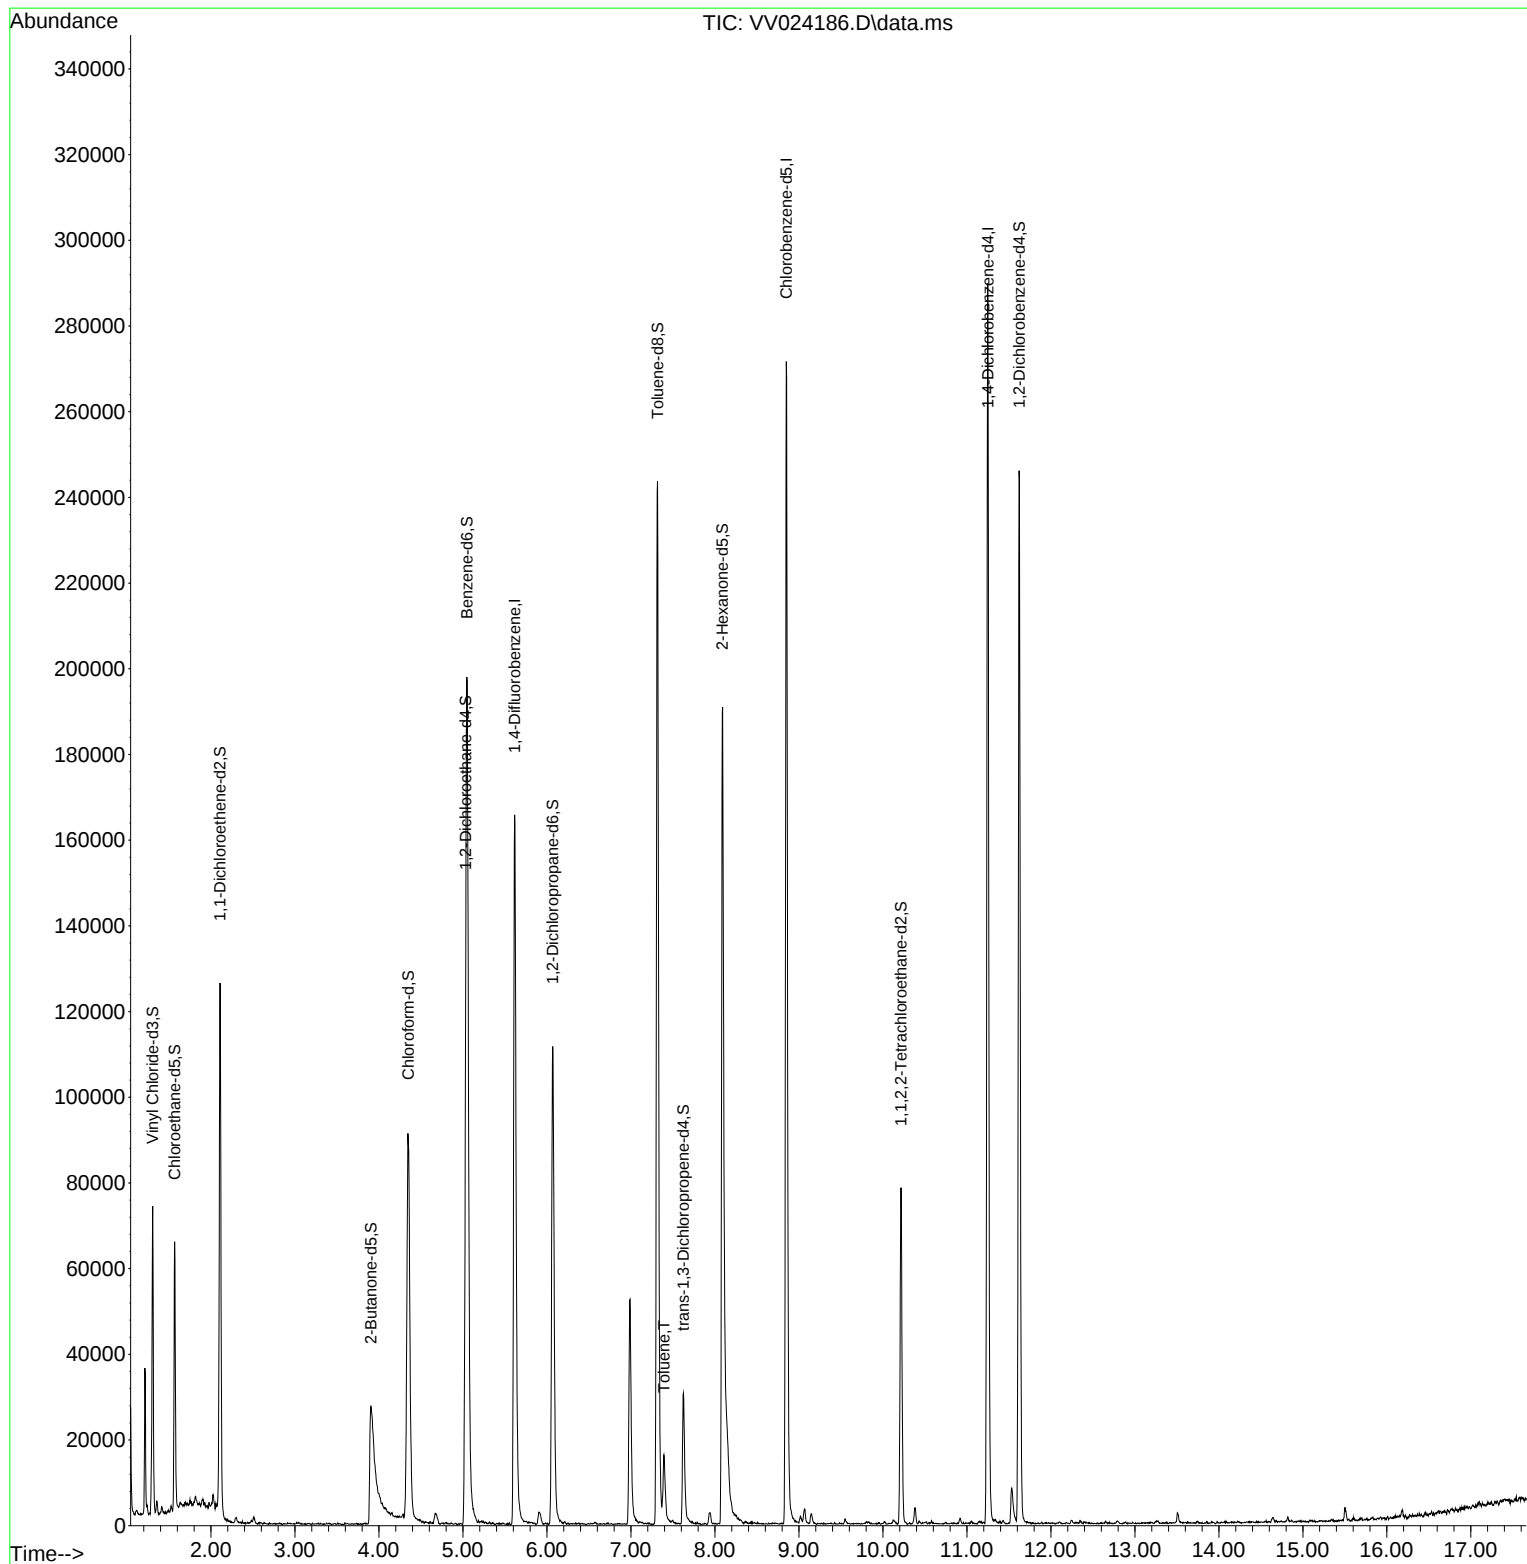

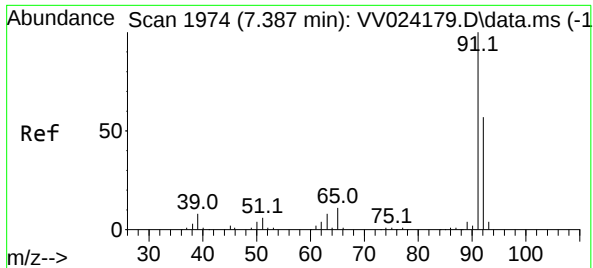

#42
Toluene
Concen: 0.130 ug/L
RT: 7.394 min Scan# 1976
Delta R.T. 0.006 min
Lab File: VV024186.D
Acq: 27 Dec 2021 17:51

Instrument :
MSVOA_V
ClientSampleId :
C0J19

Tgt Ion: 91 Resp: 11672
Ion Ratio Lower Upper
91 100
92 69.0 41.5 77.1

