

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
 Data File : VV024185.D
 Acq On : 27 Dec 2021 17:27
 Operator : SY/MD
 Sample : M5126-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	92	rBV2	79313	93195	18.10%	1.775%
2	1.359	94	99	105	rVB2	5452	5316	1.03%	0.101%
3	1.568	156	164	176	rBV	65534	79985	15.53%	1.523%
4	1.754	215	222	232	rVB	20768	28077	5.45%	0.535%
5	2.111	323	333	349	rVB	129126	192205	37.32%	3.660%
6	3.198	658	671	685	rVB2	3667	7661	1.49%	0.146%
7	3.905	875	891	930	rBV3	52771	200785	38.99%	3.823%
8	4.349	1013	1029	1057	rBV2	94260	231524	44.96%	4.409%
9	4.609	1094	1110	1129	rBV2	24829	62487	12.13%	1.190%
10	5.050	1229	1247	1277	rBV3	201590	514957	100.00%	9.805%
11	5.616	1411	1423	1454	rBV	173969	357478	69.42%	6.807%
12	5.918	1507	1517	1538	rVB4	14178	31620	6.14%	0.602%
13	6.069	1551	1564	1592	rBV	113787	237967	46.21%	4.531%
14	6.989	1837	1850	1871	rBV	55024	103915	20.18%	1.979%
15	7.316	1940	1952	1970	rBV	250577	438619	85.18%	8.352%
16	7.625	2039	2048	2070	rBV	31494	59943	11.64%	1.141%
17	7.976	2148	2157	2172	rVB2	24684	43112	8.37%	0.821%
18	8.088	2181	2192	2226	rBV	230962	431329	83.76%	8.213%
19	8.850	2419	2429	2451	rBV	279055	460686	89.46%	8.772%
20	9.146	2513	2521	2535	rVB3	3817	6370	1.24%	0.121%
21	10.213	2840	2853	2873	rBV	80417	128608	24.97%	2.449%
22	11.249	3164	3175	3196	rBV	313374	487796	94.73%	9.288%
23	11.532	3253	3263	3279	rBV7	11423	22801	4.43%	0.434%
24	11.622	3279	3291	3310	rVV	255476	415173	80.62%	7.905%
25	12.046	3414	3423	3434	rVB8	4639	7847	1.52%	0.149%
26	12.117	3434	3445	3453	rBV4	8633	14693	2.85%	0.280%
27	12.239	3475	3483	3494	rVV4	3990	6915	1.34%	0.132%
28	12.300	3494	3502	3515	rVB7	3794	7228	1.40%	0.138%
29	12.387	3521	3529	3536	rVB7	3656	5647	1.10%	0.108%
30	12.548	3573	3579	3589	rBV7	4402	5741	1.11%	0.109%
31	12.683	3614	3621	3629	rVB6	3285	5202	1.01%	0.099%
32	12.953	3698	3705	3713	rBV7	4218	6370	1.24%	0.121%
33	13.001	3713	3720	3727	rBV7	3705	6240	1.21%	0.119%
34	13.217	3778	3787	3793	rVB5	4542	6593	1.28%	0.126%
35	13.265	3793	3802	3809	rBV6	4523	6591	1.28%	0.126%
36	13.332	3809	3823	3833	rBV6	11013	26040	5.06%	0.496%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122721\
 Data File : VW024185.D
 Acq On : 27 Dec 2021 17:27
 Operator : SY/MD
 Sample : M5126-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
 Title : TRACE VOA SFAM1.0

37	13.487	3858	3871	3885	rBV6	13575	34747	6.75%	0.662%
38	13.609	3902	3909	3923	rVB5	10077	17344	3.37%	0.330%
39	13.709	3932	3940	3952	rBV7	12664	23835	4.63%	0.454%
40	13.779	3954	3962	3971	rVB4	6666	12022	2.33%	0.229%
41	13.908	3992	4002	4014	rVB5	10259	20563	3.99%	0.392%
42	14.014	4023	4035	4048	rBV5	5115	10212	1.98%	0.194%
43	14.088	4048	4058	4073	rBV5	20342	45012	8.74%	0.857%
44	14.229	4093	4102	4112	rVB6	14614	24235	4.71%	0.461%
45	14.300	4112	4124	4135	rVB5	27862	52398	10.18%	0.998%
46	14.361	4135	4143	4157	rVB7	11271	20096	3.90%	0.383%
47	14.448	4159	4170	4180	rBV3	15422	30632	5.95%	0.583%
48	14.570	4201	4208	4214	rBV7	8956	13274	2.58%	0.253%
49	14.615	4214	4222	4226	rBV6	11734	18903	3.67%	0.360%
50	14.686	4236	4244	4258	rVB8	16808	42227	8.20%	0.804%
51	14.760	4258	4267	4275	rBV4	13942	23752	4.61%	0.452%
52	14.827	4276	4288	4297	rVB6	12370	23624	4.59%	0.450%
53	14.876	4297	4303	4310	rBV7	5209	8817	1.71%	0.168%
54	15.339	4434	4447	4461	rVB5	13396	33882	6.58%	0.645%
55	15.422	4461	4473	4484	rBV5	7824	14220	2.76%	0.271%
56	15.503	4491	4498	4507	rBV8	4549	7926	1.54%	0.151%
57	15.564	4507	4517	4520	rVV8	4924	8006	1.55%	0.152%
58	15.586	4520	4524	4533	rVB6	8269	12282	2.39%	0.234%
59	16.184	4701	4710	4718	rVB6	4431	7002	1.36%	0.133%


Sum of corrected areas: 5251727

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024185.D
Acq On : 27 Dec 2021 17:27
Operator : SY/MD
Sample : M5126-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

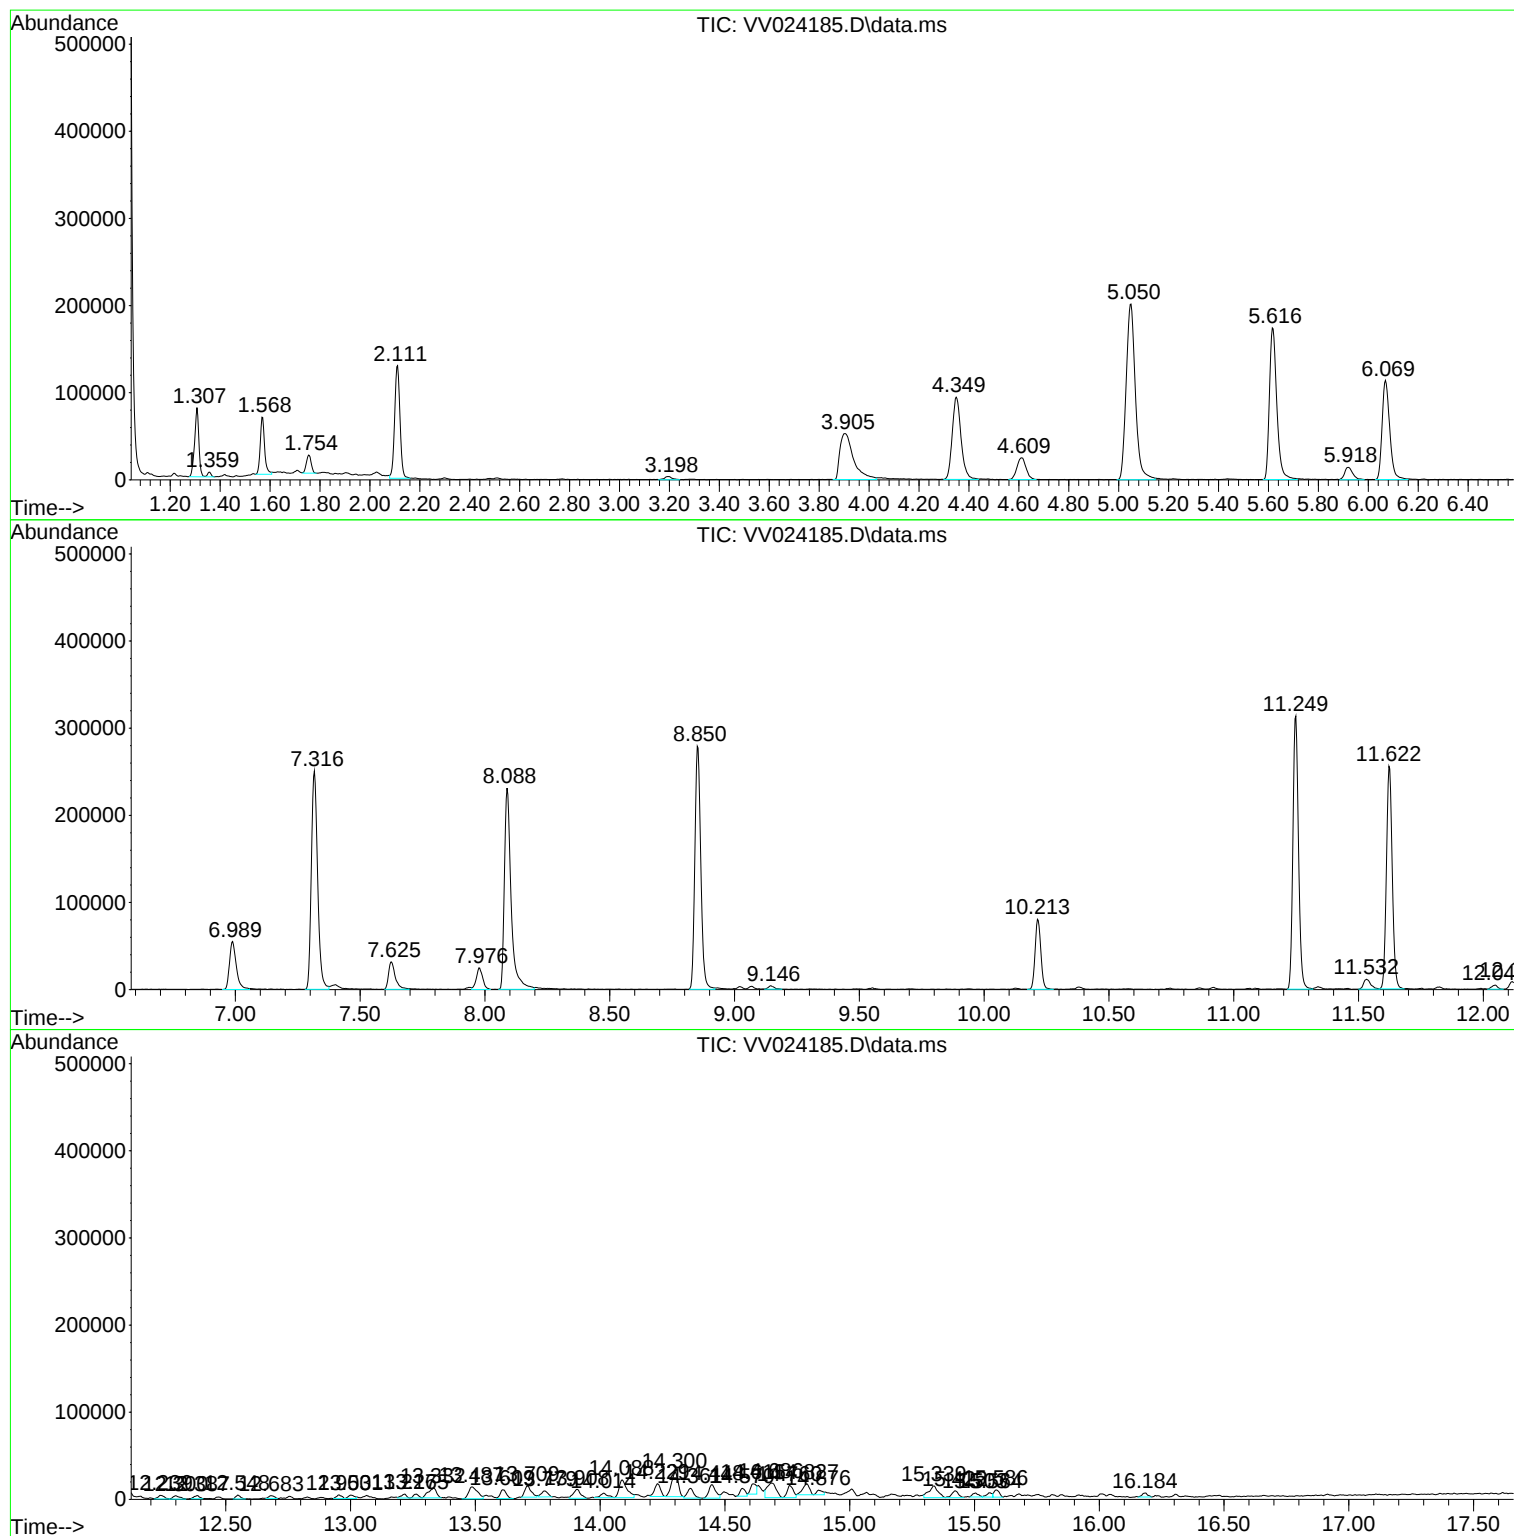

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024185.D
Acq On : 27 Dec 2021 17:27
Operator : SY/MD
Sample : M5126-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J10










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1H-Indene, 2,3-dihydro-1,1,... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.300	0.54 ug/L	52398	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1H-Indene, 2,3-dihydro-1,1,3-tri...	160	C12H16	002613-76-5	90
2			Benzene, 1-(1-methylethenyl)-2-(...	160	C12H16	005557-93-7	89
3			Benzene, 4-(2-butenyl)-1,2-dimet...	160	C12H16	054340-86-2	81
4			Benzene, 1-(2-butenyl)-2,3-dimet...	160	C12H16	054340-85-1	76
5			1H-Indene, 2,3-dihydro-4,5,7-tri...	160	C12H16	006682-06-0	76

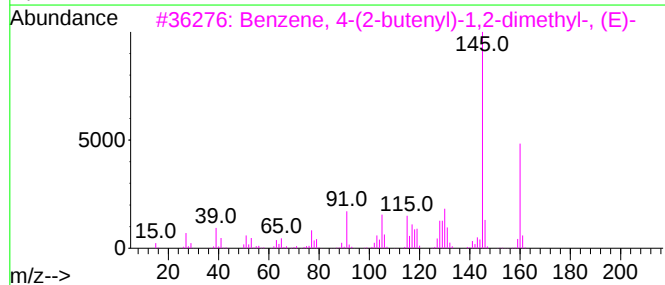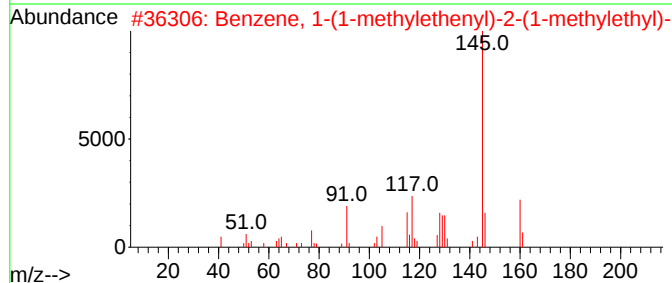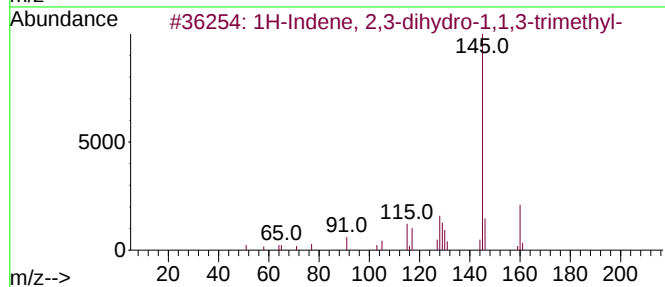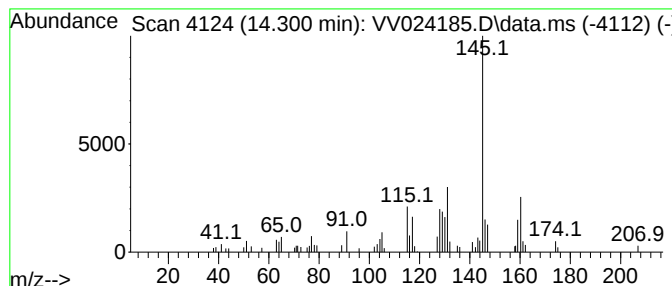

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024185.D
Acq On : 27 Dec 2021 17:27
Operator : SY/MD
Sample : M5126-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J10

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1H-Indene, 2,3-...	14.300	0.5	ug/L	52398	3	11.249	487796	5.0