

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
 Data File : VV024187.D
 Acq On : 27 Dec 2021 18:15
 Operator : SY/MD
 Sample : M5126-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J27

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024187.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	94	rBV	68113	75655	15.60%	1.876%
2	1.568	156	164	174	rBV	60391	69028	14.23%	1.711%
3	2.108	321	332	347	rVB	118081	172410	35.54%	4.275%
4	3.915	881	894	921	rBV	24649	104896	21.62%	2.601%
5	4.352	1013	1030	1056	rBV2	87607	218359	45.01%	5.414%
6	5.047	1230	1246	1275	rBV2	192172	485104	100.00%	12.028%
7	5.616	1412	1423	1447	rBV2	161081	331758	68.39%	8.226%
8	5.908	1506	1514	1527	rBV7	3125	6063	1.25%	0.150%
9	6.069	1550	1564	1586	rBV	109099	227334	46.86%	5.636%
10	6.989	1839	1850	1869	rBV	50439	95008	19.59%	2.356%
11	7.317	1939	1952	1969	rBV	232367	407620	84.03%	10.106%
12	7.397	1970	1977	1985	rVB2	6207	10752	2.22%	0.267%
13	7.625	2039	2048	2071	rBV2	29358	54028	11.14%	1.340%
14	8.092	2182	2193	2234	rBV	176008	403177	83.11%	9.996%
15	8.850	2418	2429	2457	rBV	264278	430923	88.83%	10.684%
16	9.066	2489	2496	2511	rVB3	3368	5714	1.18%	0.142%
17	10.217	2841	2854	2873	rBV	74006	121594	25.07%	3.015%
18	10.378	2897	2904	2916	rVB5	4020	6376	1.31%	0.158%
19	11.249	3164	3175	3198	rBV	276641	433538	89.37%	10.749%
20	11.622	3280	3291	3316	rBV	239414	373948	77.09%	9.272%




Sum of corrected areas: 4033285

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024187.D
Acq On : 27 Dec 2021 18:15
Operator : SY/MD
Sample : M5126-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

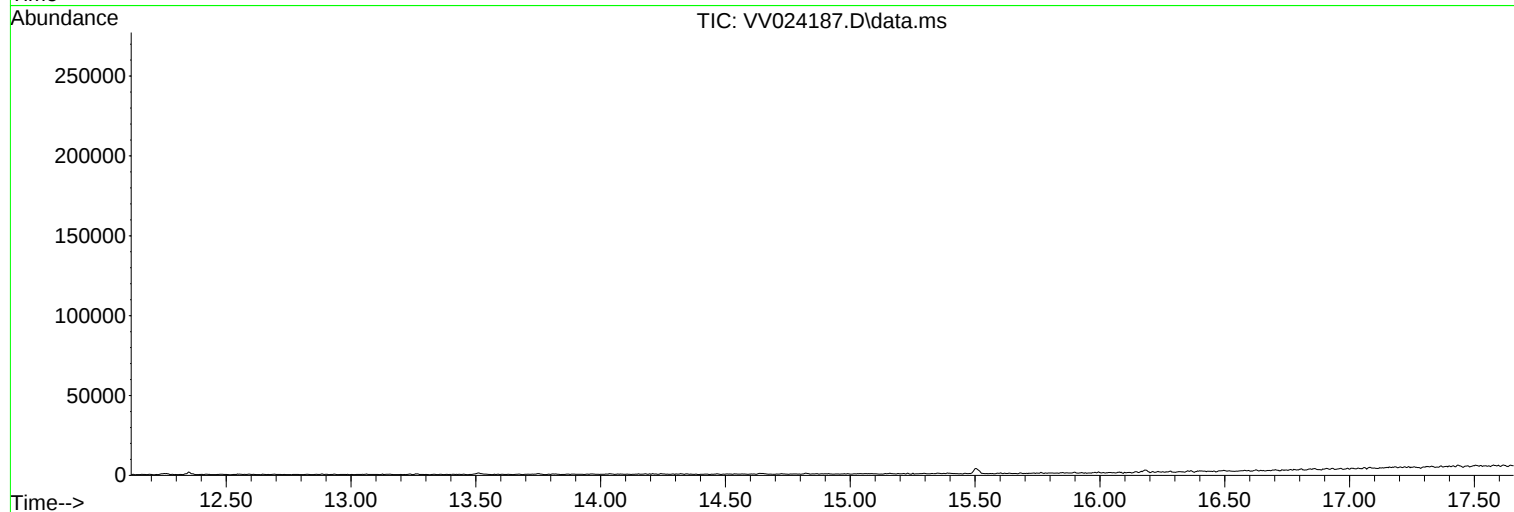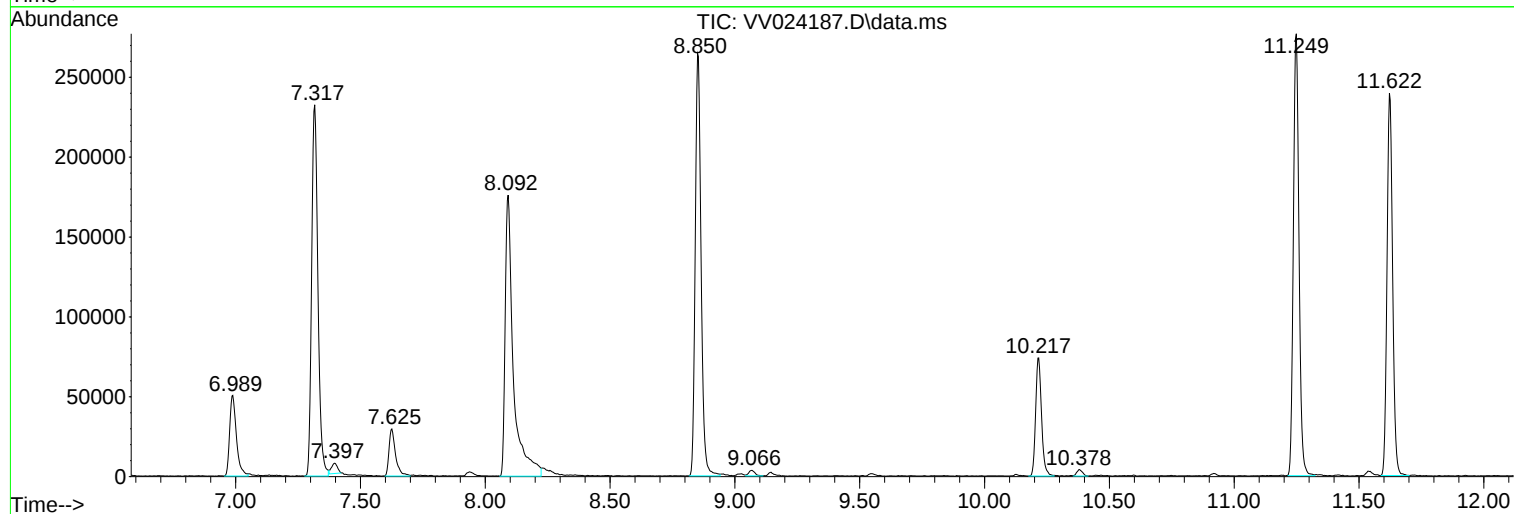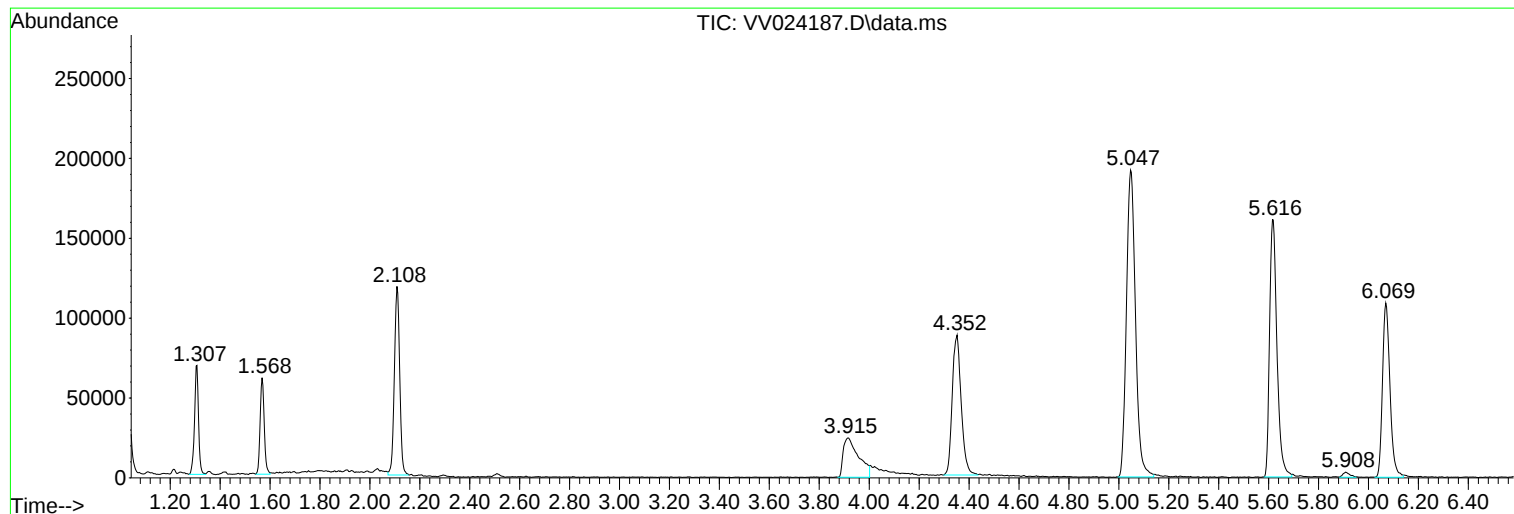

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024187.D
Acq On : 27 Dec 2021 18:15
Operator : SY/MD
Sample : M5126-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024187.D
Acq On : 27 Dec 2021 18:15
Operator : SY/MD
Sample : M5126-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
