

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
 Data File : VV024188.D
 Acq On : 27 Dec 2021 18:39
 Operator : SY/MD
 Sample : M5126-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J28

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024188.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	49	54	60	rBV	12226	11127	2.28%	0.279%
2	1.307	74	83	94	rVB	68834	69452	14.25%	1.741%
3	1.564	156	163	175	rVB	58706	65140	13.37%	1.633%
4	2.105	320	331	345	rBV	120343	169289	34.74%	4.243%
5	3.925	884	897	928	rBV	25910	122883	25.22%	3.080%
6	4.349	1013	1029	1057	rBV	89938	217732	44.68%	5.458%
7	5.047	1229	1246	1275	rBV2	197614	487275	100.00%	12.214%
8	5.616	1412	1423	1450	rBV	152836	314722	64.59%	7.889%
9	5.908	1506	1514	1527	rVB4	2725	5697	1.17%	0.143%
10	6.069	1551	1564	1590	rBV	108037	227183	46.62%	5.695%
11	6.989	1839	1850	1873	rBV	50674	96263	19.76%	2.413%
12	7.313	1939	1951	1968	rBV	232057	405403	83.20%	10.162%
13	7.394	1969	1976	1989	rVB2	8452	15851	3.25%	0.397%
14	7.625	2039	2048	2069	rBV	29885	55820	11.46%	1.399%
15	7.940	2134	2146	2157	rBV2	2794	5009	1.03%	0.126%
16	8.092	2183	2193	2225	rBV2	199817	407457	83.62%	10.213%
17	8.850	2418	2429	2450	rBV	247074	405460	83.21%	10.163%
18	10.217	2843	2854	2872	rBV2	76977	121011	24.83%	3.033%
19	10.381	2894	2905	2916	rBV3	3500	5470	1.12%	0.137%
20	11.249	3164	3175	3192	rBV	264864	410122	84.17%	10.280%
21	11.622	3280	3291	3310	rBV	236414	371123	76.16%	9.303%




Sum of corrected areas: 3989489

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024188.D
Acq On : 27 Dec 2021 18:39
Operator : SY/MD
Sample : M5126-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

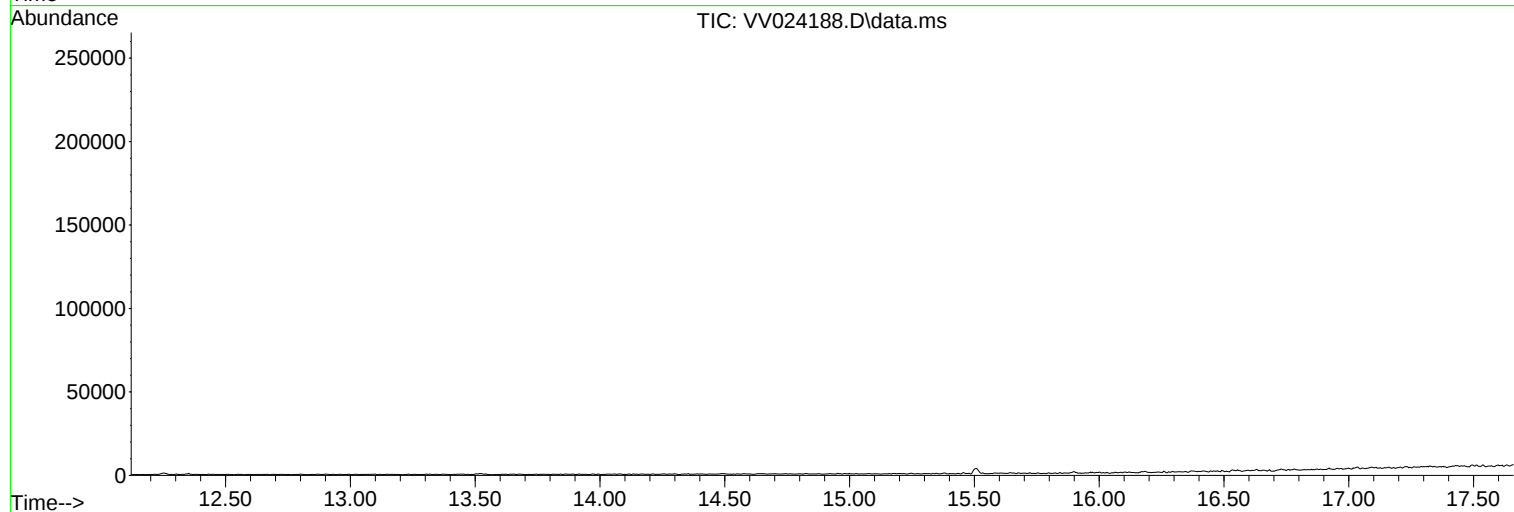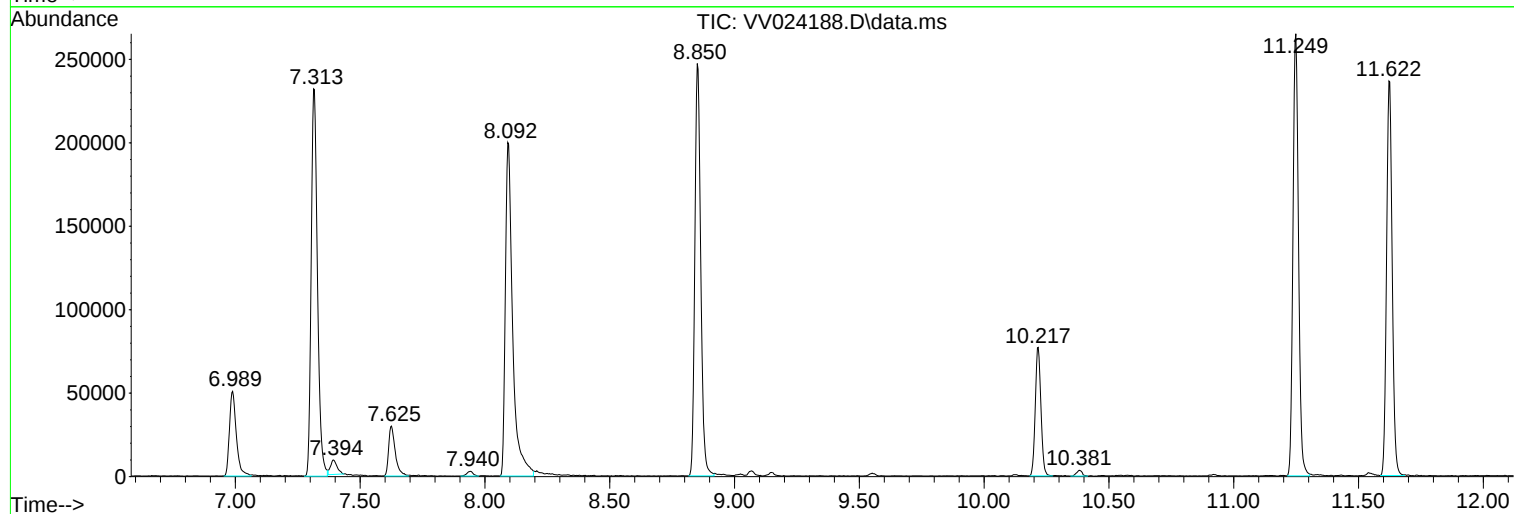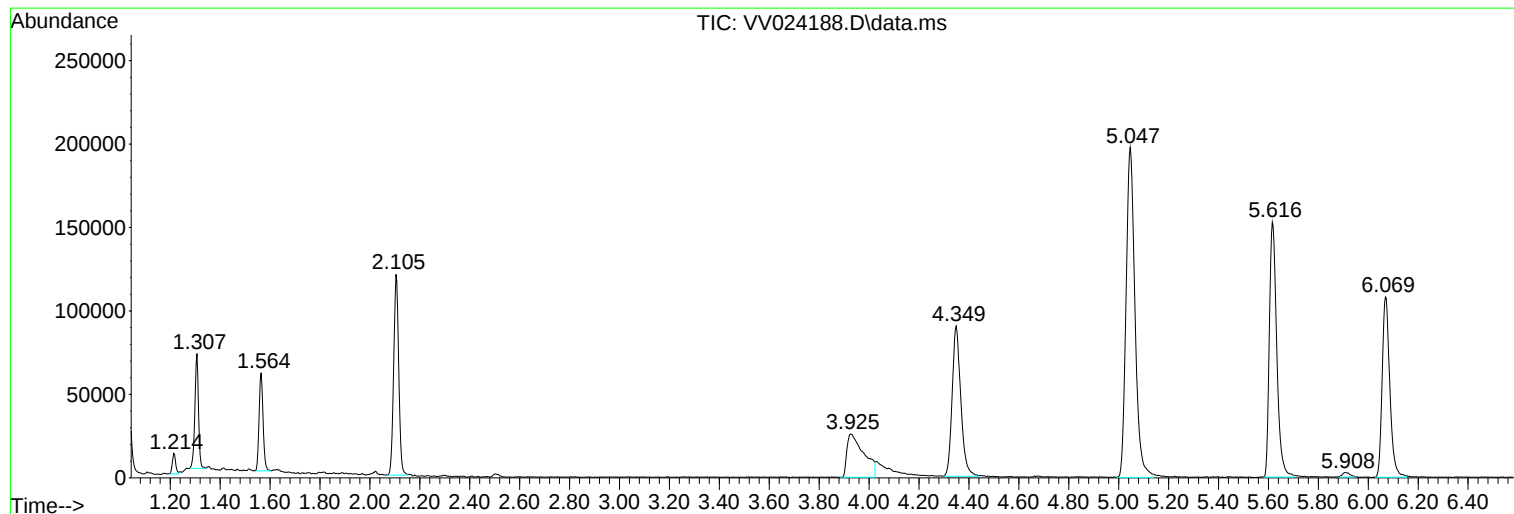

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024188.D
Acq On : 27 Dec 2021 18:39
Operator : SY/MD
Sample : M5126-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024188.D
Acq On : 27 Dec 2021 18:39
Operator : SY/MD
Sample : M5126-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
