

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
 Data File : VV024189.D
 Acq On : 27 Dec 2021 19:02
 Operator : SY/MD
 Sample : M5170-03DL2 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AN8DL2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024189.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	92	rVB	65229	70156	12.88%	1.591%
2	1.568	155	164	175	rBV	60815	69244	12.71%	1.571%
3	2.108	322	332	347	rVB	121399	170358	31.28%	3.864%
4	2.510	448	457	470	rVB2	8052	13666	2.51%	0.310%
5	3.912	875	893	926	rBV2	200643	544591	100.00%	12.352%
6	4.349	1013	1029	1056	rVB	86706	221295	40.64%	5.019%
7	5.047	1229	1246	1277	rBV2	195565	491127	90.18%	11.139%
8	5.616	1410	1423	1454	rBV	144748	297407	54.61%	6.746%
9	5.921	1505	1518	1532	rBV7	9155	20880	3.83%	0.474%
10	6.069	1551	1564	1588	rBV	110561	228275	41.92%	5.178%
11	6.989	1839	1850	1874	rBV	51426	96667	17.75%	2.193%
12	7.317	1940	1952	1972	rBV	232816	413692	75.96%	9.383%
13	7.625	2036	2048	2068	rBV	29216	54362	9.98%	1.233%
14	7.976	2148	2157	2171	rVB3	13393	24004	4.41%	0.544%
15	8.092	2183	2193	2230	rBV	173431	405551	74.47%	9.198%
16	8.420	2284	2295	2310	rBV3	7364	13864	2.55%	0.314%
17	8.850	2417	2429	2453	rBV	231631	381632	70.08%	8.656%
18	10.217	2842	2854	2870	rBV	77043	122225	22.44%	2.772%
19	11.249	3163	3175	3193	rBV	254811	392466	72.07%	8.902%
20	11.622	3280	3291	3311	rBV	236315	377502	69.32%	8.562%




Sum of corrected areas: 4408964

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024189.D
Acq On : 27 Dec 2021 19:02
Operator : SY/MD
Sample : M5170-03DL2 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AN8DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

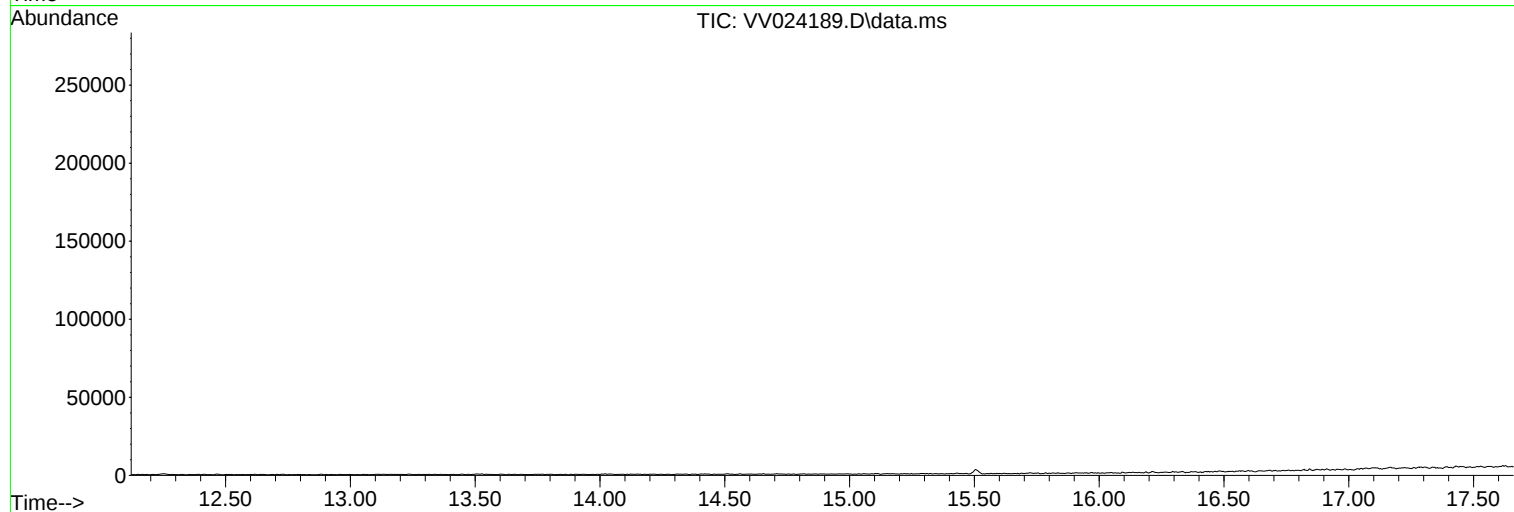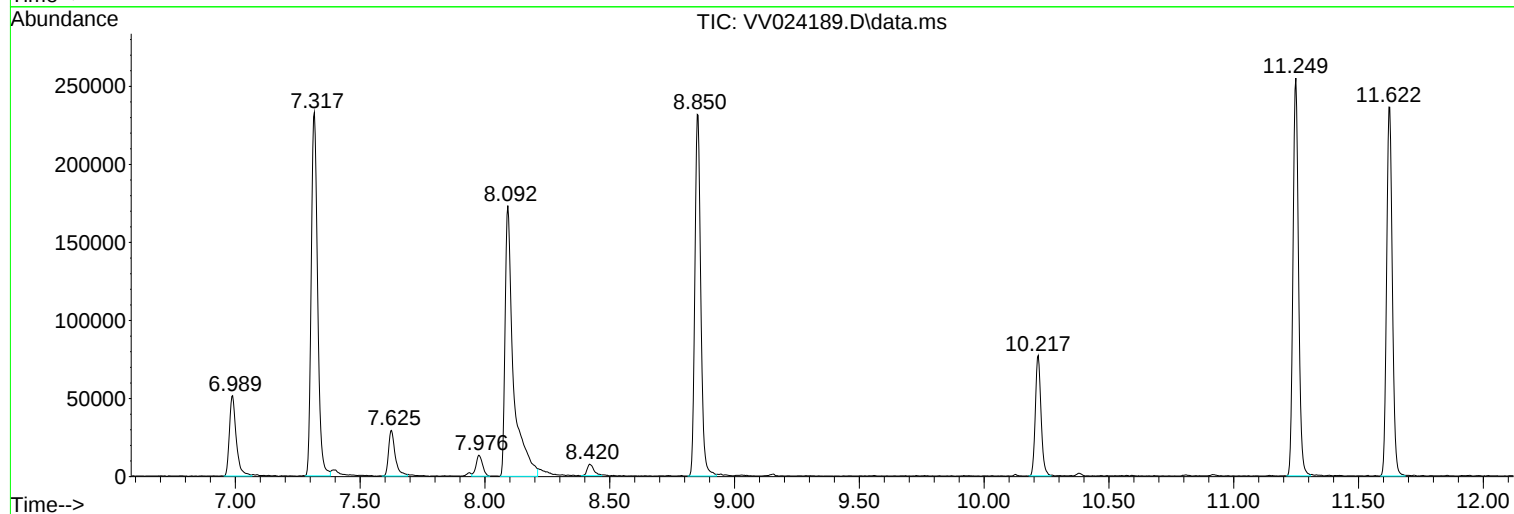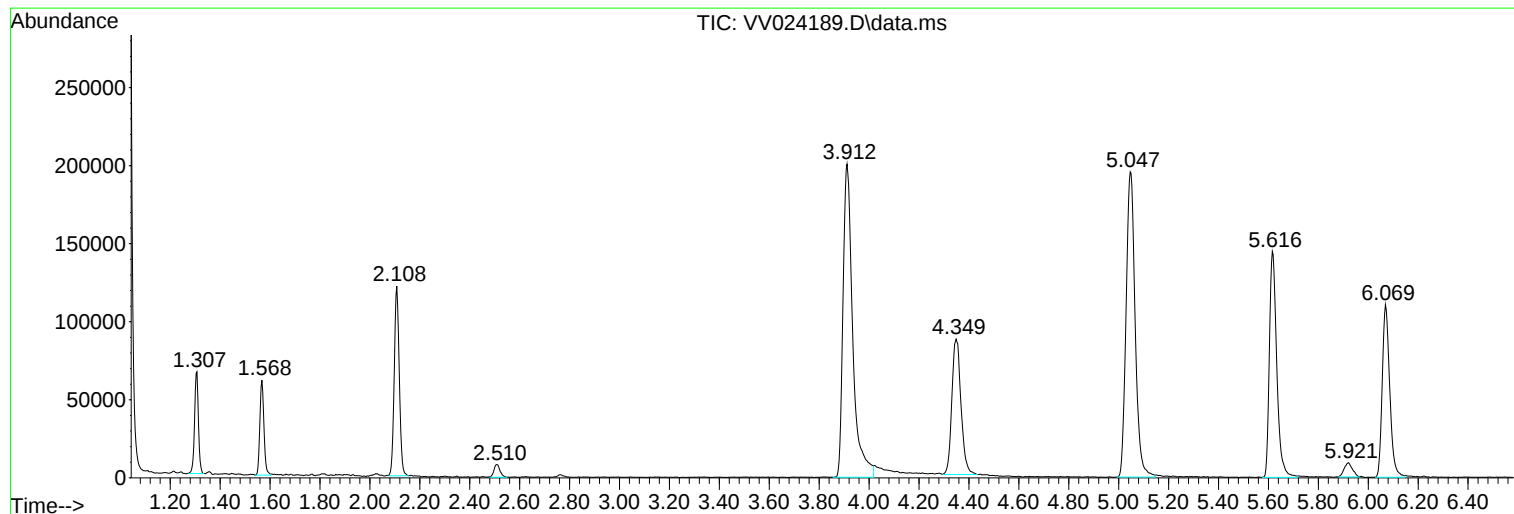

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024189.D
Acq On : 27 Dec 2021 19:02
Operator : SY/MD
Sample : M5170-03DL2 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AN8DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024189.D
Acq On : 27 Dec 2021 19:02
Operator : SY/MD
Sample : M5170-03DL2 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AN8DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc