

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
 Data File : VV024191.D
 Acq On : 27 Dec 2021 19:50
 Operator : SY/MD
 Sample : M5170-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	94	rBV	65382	67472	14.57%	1.816%
2	1.568	155	164	178	rBV	59989	68508	14.79%	1.844%
3	2.108	319	332	346	rBV	114922	164270	35.46%	4.421%
4	2.506	447	456	468	rBV2	5821	10670	2.30%	0.287%
5	3.921	883	896	927	rBV3	20206	99965	21.58%	2.690%
6	4.349	1012	1029	1052	rBV	86804	207463	44.79%	5.583%
7	5.047	1229	1246	1277	rBV3	186345	463193	100.00%	12.465%
8	5.616	1410	1423	1449	rBV	135780	277715	59.96%	7.474%
9	5.915	1507	1516	1528	rVB4	3469	6336	1.37%	0.171%
10	6.069	1551	1564	1591	rBV	101049	216262	46.69%	5.820%
11	6.989	1838	1850	1870	rBV3	47636	90581	19.56%	2.438%
12	7.317	1938	1952	1971	rBV	220318	391958	84.62%	10.548%
13	7.625	2036	2048	2067	rBV	28139	52220	11.27%	1.405%
14	8.091	2182	2193	2236	rBV	155842	392230	84.68%	10.556%
15	8.423	2286	2296	2308	rBV3	7050	12672	2.74%	0.341%
16	8.853	2418	2430	2452	rBV	216678	359735	77.66%	9.681%
17	10.217	2843	2854	2868	rBV2	74315	116656	25.19%	3.139%
18	11.249	3163	3175	3197	rBV	231206	361118	77.96%	9.718%
19	11.622	3280	3291	3308	rBV	221811	356778	77.03%	9.602%




Sum of corrected areas: 3715802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024191.D
Acq On : 27 Dec 2021 19:50
Operator : SY/MD
Sample : M5170-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

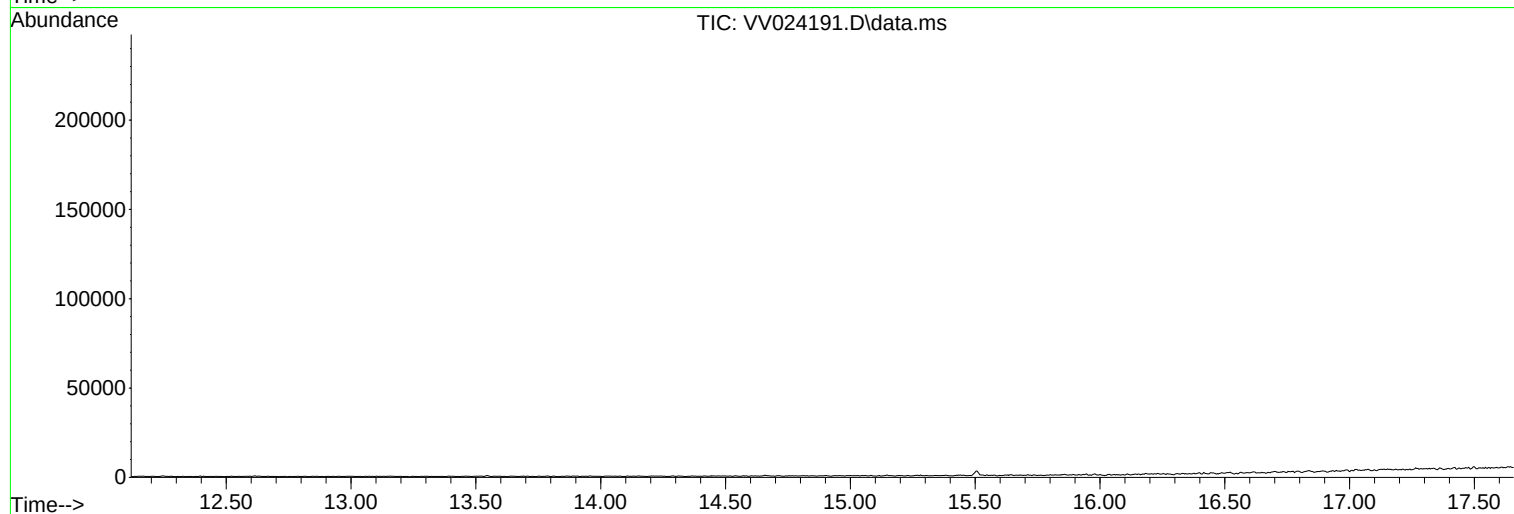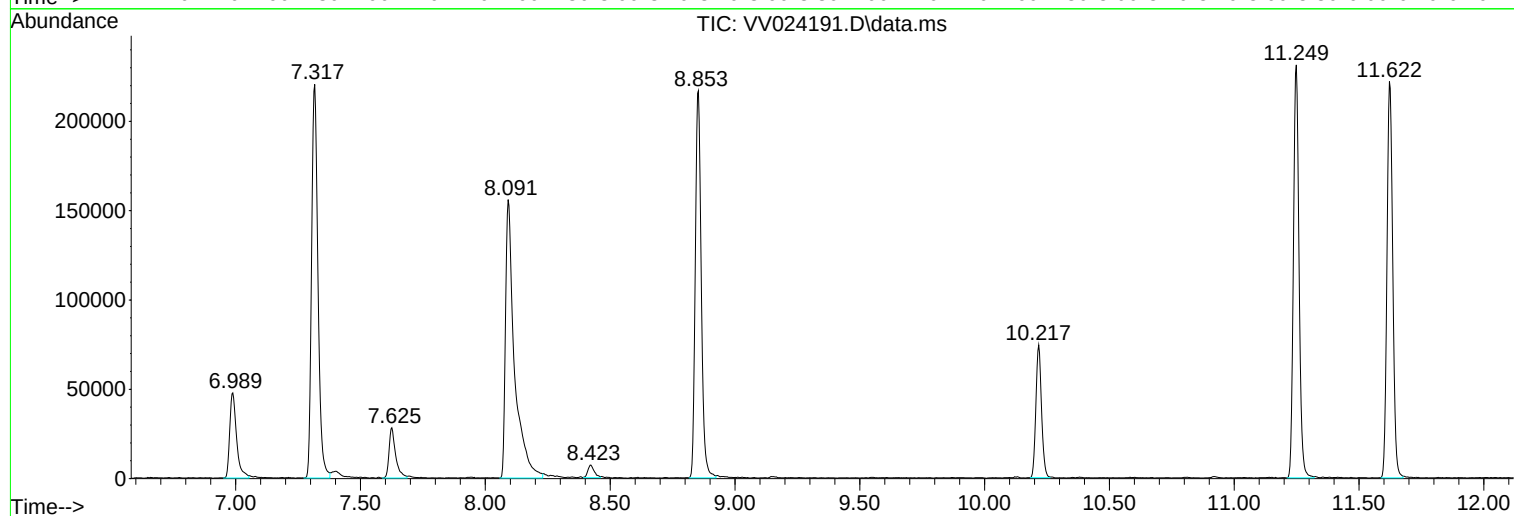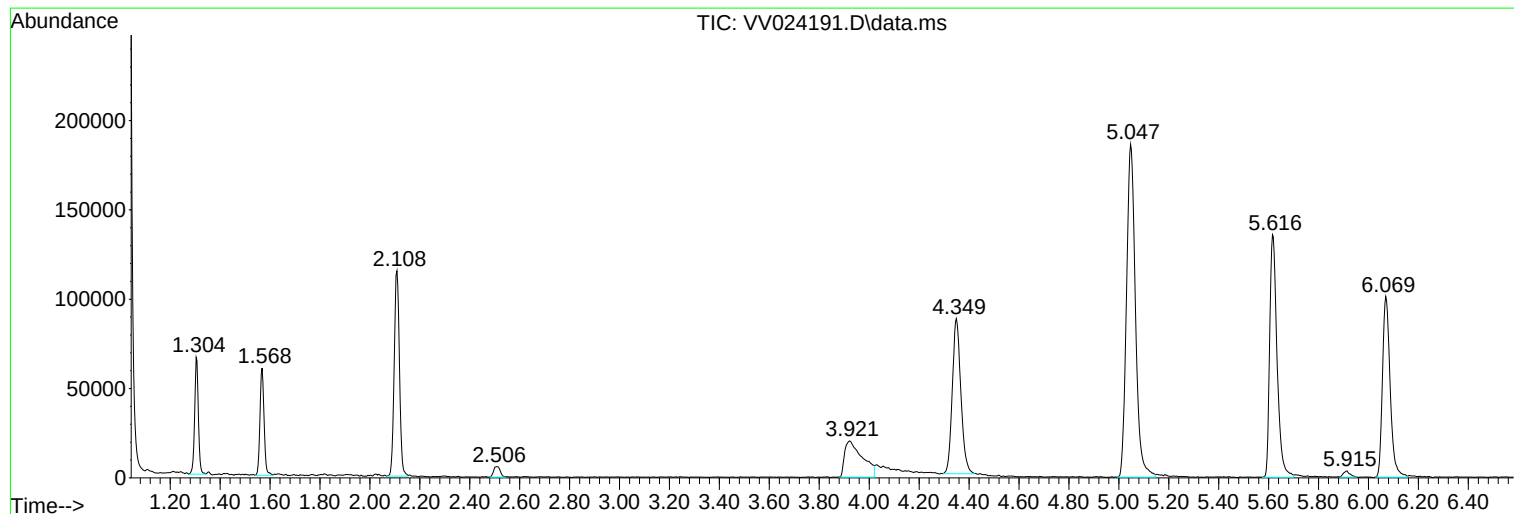

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024191.D
Acq On : 27 Dec 2021 19:50
Operator : SY/MD
Sample : M5170-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.989	1.63 ug/L	90581	1,4-Difluorobenzene	5.616

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Cyclohexadiene	80	C6H8	000592-57-4	37
2			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	32
3			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25
4			Thiophosgene	114	CCl2S	000463-71-8	25
5			1,3-Cyclohexadiene	80	C6H8	000592-57-4	25

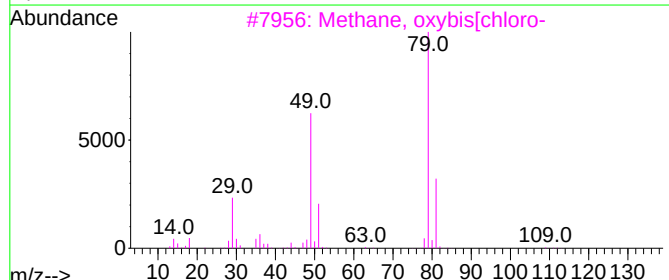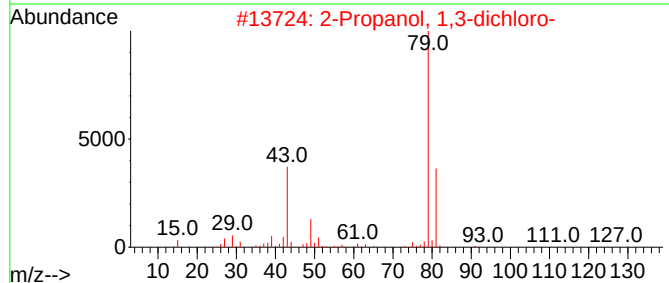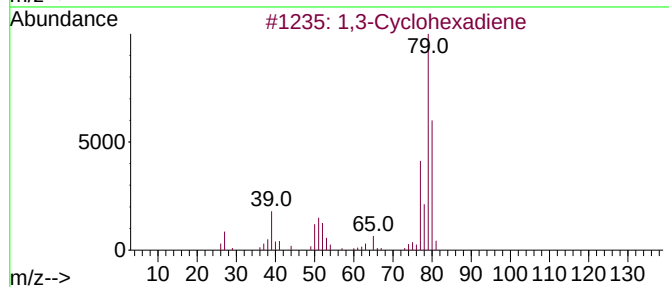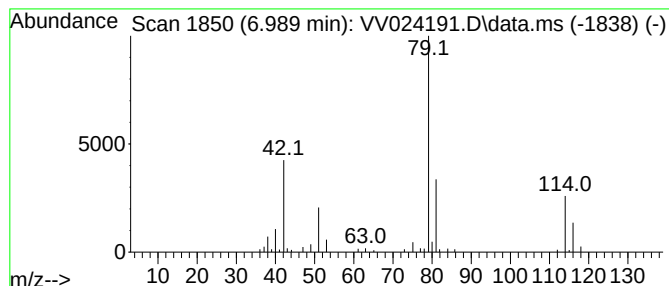

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024191.D
Acq On : 27 Dec 2021 19:50
Operator : SY/MD
Sample : M5170-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	6.989	1.6	ug/L	90581	1	5.616	277715	5.0