

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
 Data File : VV024196.D
 Acq On : 27 Dec 2021 21:49
 Operator : SY/MD
 Sample : M5233-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBCD2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	71	83	91	rBV	60710	62335	14.80%	1.880%
2	1.568	155	164	174	rBV	57070	63859	15.16%	1.926%
3	2.108	321	332	346	rBV	106958	154060	36.58%	4.646%
4	3.918	884	895	905	rBV	17077	48490	11.51%	1.462%
5	4.349	1015	1029	1056	rVB2	75801	186022	44.17%	5.610%
6	5.047	1231	1246	1276	rBV2	167001	421129	100.00%	12.701%
7	5.619	1408	1424	1452	rBV	120953	254250	60.37%	7.668%
8	5.908	1505	1514	1524	rBV5	3859	7215	1.71%	0.218%
9	6.069	1552	1564	1589	rBV	92526	195437	46.41%	5.894%
10	6.989	1839	1850	1867	rBV2	44431	84412	20.04%	2.546%
11	7.317	1941	1952	1969	rBV	197486	347728	82.57%	10.487%
12	7.394	1972	1976	1990	rVB3	4444	8096	1.92%	0.244%
13	7.625	2038	2048	2064	rBV	26552	49443	11.74%	1.491%
14	8.092	2183	2193	2232	rBV	135849	339539	80.63%	10.240%
15	8.854	2418	2430	2450	rBV	199708	329535	78.25%	9.938%
16	10.217	2843	2854	2871	rVB	61630	101822	24.18%	3.071%
17	11.249	3164	3175	3196	rBV	212922	331547	78.73%	9.999%
18	11.625	3280	3292	3311	rBV	204467	322185	76.51%	9.717%
19	12.349	3511	3517	3524	rBV6	3513	4377	1.04%	0.132%
20	13.435	3847	3855	3864	rBV6	3088	4315	1.02%	0.130%




Sum of corrected areas: 3315796

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024196.D
Acq On : 27 Dec 2021 21:49
Operator : SY/MD
Sample : M5233-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

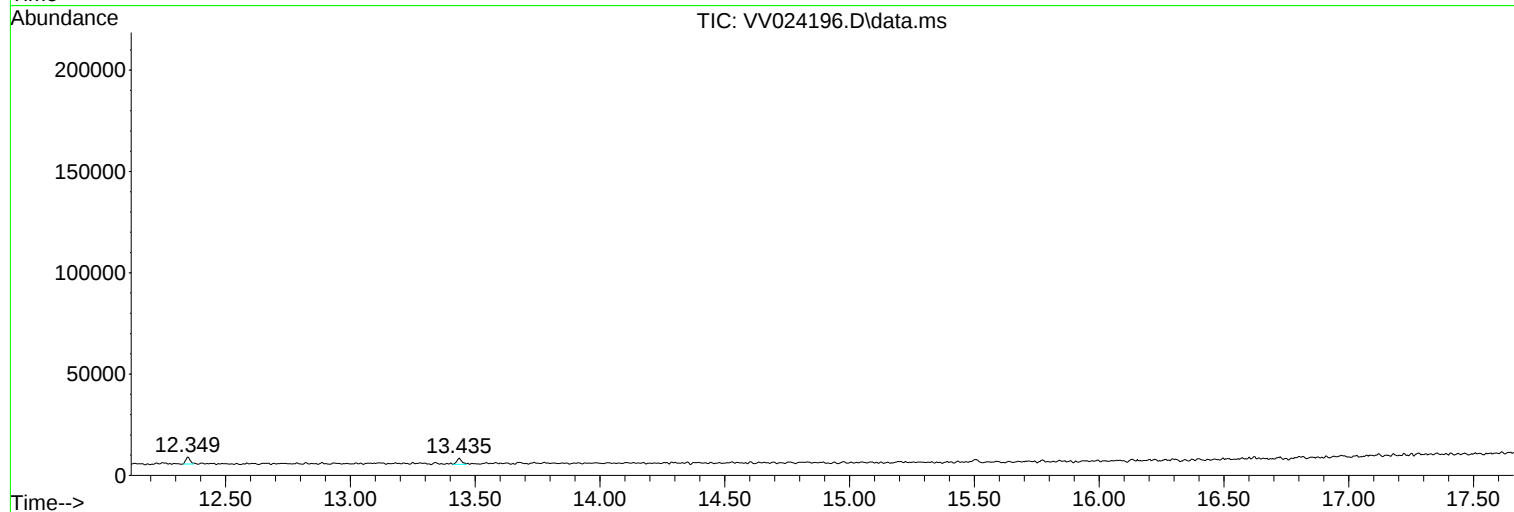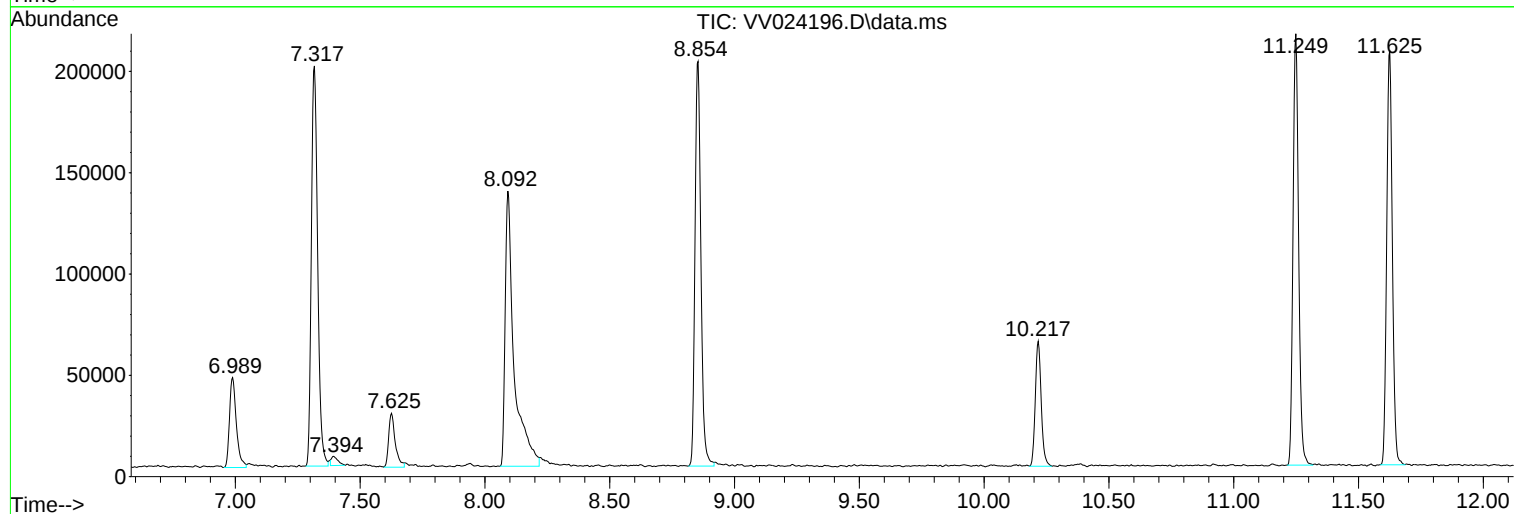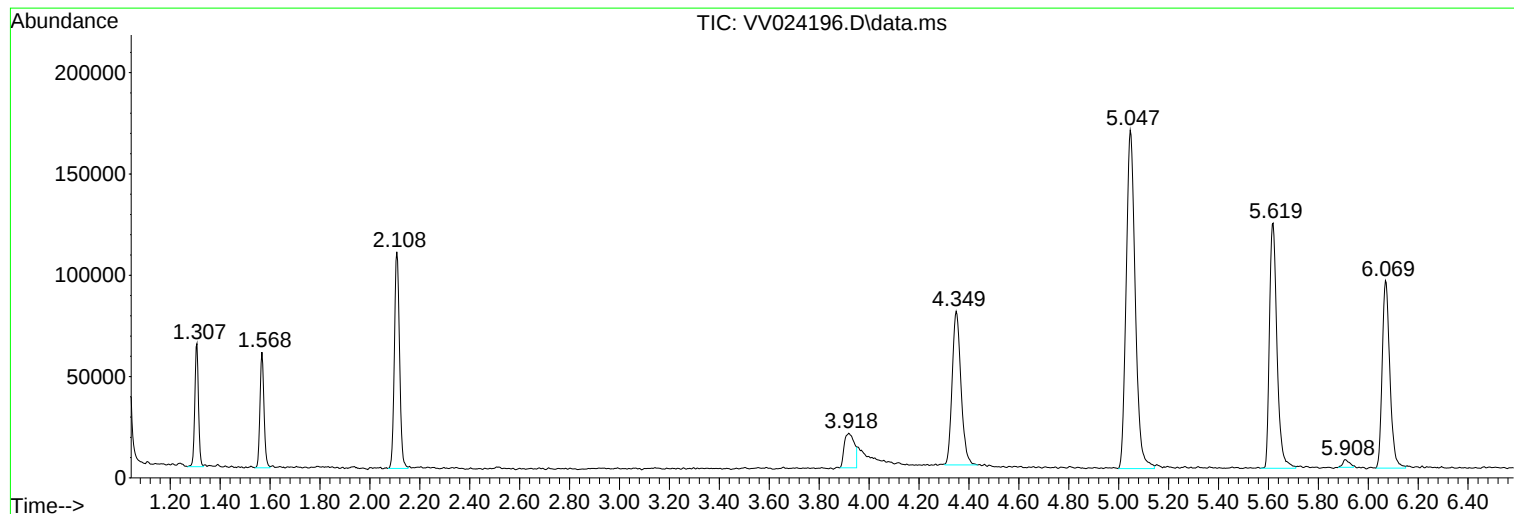

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024196.D
Acq On : 27 Dec 2021 21:49
Operator : SY/MD
Sample : M5233-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024196.D
Acq On : 27 Dec 2021 21:49
Operator : SY/MD
Sample : M5233-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBCD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc