

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
 Data File : VV024201.D
 Acq On : 27 Dec 2021 23:48
 Operator : SY/MD
 Sample : M5201-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 P080-TW001-C-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	94	rVB	53022	54076	14.48%	1.752%
2	1.568	155	164	177	rBV	50724	58364	15.63%	1.891%
3	2.111	319	333	345	rBV	98899	144031	38.57%	4.667%
4	3.912	883	893	915	rBV2	15618	58662	15.71%	1.901%
5	4.352	1015	1030	1062	rVB4	82167	251222	67.28%	8.141%
6	5.047	1229	1246	1274	rBV2	149094	373398	100.00%	12.100%
7	5.619	1412	1424	1450	rBV	109033	220847	59.15%	7.157%
8	5.915	1506	1516	1529	rBV6	2545	6321	1.69%	0.205%
9	6.069	1552	1564	1583	rBV2	83698	176197	47.19%	5.710%
10	6.516	1695	1703	1715	rVB6	3714	7293	1.95%	0.236%
11	6.989	1834	1850	1866	rBV	40906	76404	20.46%	2.476%
12	7.317	1941	1952	1971	rBV	178319	314477	84.22%	10.191%
13	7.394	1973	1976	1992	rVB6	3512	6690	1.79%	0.217%
14	7.625	2039	2048	2063	rBV2	23288	42452	11.37%	1.376%
15	8.092	2183	2193	2233	rBV	121721	317117	84.93%	10.276%
16	8.850	2417	2429	2446	rBV	178813	296314	79.36%	9.602%
17	10.217	2841	2854	2872	rBV	59894	98649	26.42%	3.197%
18	11.249	3161	3175	3195	rBV	187813	291978	78.19%	9.462%
19	11.622	3280	3291	3310	rBV	183943	291388	78.04%	9.443%




Sum of corrected areas: 3085880

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024201.D
Acq On : 27 Dec 2021 23:48
Operator : SY/MD
Sample : M5201-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P080-TW001-C-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

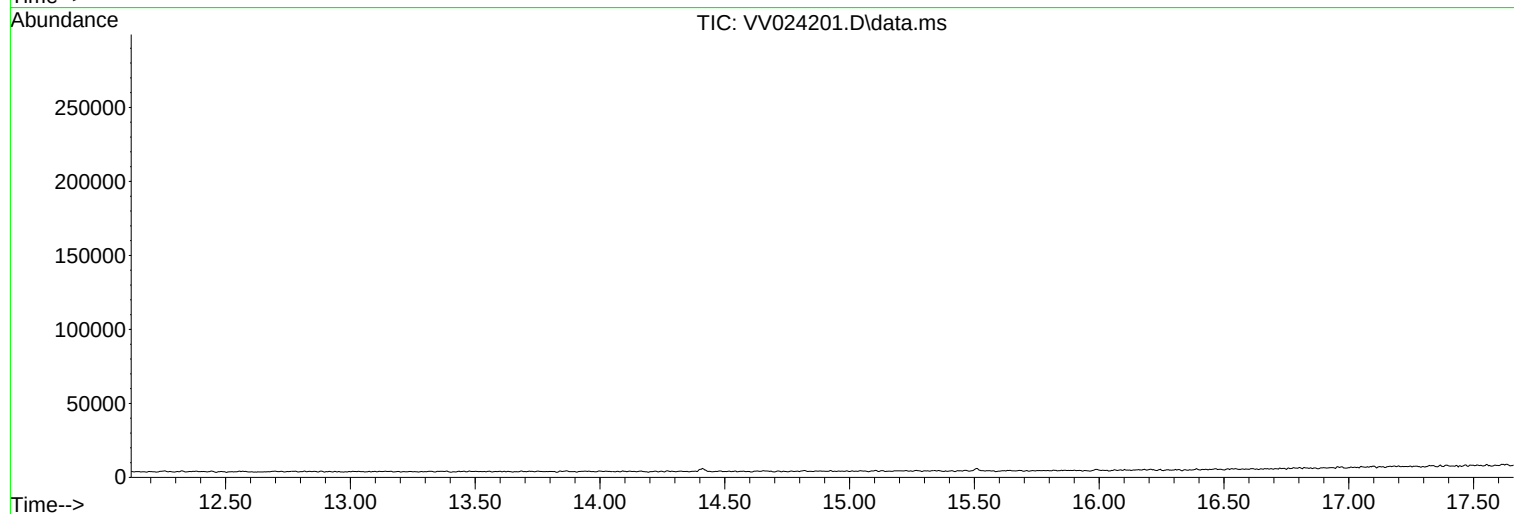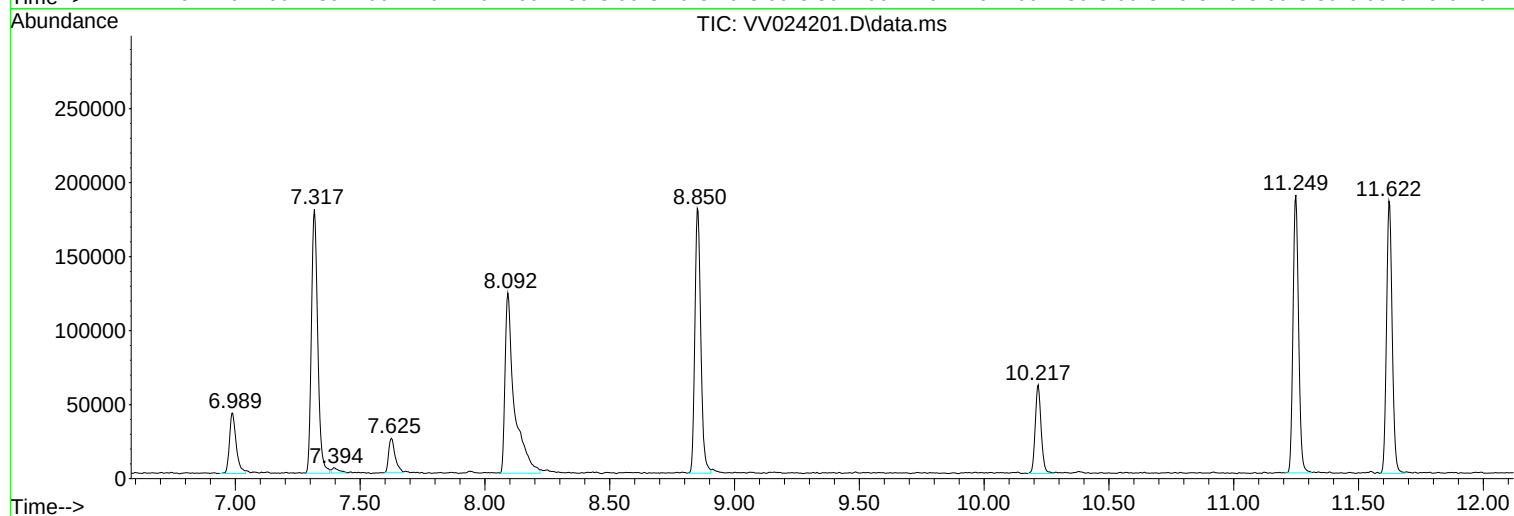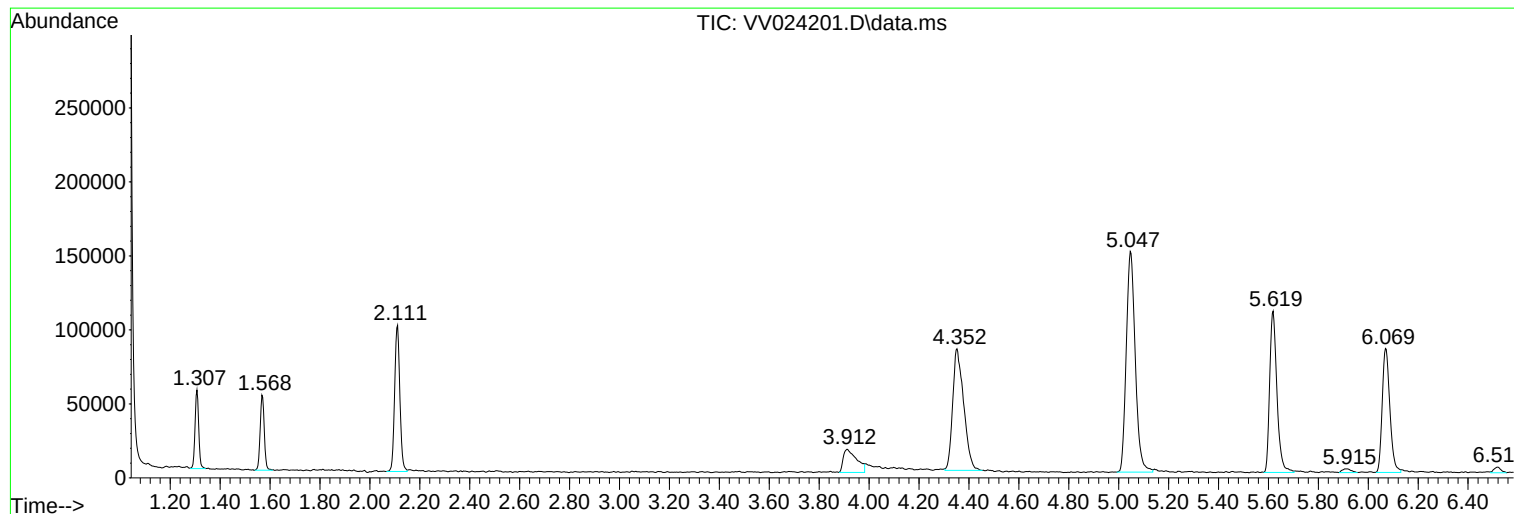

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024201.D
Acq On : 27 Dec 2021 23:48
Operator : SY/MD
Sample : M5201-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P080-TW001-C-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024201.D
Acq On : 27 Dec 2021 23:48
Operator : SY/MD
Sample : M5201-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P080-TW001-C-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------