
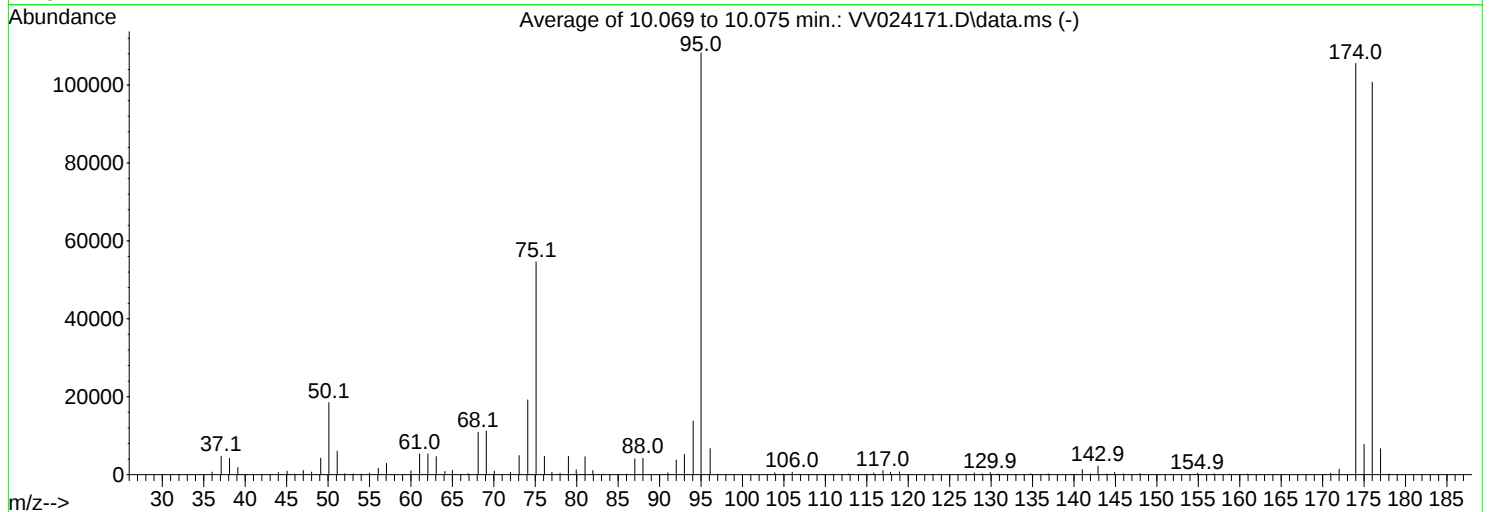


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122721\
Data File : VV024171.D
Acq On : 27 Dec 2021 09:27
Operator : SY/MD
Sample : BFB256
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB256

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 31 03:39:03 2021

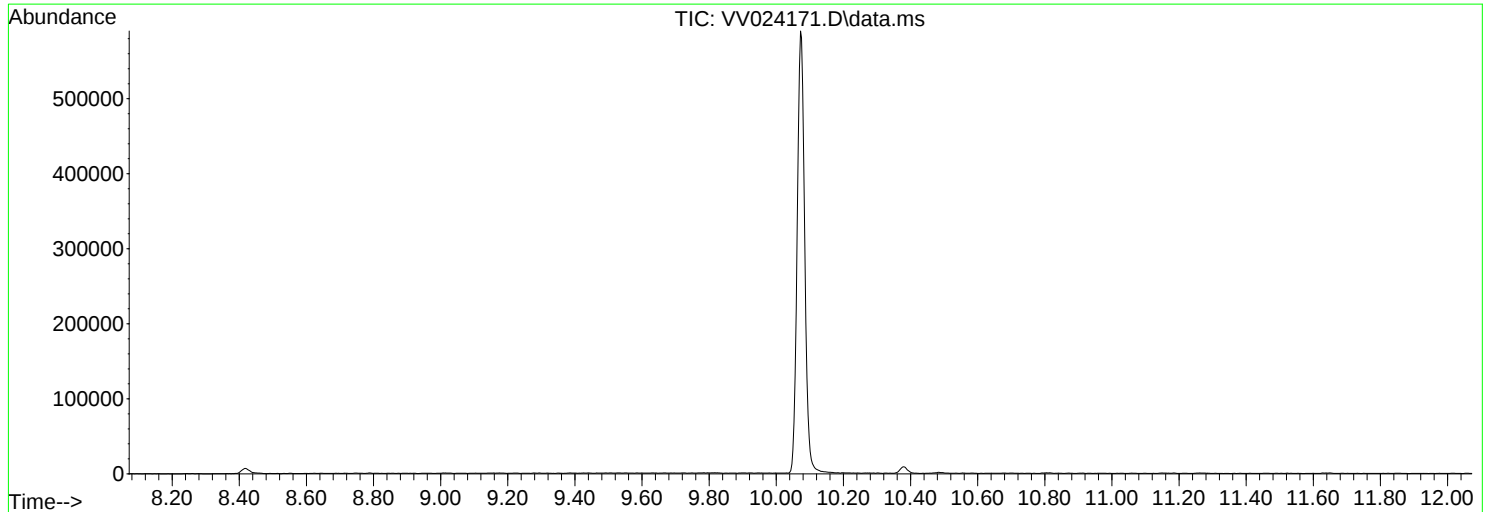

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	18496	PASS
75	95	30	80	50.5	54643	PASS
95	95	100	100	100.0	108272	PASS
96	95	5	9	6.2	6719	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	97.5	105536	PASS
175	174	5	9	7.4	7776	PASS
176	174	95	105	95.5	100736	PASS
177	176	5	10	6.6	6641	PASS

m/z	Abundance
36.00	615.0
36.90	116.0
37.90	281.0
40.10	104.0
44.00	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
36.00	1372.0
37.10	4608.0
38.10	3978.0
39.10	1724.0
40.20	151.0
44.10	658.0
45.00	915.0
45.90	144.0
47.00	1013.0
48.00	588.0
49.10	3980.0
50.10	18128.0
51.10	5927.0
52.00	250.0
53.10	172.0
54.00	143.0
55.00	390.0
56.00	1590.0
57.00	2698.0
60.00	1030.0
61.10	5215.0
62.00	5132.0
63.10	4384.0
64.10	809.0
65.00	997.0
66.90	290.0
68.10	10547.0
69.10	10615.0
70.10	854.0
72.00	607.0
73.00	4640.0
74.10	18432.0
75.10	52128.0
76.10	4434.0
77.00	610.0
78.00	338.0
79.00	4416.0
79.90	1162.0
81.00	4173.0
81.90	1076.0
83.20	112.0
86.00	122.0
87.00	3556.0
88.00	3978.0
91.00	439.0
92.00	3675.0
93.00	4730.0
94.00	13213.0
95.00	103704.0
96.10	6638.0
97.00	162.0
103.90	489.0
104.90	244.0
106.00	521.0
107.10	161.0
110.90	160.0
112.80	144.0
115.00	138.0
115.90	444.0
116.90	923.0
117.80	538.0
119.00	687.0
127.90	402.0
128.90	252.0
129.90	513.0
130.80	227.0
134.80	274.0
136.90	256.0
139.80	110.0
141.00	1237.0
142.10	175.0
142.90	2000.0
144.00	143.0
144.90	683.0
145.90	224.0
147.00	108.0
148.00	339.0
149.90	131.0
154.90	300.0
156.90	254.0
158.70	117.0
160.90	109.0
171.00	301.0
172.00	1275.0
174.00	97864.0
175.00	7284.0
176.00	94152.0
177.00	6480.0
178.10	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
36.00	1277.0
37.10	4916.0
38.10	4344.0
39.10	1791.0
40.20	203.0
40.90	108.0
44.00	677.0
45.10	932.0
46.00	172.0
47.00	1107.0
48.00	688.0
49.10	4369.0
50.10	19120.0
51.10	6306.0
52.00	234.0
53.00	212.0
54.00	142.0
55.00	379.0
56.10	1707.0
57.00	2984.0
57.90	124.0
60.00	1060.0
61.10	5455.0
62.10	5477.0
63.00	4822.0
64.10	841.0
65.00	1154.0
66.10	103.0
66.90	304.0
68.10	11202.0
69.10	11585.0
70.00	949.0
72.00	658.0
73.10	5048.0
74.10	19872.0
75.10	56472.0
76.10	4870.0
77.00	636.0
78.00	363.0
79.00	4796.0
79.90	1282.0
81.00	4772.0
82.00	1083.0
83.20	118.0
86.00	157.0
87.00	4151.0
88.00	4385.0
91.00	525.0
92.00	3873.0
93.00	5423.0
94.10	14333.0
95.00	112272.0
96.10	6944.0
97.00	147.0
103.90	538.0
104.90	213.0
106.00	605.0
106.90	131.0
110.90	139.0
112.80	195.0
115.00	140.0
115.80	481.0
116.90	1009.0
117.90	640.0
118.90	702.0
127.90	449.0
128.90	270.0
129.90	574.0
130.90	235.0
134.80	273.0
136.90	245.0
139.70	120.0
141.00	1364.0
142.00	220.0
142.90	2255.0
143.90	151.0
144.90	615.0
145.90	250.0
148.00	320.0
150.00	110.0
153.90	109.0
154.90	338.0
156.90	273.0
158.70	113.0
161.00	105.0
170.90	331.0
172.00	1495.0
174.00	109272.0
175.00	8065.0
176.00	103904.0
177.00	6913.0
178.00	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
36.00	1214.0
37.10	4703.0
38.10	4225.0
39.10	1893.0
40.20	210.0
41.00	112.0
44.00	750.0
45.00	876.0
46.00	183.0
47.00	1052.0
48.00	675.0
49.10	4301.0
50.10	18240.0
51.10	5898.0
52.00	209.0
53.00	215.0
54.00	115.0
55.00	297.0
56.10	1628.0
57.10	2894.0
57.90	149.0
60.00	929.0
61.00	5326.0
62.10	5311.0
63.00	4760.0
64.10	794.0
65.00	1181.0
66.00	134.0
66.90	282.0
68.10	10951.0
69.10	11302.0
70.00	933.0
72.00	652.0
73.10	4971.0
74.10	19256.0
75.10	55328.0
76.10	4715.0
77.00	578.0
78.00	387.0
79.00	4814.0
80.00	1220.0
81.00	4831.0
82.00	1051.0
82.70	117.0
83.20	122.0
86.00	198.0
87.00	4453.0
88.00	4219.0
91.00	550.0
92.00	3626.0
93.00	5549.0
94.10	13696.0
95.00	108840.0
96.10	6575.0
97.10	128.0
103.90	508.0
105.00	186.0
106.00	675.0
106.80	143.0
107.80	104.0
110.90	104.0
112.80	193.0
115.00	160.0
115.80	466.0
117.00	1108.0
117.90	642.0
118.90	700.0
128.00	456.0
128.90	274.0
129.90	540.0
130.90	218.0
134.80	240.0
136.90	242.0
139.70	111.0
141.00	1378.0
141.90	242.0
142.90	2224.0
143.90	167.0
144.90	549.0
146.00	243.0
147.90	269.0
150.00	112.0
153.80	115.0
154.90	348.0
156.90	236.0
158.80	128.0
160.80	116.0
161.10	145.0
170.90	304.0
172.00	1483.0
174.00	109472.0
175.00	7980.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

176.00104152.0

177.006529.0

177.90187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256