

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122819\
 Data File : VV014214.D
 Acq On : 28 Dec 2019 14:08
 Operator : SY/MD
 Sample : K6432-13
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Dec 30 09:04:14 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Dec 30 00:30:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	808826	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	721874	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	339640	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	210325	5.55	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.00%
7) Chloroethane-d5	1.58	69	186818	5.92	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	118.40%
11) 1,1-Dichloroethene-d2	2.13	63	275575	4.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.00%
20) 2-Butanone-d5	3.92	46	589989	62.70	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.40%
24) Chloroform-d	4.40	84	481840	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
26) 1,2-Dichloroethane-d4	5.08	65	242383	5.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.80%
32) Benzene-d6	5.09	84	1017145	5.16	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.20%
36) 1,2-Dichloropropane-d6	6.11	67	319790	5.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.20%
41) Toluene-d8	7.36	98	927118	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
43) trans-1,3-Dichloropropene-	7.66	79	131767	4.94	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.80%
46) 2-Hexanone-d5	8.13	63	529071	52.23	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.46%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	221334	5.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	310876	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%


Target Compounds					Ovalue
16) Methylene chloride	2.54	84	19339	0.321 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV122819\
Data File : VV014214.D
Acq On : 28 Dec 2019 14:08
Operator : SY/MD
Sample : K6432-13
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Dec 30 09:04:14 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR122719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Dec 30 00:30:20 2019
Response via : Initial Calibration

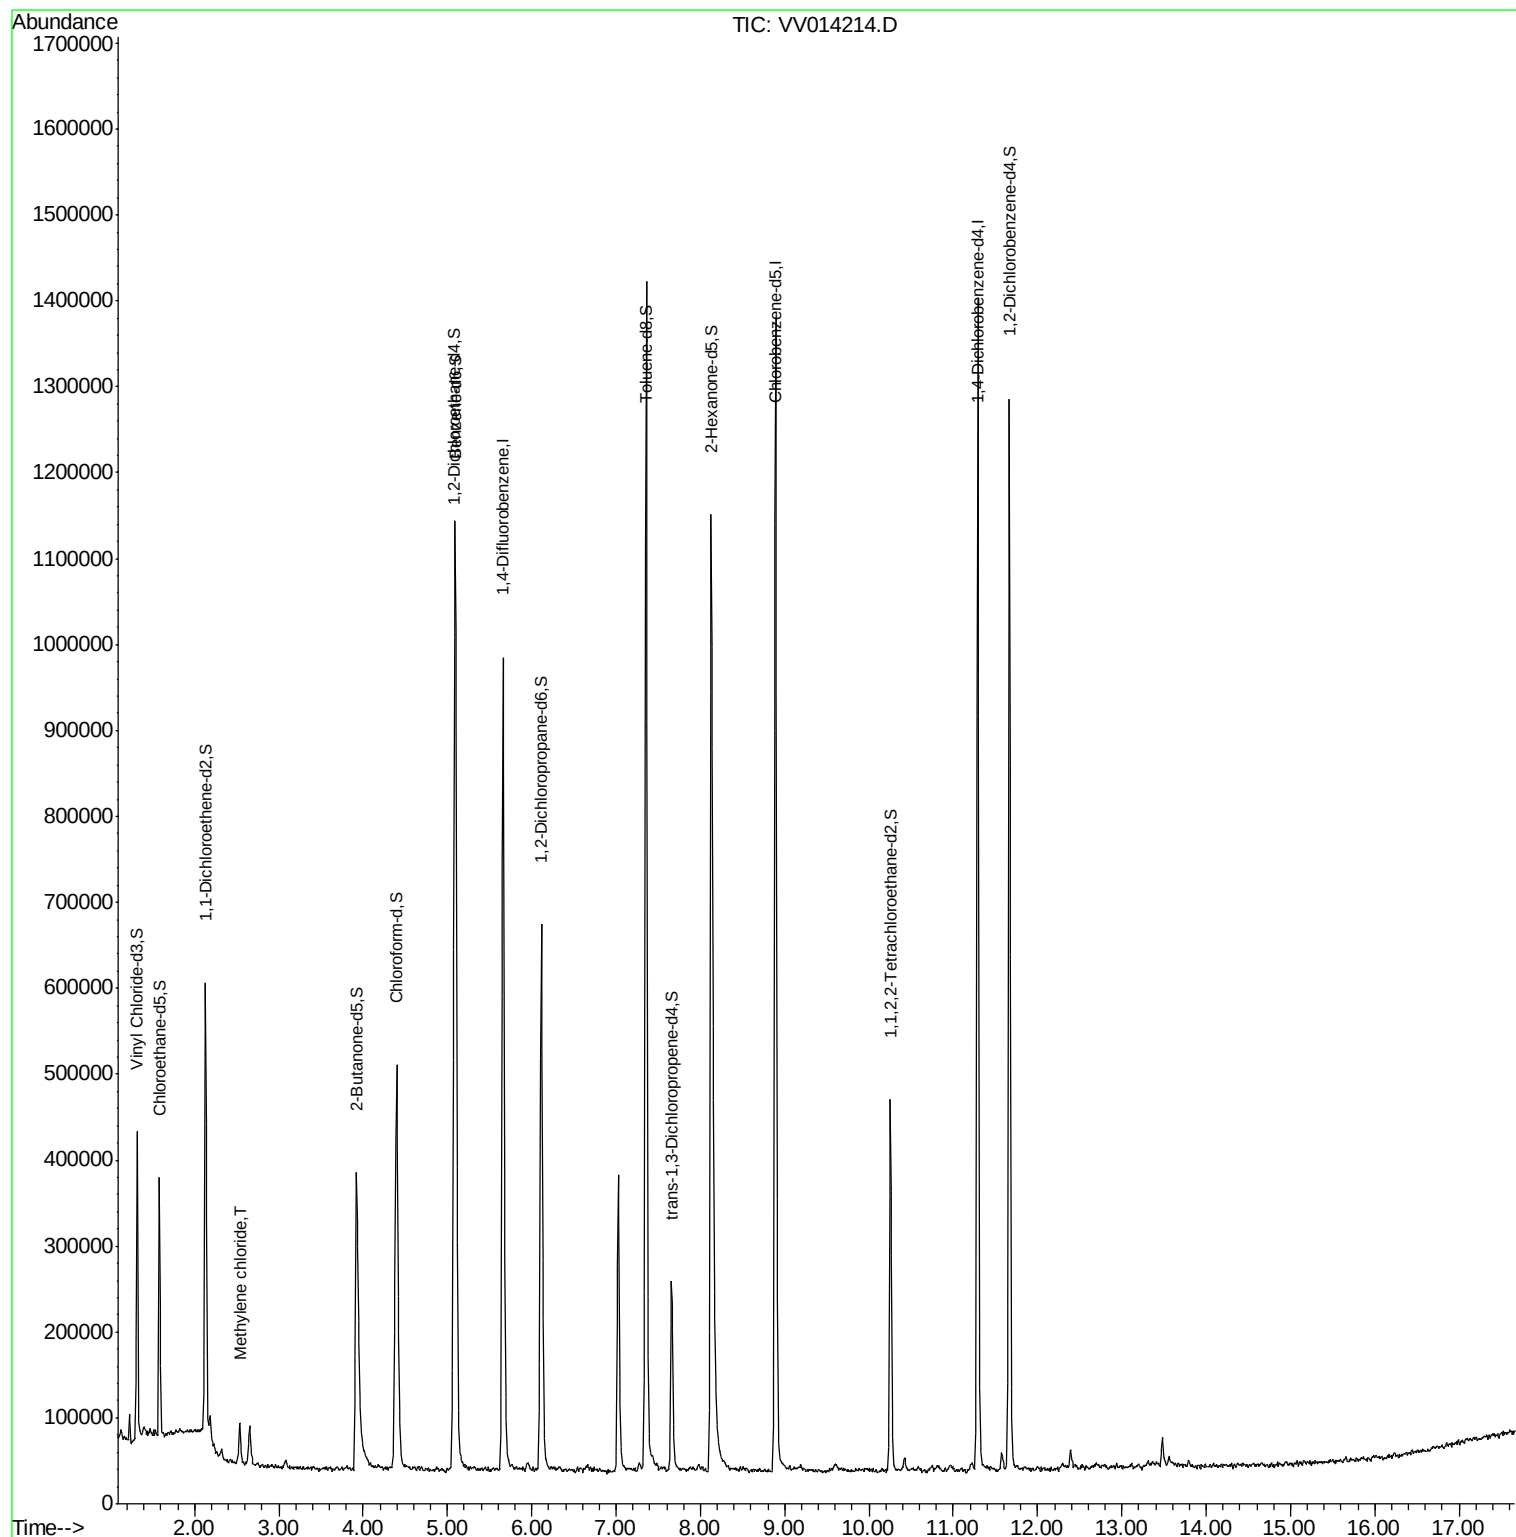

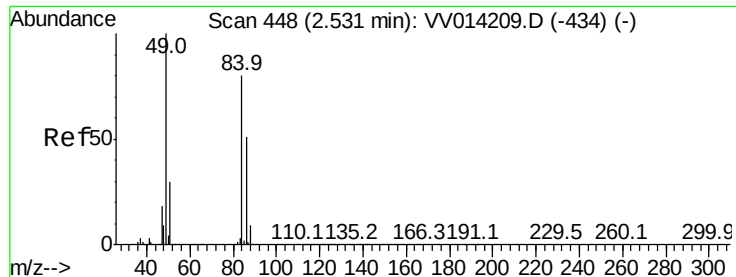

#16
Methylene chloride
Concen: 0.321 ug/L
RT: 2.54 min Scan# 450
Delta R.T. 0.01 min
Lab File: VV014214.D
Acq: 28 Dec 2019 14:08

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Tot Ion	Ratio	Lower	Upper
84	100		
86	57.1	43.1	80.1
49	116.4	82.1	152.5

