

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122820\
 Data File : VV019851.D
 Acq On : 28 Dec 2020 15:36
 Operator : SY/MD
 Sample : L5204-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	366866	378605	14.74%	1.955%
2	1.569	142	149	163	rVB	295789	336777	13.11%	1.739%
3	2.110	308	317	353	rVB	603733	932112	36.29%	4.812%
4	2.746	512	515	516	rBV2	1188	641	0.02%	0.003%
5	2.836	540	543	547	rBV5	976	946	0.04%	0.005%
6	3.097	622	624	625	rBV	672	258	0.01%	0.001%
7	3.383	707	713	720	rBV7	969	1304	0.05%	0.007%
8	3.479	739	743	747	rVB5	603	384	0.01%	0.002%
9	3.515	752	754	755	rBV2	780	367	0.01%	0.002%
10	3.550	761	765	766	rBV3	744	549	0.02%	0.003%
11	3.592	775	778	780	rBV3	636	445	0.02%	0.002%
12	3.643	791	794	796	rBV4	945	705	0.03%	0.004%
13	3.685	805	807	809	rVB3	368	131	0.01%	0.001%
14	3.704	809	813	814	rBV2	805	579	0.02%	0.003%
15	3.791	837	840	843	rVB3	692	315	0.01%	0.002%
16	3.894	861	872	919	rBV	186577	593325	23.10%	3.063%
17	4.354	1000	1015	1042	rVB	407903	998525	38.88%	5.155%
18	4.839	1164	1166	1170	rBV4	865	645	0.03%	0.003%
19	4.891	1177	1182	1185	rBV3	923	966	0.04%	0.005%
20	5.052	1215	1232	1264	rBV2	1002901	2568266	100.00%	13.260%
21	5.457	1355	1358	1361	rBV3	850	666	0.03%	0.003%
22	5.621	1395	1409	1440	rBV	743677	1486618	57.88%	7.675%
23	5.910	1491	1499	1521	rVB2	38005	79019	3.08%	0.408%
24	6.074	1536	1550	1579	rBV	581423	1179907	45.94%	6.092%
25	6.396	1646	1650	1652	rBV4	1066	854	0.03%	0.004%
26	6.434	1659	1662	1664	rBV3	1183	779	0.03%	0.004%
27	6.618	1716	1719	1721	rVB2	797	408	0.02%	0.002%
28	6.637	1721	1725	1728	rBV4	1072	1052	0.04%	0.005%
29	6.653	1728	1730	1737	rVV6	852	860	0.03%	0.004%
30	6.736	1754	1756	1759	rBV2	762	469	0.02%	0.002%
31	6.772	1764	1767	1772	rVV4	799	723	0.03%	0.004%
32	6.862	1794	1795	1799	rVB2	857	469	0.02%	0.002%
33	6.945	1819	1821	1823	rBV3	689	286	0.01%	0.001%
34	6.990	1823	1835	1859	rBV2	328063	598167	23.29%	3.088%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122820\
 Data File : VV019851.D
 Acq On : 28 Dec 2020 15:36
 Operator : SY/MD
 Sample : L5204-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
 Title : VOC Analysis

35	7.322	1925	1938	1963	rBV	1151884	2007228	78.15%	10.363%
36	7.627	2022	2033	2060	rBV	227053	407805	15.88%	2.105%
37	7.904	2118	2119	2122	rBV3	1055	619	0.02%	0.003%
38	8.093	2167	2178	2217	rBV	647686	1258103	48.99%	6.495%
39	8.778	2388	2391	2392	rBV2	774	384	0.01%	0.002%
40	8.855	2403	2415	2444	rBV	1108874	1825669	71.09%	9.426%
41	9.318	2556	2559	2561	rBV2	864	601	0.02%	0.003%
42	9.505	2615	2617	2620	rBV3	929	593	0.02%	0.003%
43	9.653	2661	2663	2665	rBV2	685	337	0.01%	0.002%
44	9.701	2675	2678	2680	rBV3	670	459	0.02%	0.002%
45	10.161	2817	2821	2824	rBV5	930	767	0.03%	0.004%
46	10.222	2828	2840	2860	rVV	713279	1112924	43.33%	5.746%
47	10.386	2888	2891	2892	rBV2	1005	523	0.02%	0.003%
48	10.463	2912	2915	2917	rBV3	1079	846	0.03%	0.004%
49	10.505	2926	2928	2933	rVB3	789	475	0.02%	0.002%
50	11.254	3150	3161	3186	rBV	1154159	1779469	69.29%	9.187%
51	11.440	3217	3219	3221	rBV3	1072	387	0.02%	0.002%
52	11.630	3266	3278	3299	rBV	1165087	1803114	70.21%	9.309%
53	12.203	3454	3456	3459	rBV2	828	365	0.01%	0.002%
54	12.370	3505	3508	3510	rBV4	668	456	0.02%	0.002%
55	12.990	3697	3701	3704	rBV3	1091	962	0.04%	0.005%
56	13.813	3955	3957	3962	rBV2	1205	821	0.03%	0.004%


Sum of corrected areas: 19369029

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV122820\
Data File : VV019851.D
Acq On : 28 Dec 2020 15:36
Operator : SY/MD
Sample : L5204-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

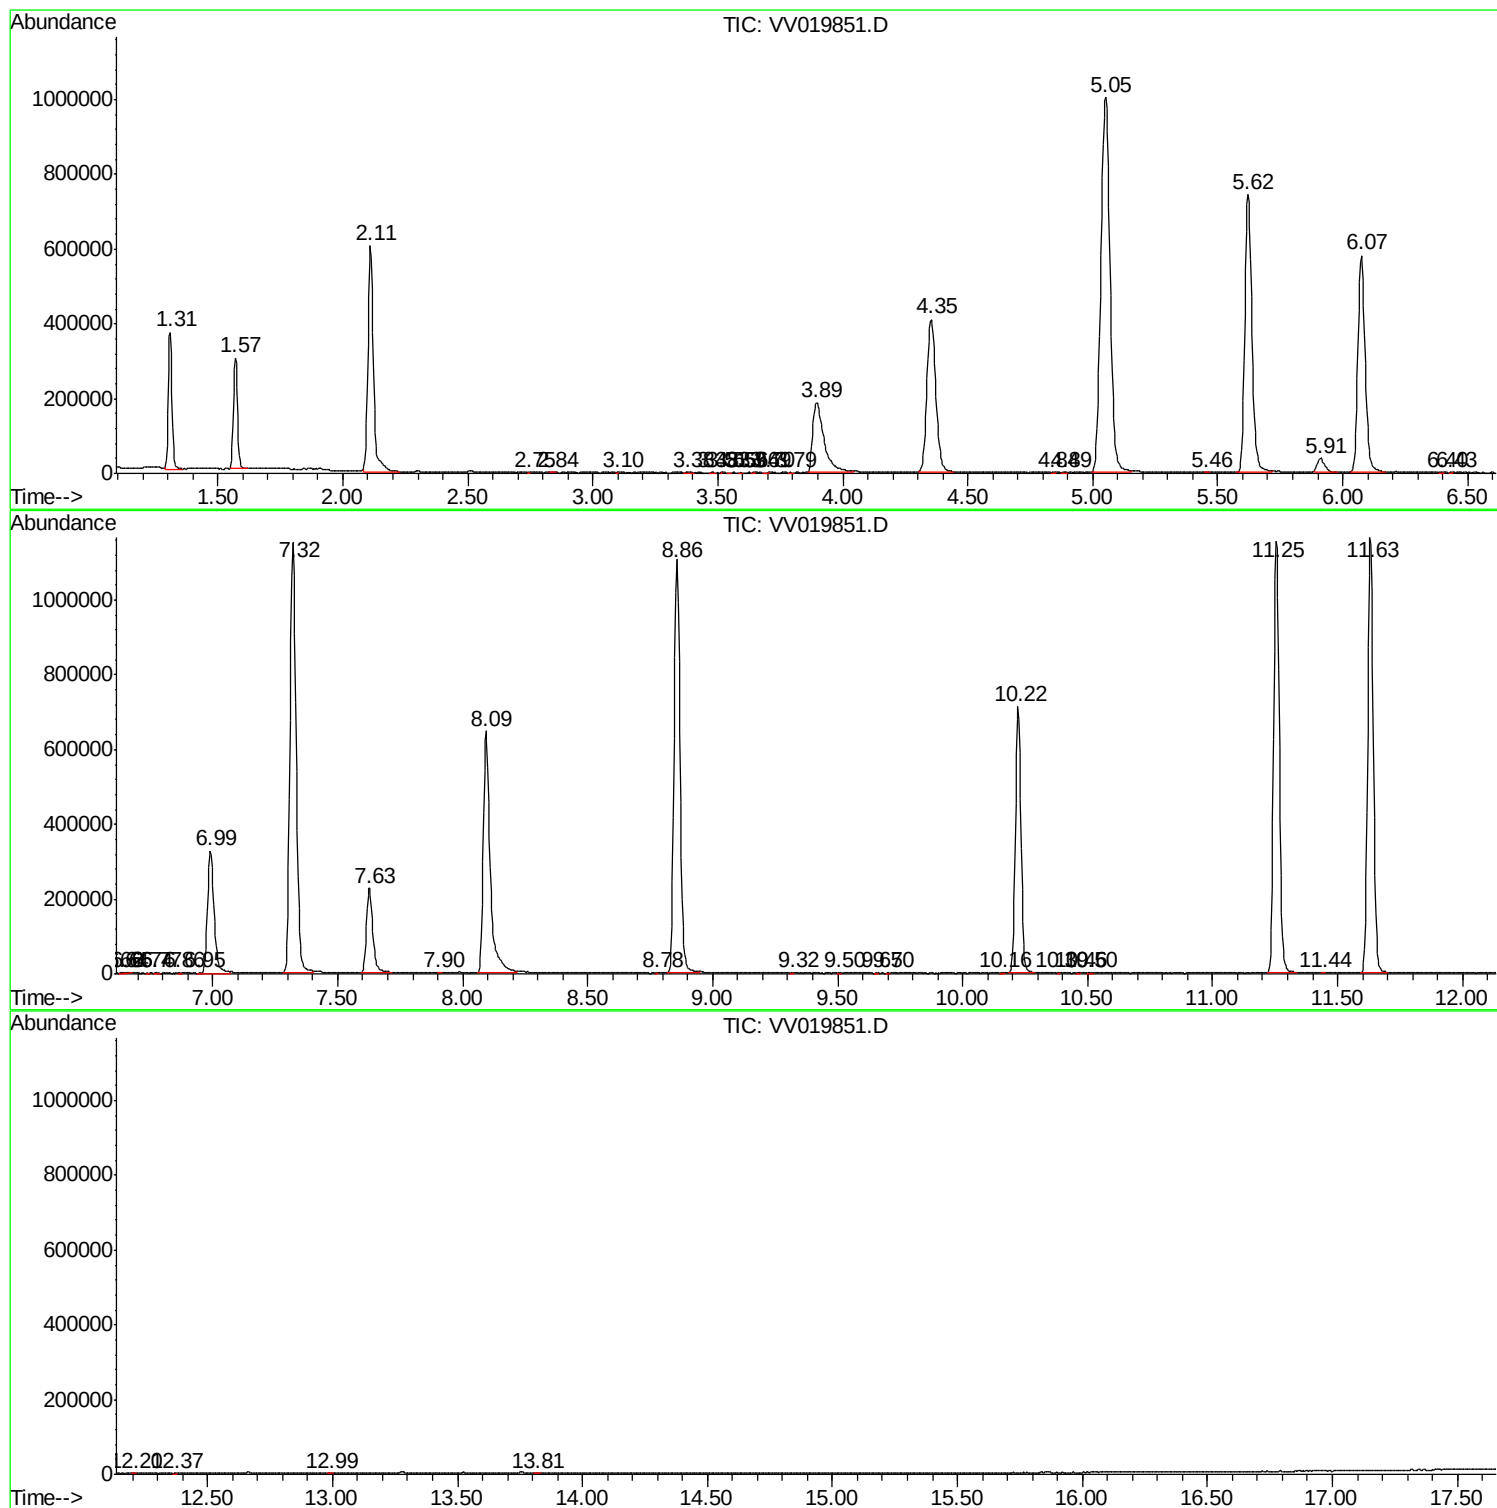

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV122820\
Data File : VV019851.D
Acq On : 28 Dec 2020 15:36
Operator : SY/MD
Sample : L5204-05
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV122820\
Data File : VV019851.D
Acq On : 28 Dec 2020 15:36
Operator : SY/MD
Sample : L5204-05
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM122820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc