

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122821\
 Data File : VW024215.D
 Acq On : 28 Dec 2021 14:00
 Operator : SY/MD
 Sample : M5201-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 P036-TW001-01

Quant Time: Dec 29 05:05:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 29 04:43:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	77679	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	81456	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	42188	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	25698	4.398	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.000%	
7) Chloroethane-d5	1.568	69	25488	5.231	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	104.600%	
11) 1,1-Dichloroethene-d2	2.108	63	41423	2.917	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	58.400%#	
20) 2-Butanone-d5	3.915	46	33437	51.520	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.040%	
24) Chloroform-d	4.349	84	62476	5.037	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.800%	
26) 1,2-Dichloroethane-d4	5.034	65	31208	5.621	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	112.400%	
32) Benzene-d6	5.050	84	111327	5.061	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.200%	
36) 1,2-Dichloropropane-d6	6.069	67	32703	5.427	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	108.600%	
41) Toluene-d8	7.317	98	97961	4.518	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.400%	
43) trans-1,3-Dichloroprop...	7.625	79	12355	4.842	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	96.800%	
46) 2-Hexanone-d5	8.092	63	44772	52.189	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	104.380%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	21548	5.238	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	104.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	41347	5.638	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	112.800%	
Target Compounds					Qvalue	
25) Chloroform	4.381	83	13892	0.659	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024215.D
Acq On : 28 Dec 2021 14:00
Operator : SY/MD
Sample : M5201-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P036-TW001-01

Quant Time: Dec 29 05:05:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 29 04:43:10 2021
Response via : Initial Calibration

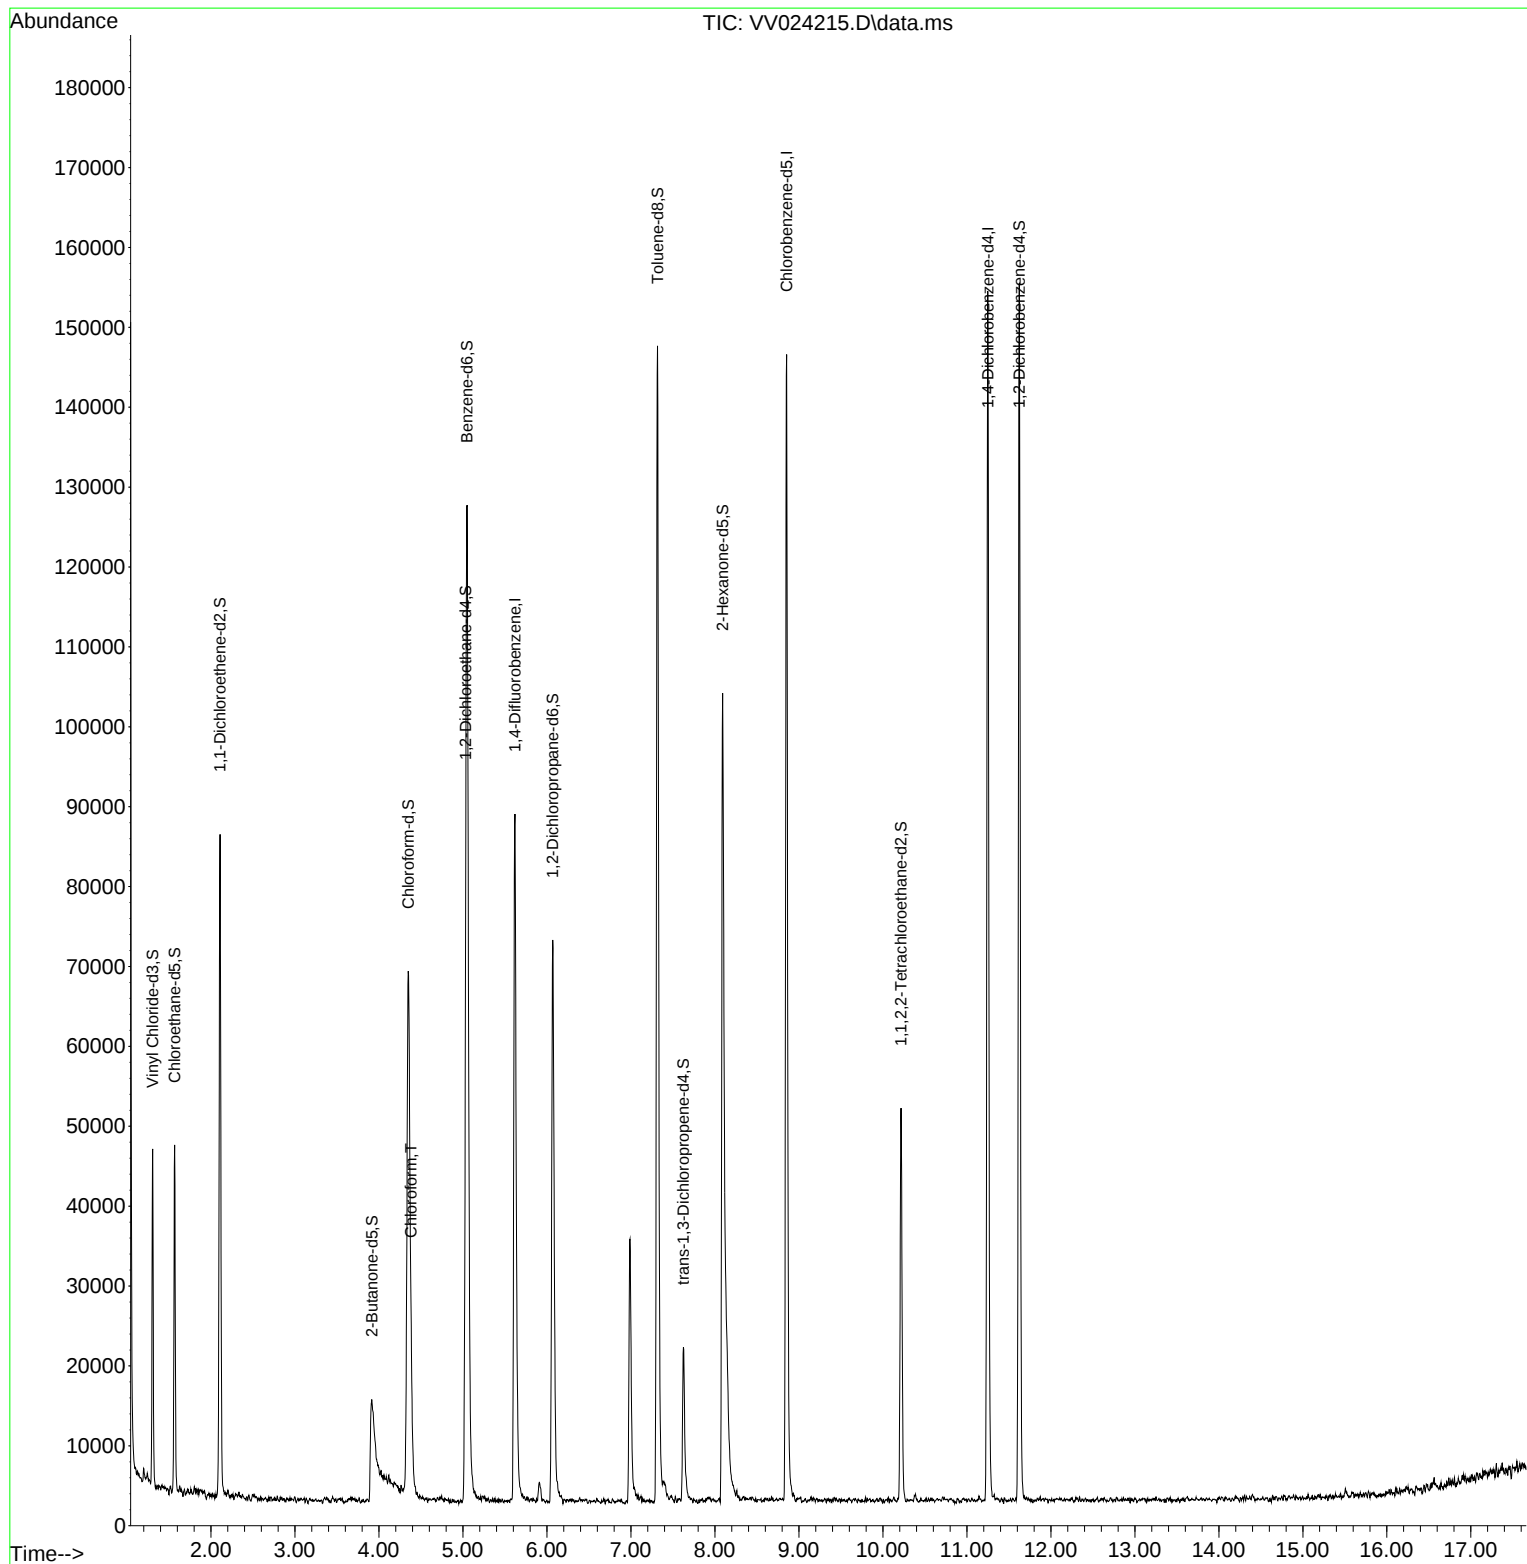

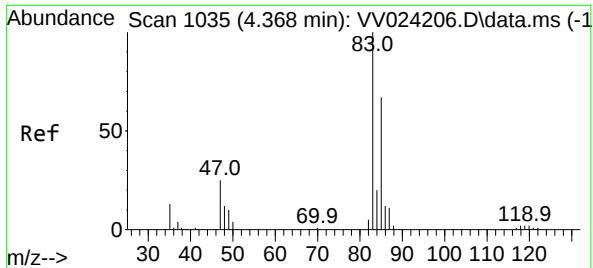

#25
 Chloroform
 Concen: 0.659 ug/L
 RT: 4.381 min Scan# 10
 Delta R.T. 0.006 min
 Lab File: VV024215.D
 Acq: 28 Dec 2021 14:00

Instrument :
 MSVOA_V
 ClientSampleId :
 P036-TW001-01

Tgt Ion: 83 Resp: 13892
 Ion Ratio Lower Upper
 83 100
 85 69.4 45.2 84.0

