

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW122821\
 Data File : VW024222.D
 Acq On : 28 Dec 2021 16:47
 Operator : SY/MD
 Sample : M5193-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J29

Quant Time: Dec 29 05:06:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 29 04:43:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	81098	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	87548	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	43892	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	27869	4.569	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	91.400%	
7) Chloroethane-d5	1.568	69	26538	5.217	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	104.400%	
11) 1,1-Dichloroethene-d2	2.108	63	45818	3.090	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	61.800%	
20) 2-Butanone-d5	3.905	46	53179	78.484	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	156.960%#	
24) Chloroform-d	4.349	84	65783	5.080	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.600%	
26) 1,2-Dichloroethane-d4	5.034	65	32403	5.590	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	111.800%	
32) Benzene-d6	5.050	84	119008	5.034	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.600%	
36) 1,2-Dichloropropane-d6	6.069	67	33762	5.213	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.200%	
41) Toluene-d8	7.317	98	103314	4.434	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.600%	
43) trans-1,3-Dichloroprop...	7.625	79	12372	4.512	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.200%	
46) 2-Hexanone-d5	8.092	63	47638	51.666	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	103.340%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	22289	5.041	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	100.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	43375	5.685	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	113.800%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.240	50	1433	0.101	ug/L	96
42) Toluene	7.394	91	4995	0.097	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024222.D
Acq On : 28 Dec 2021 16:47
Operator : SY/MD
Sample : M5193-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J29

Quant Time: Dec 29 05:06:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 29 04:43:10 2021
Response via : Initial Calibration




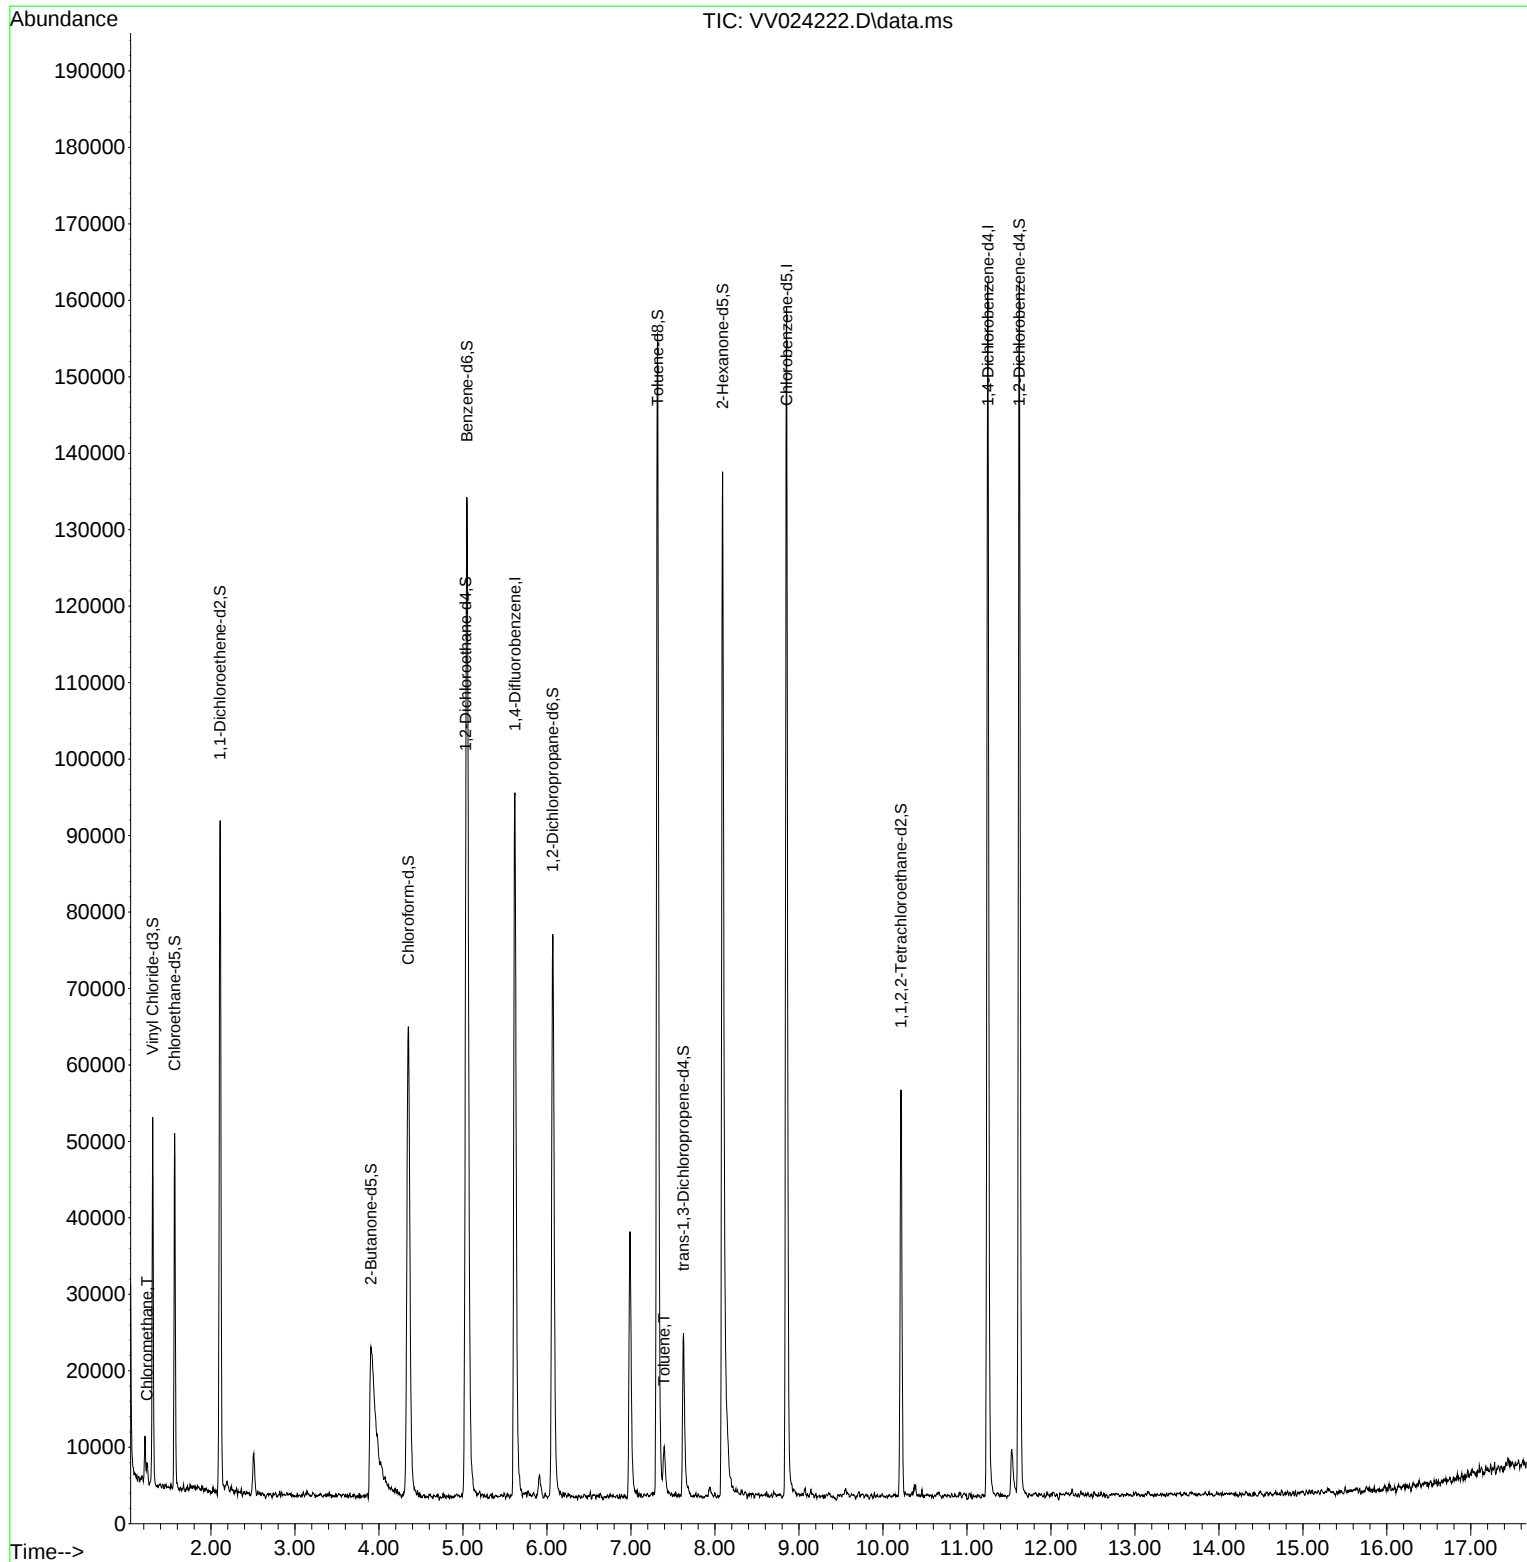


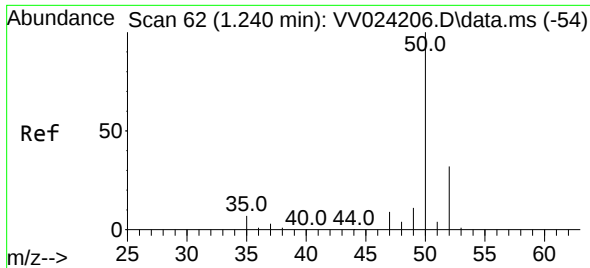

#3
Chloromethane
Concen: 0.101 ug/L
RT: 1.240 min Scan# 61
Delta R.T. 0.000 min
Lab File: VV024222.D
Acq: 28 Dec 2021 16:47

Instrument :
MSVOA_V
ClientSampleId :
C0J29

Tgt Ion: 50 Resp: 1433
Ion Ratio Lower Upper
50 100
52 33.5 22.0 41.0

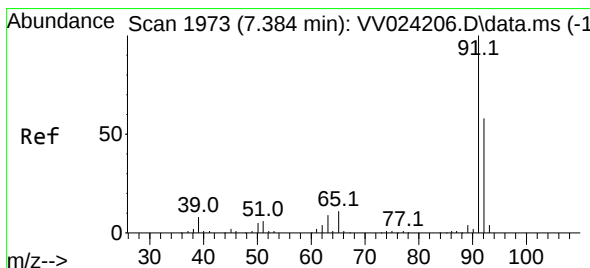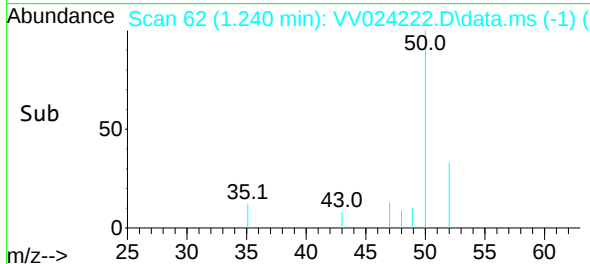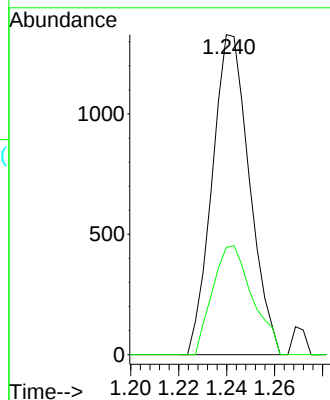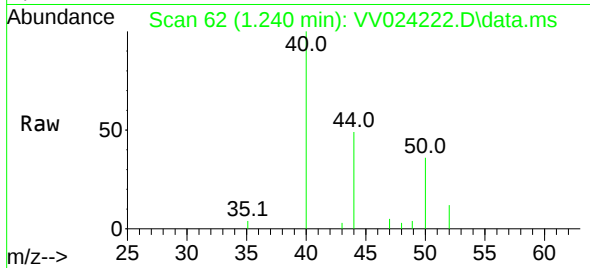

#42
Toluene
Concen: 0.097 ug/L
RT: 7.394 min Scan# 1976
Delta R.T. 0.007 min
Lab File: VV024222.D
Acq: 28 Dec 2021 16:47

Tgt Ion: 91 Resp: 4995
Ion Ratio Lower Upper
91 100
92 56.4 41.5 77.1

