

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
 Data File : VV024210.D
 Acq On : 28 Dec 2021 12:01
 Operator : SY/MD
 Sample : M5201-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 TB-211221-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024210.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	72	82	94	rVB2	48580	58882	18.75%	2.362%
2	1.565	153	163	178	rBV	42596	49159	15.65%	1.972%
3	2.105	320	331	345	rBV	80598	117165	37.30%	4.700%
4	2.507	449	456	467	rBB5	4562	6971	2.22%	0.280%
5	3.912	882	893	904	rBV2	12981	37878	12.06%	1.520%
6	4.349	1013	1029	1058	rVB3	64052	189183	60.23%	7.589%
7	5.047	1229	1246	1273	rBV2	124036	314098	100.00%	12.600%
8	5.616	1412	1423	1444	rBV	82134	166274	52.94%	6.670%
9	5.912	1501	1515	1523	rBV5	3595	7462	2.38%	0.299%
10	6.069	1551	1564	1586	rBV2	70638	146081	46.51%	5.860%
11	6.989	1839	1850	1866	rBV2	32346	62324	19.84%	2.500%
12	7.317	1940	1952	1968	rBV	146992	255277	81.27%	10.241%
13	7.394	1968	1976	1992	rVB	13796	25855	8.23%	1.037%
14	7.625	2037	2048	2061	rBV2	18805	35205	11.21%	1.412%
15	7.940	2136	2146	2156	rVB4	2253	3656	1.16%	0.147%
16	8.092	2182	2193	2232	rBV	98684	260043	82.79%	10.432%
17	8.854	2417	2430	2447	rBV	134979	224303	71.41%	8.998%
18	10.217	2840	2854	2870	rBV2	46903	74903	23.85%	3.005%
19	10.384	2897	2906	2915	rBV	2685	3732	1.19%	0.150%
20	11.249	3164	3175	3191	rBV	144819	219858	70.00%	8.820%
21	11.625	3276	3292	3310	rBV	145857	234436	74.64%	9.405%




Sum of corrected areas: 2492745

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024210.D
Acq On : 28 Dec 2021 12:01
Operator : SY/MD
Sample : M5201-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
TB-211221-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

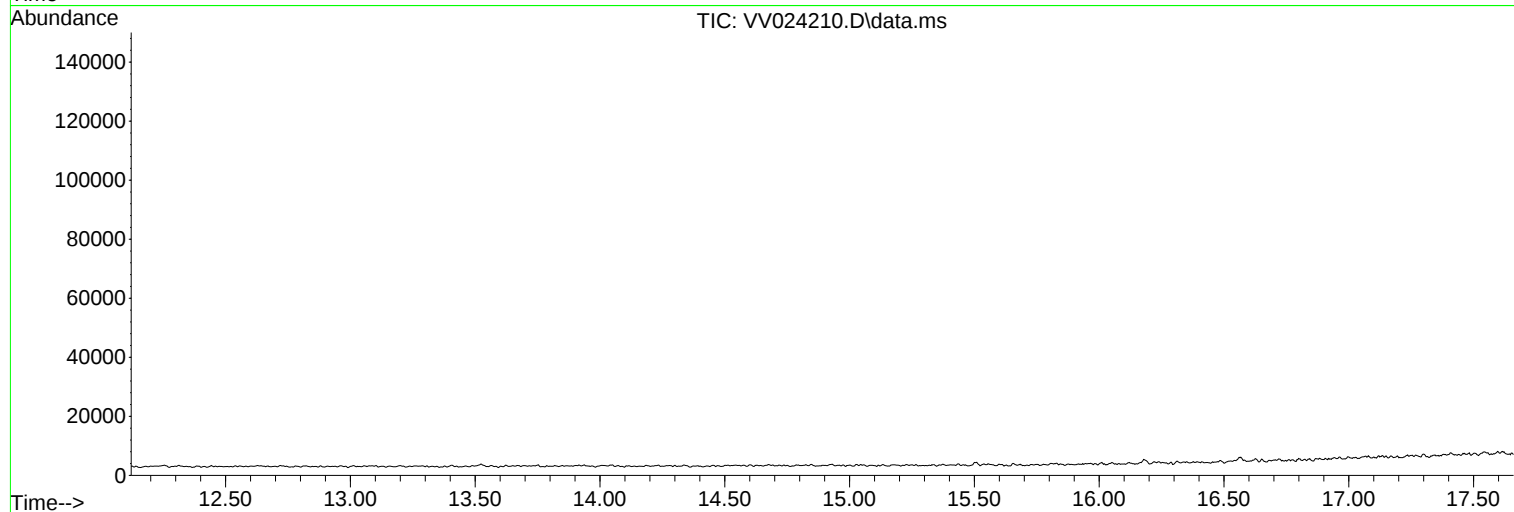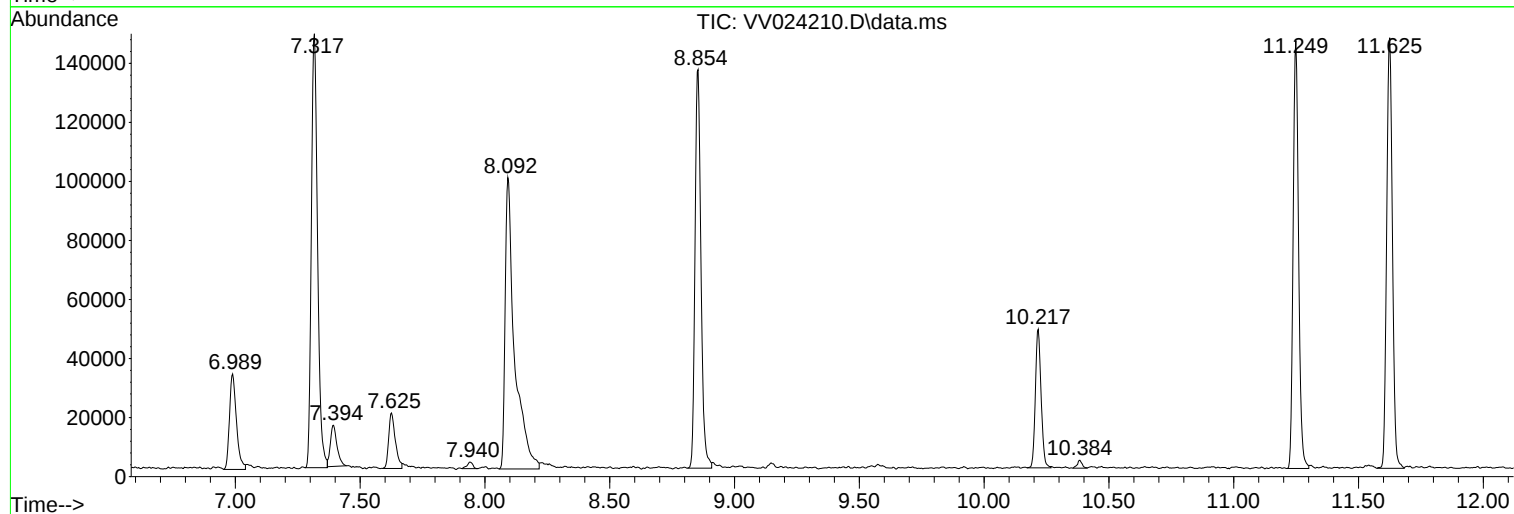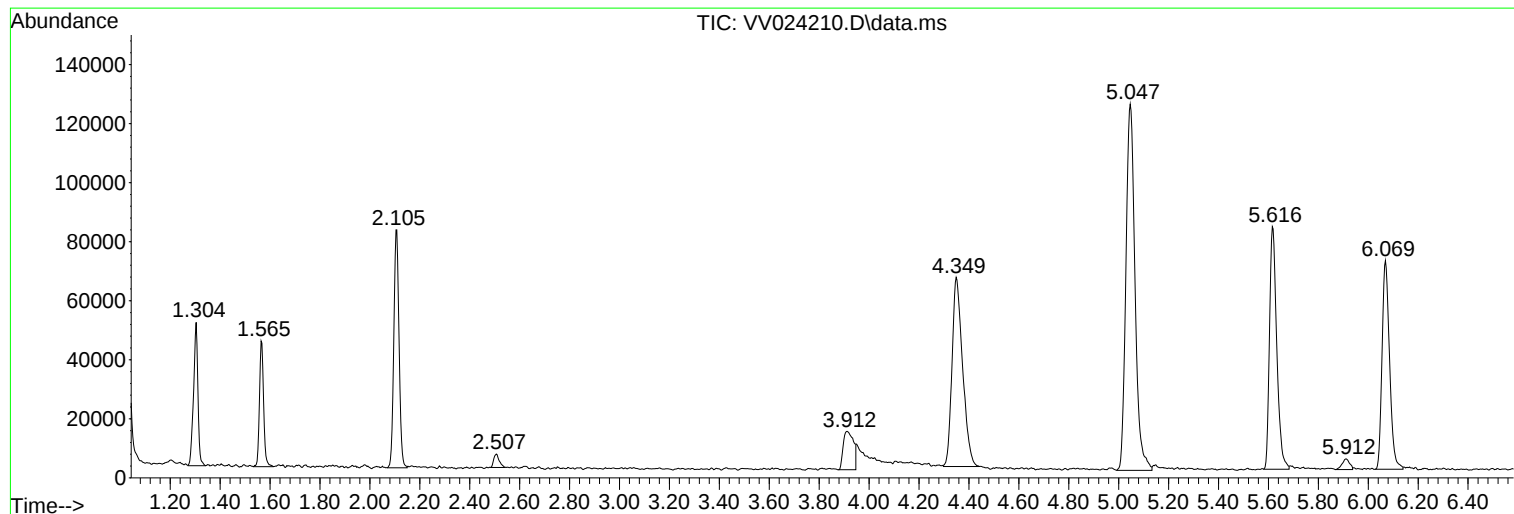

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024210.D
Acq On : 28 Dec 2021 12:01
Operator : SY/MD
Sample : M5201-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
TB-211221-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024210.D
Acq On : 28 Dec 2021 12:01
Operator : SY/MD
Sample : M5201-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
TB-211221-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
