

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
 Data File : VV024213.D
 Acq On : 28 Dec 2021 13:13
 Operator : SY/MD
 Sample : M5201-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 P033-TW001-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	92	rVB	44433	46691	14.33%	1.862%
2	1.568	156	164	177	rBV	43753	48996	15.03%	1.954%
3	2.108	320	332	349	rBV	87406	125145	38.40%	4.991%
4	3.912	883	893	911	rBV2	13640	47222	14.49%	1.883%
5	4.098	944	951	961	rVB5	2369	4374	1.34%	0.174%
6	4.349	1015	1029	1052	rVB2	60454	149090	45.75%	5.945%
7	5.047	1229	1246	1273	rBV3	128631	325909	100.00%	12.997%
8	5.619	1412	1424	1449	rBV	87686	176806	54.25%	7.051%
9	5.911	1507	1515	1520	rBV4	2182	3517	1.08%	0.140%
10	6.069	1552	1564	1583	rBV2	73641	150194	46.08%	5.989%
11	6.989	1840	1850	1866	rBV2	34166	64155	19.68%	2.558%
12	7.317	1941	1952	1973	rBV	153346	268830	82.49%	10.720%
13	7.625	2040	2048	2062	rBV2	20371	35136	10.78%	1.401%
14	8.091	2183	2193	2230	rBV	106461	266805	81.86%	10.640%
15	8.853	2419	2430	2456	rVB	141923	233137	71.53%	9.297%
16	10.217	2843	2854	2867	rBV	51272	80442	24.68%	3.208%
17	11.249	3164	3175	3190	rBV	149746	230869	70.84%	9.207%
18	11.625	3276	3292	3306	rBV	156589	246677	75.69%	9.837%
19	16.557	4819	4826	4835	rBV7	2416	3638	1.12%	0.145%




Sum of corrected areas: 2507633

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024213.D
Acq On : 28 Dec 2021 13:13
Operator : SY/MD
Sample : M5201-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P033-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

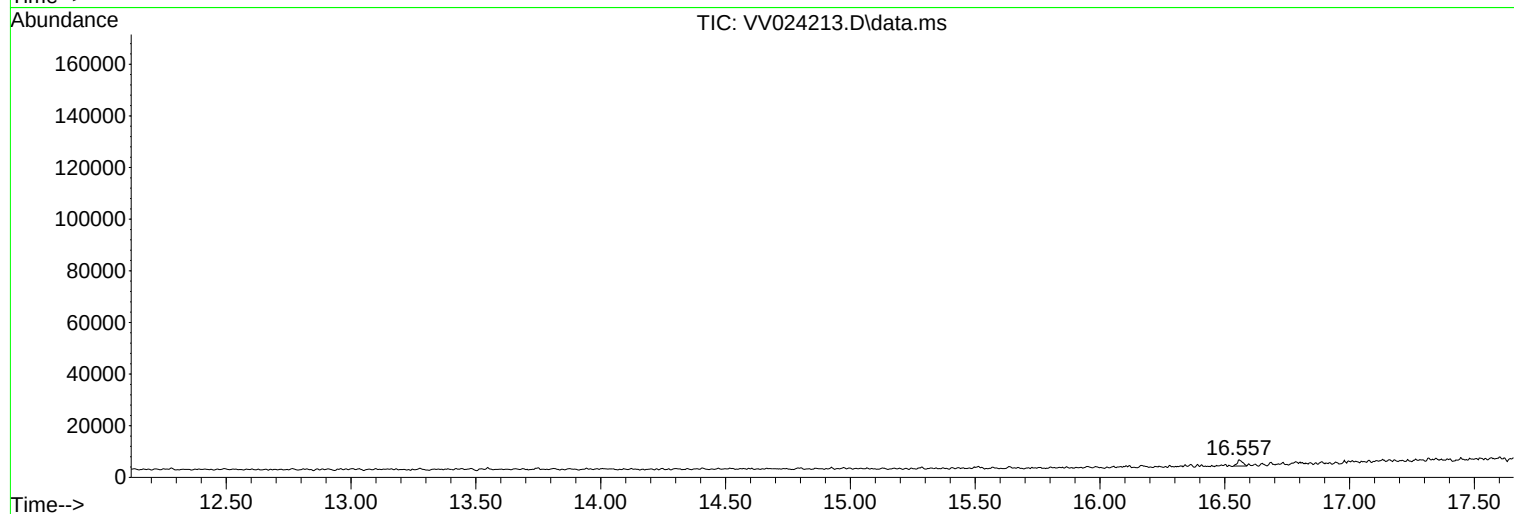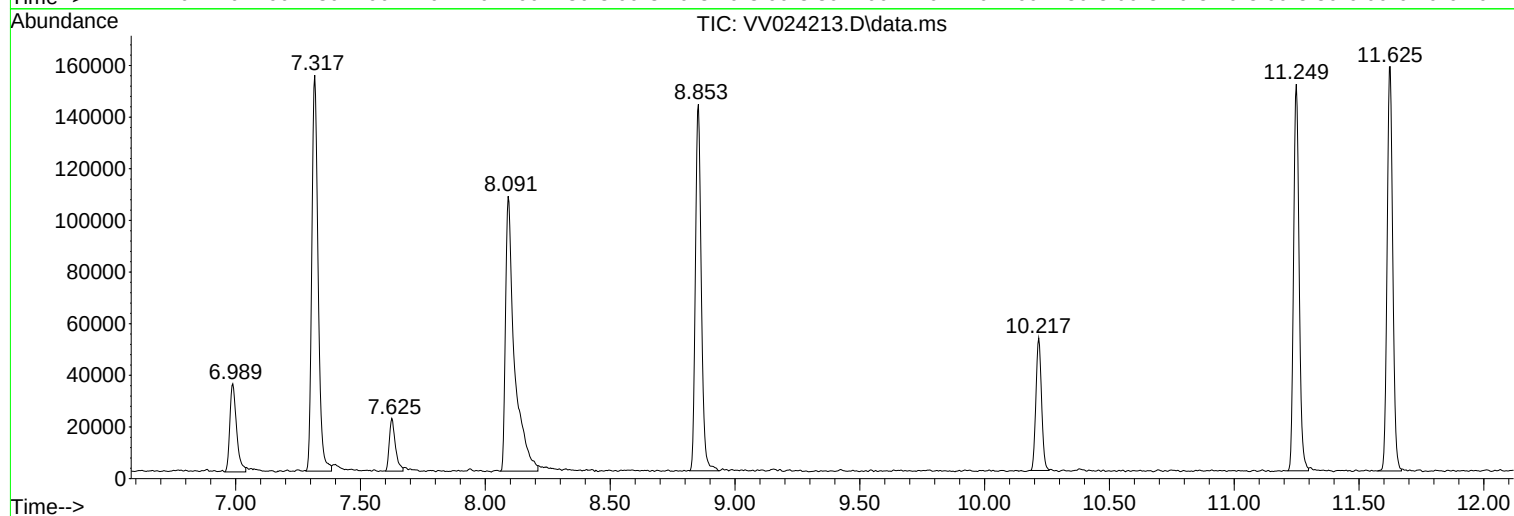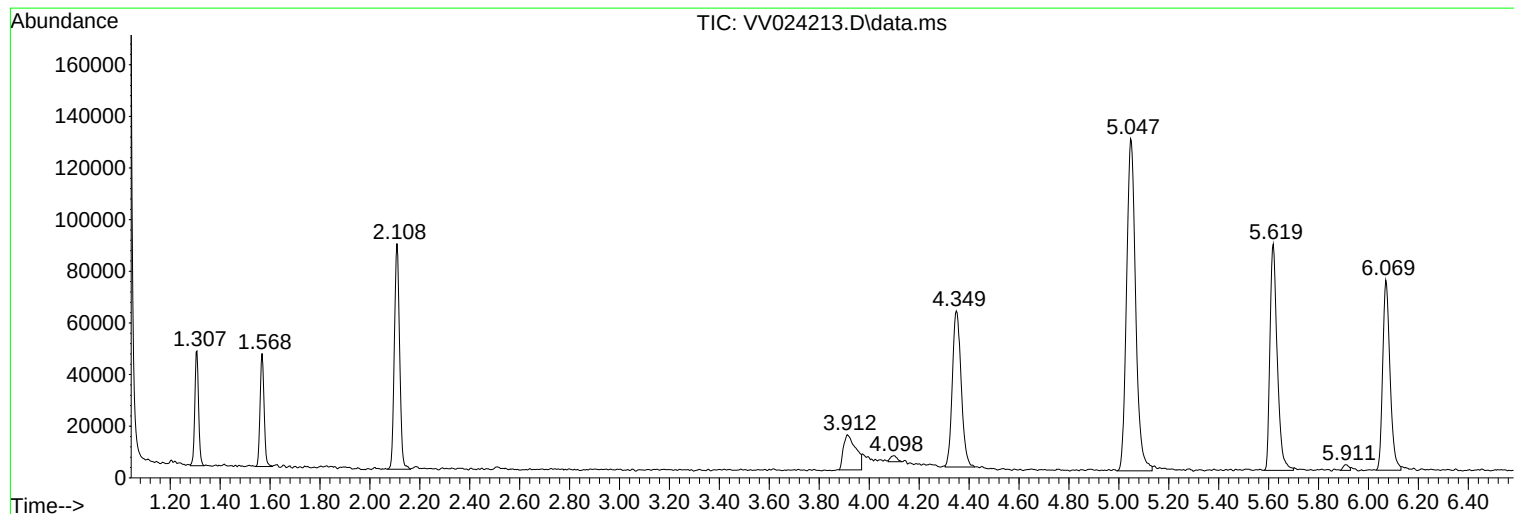

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024213.D
Acq On : 28 Dec 2021 13:13
Operator : SY/MD
Sample : M5201-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P033-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024213.D
Acq On : 28 Dec 2021 13:13
Operator : SY/MD
Sample : M5201-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
P033-TW001-02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc