

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
 Data File : VV024223.D
 Acq On : 28 Dec 2021 17:11
 Operator : SY/MD
 Sample : M5193-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J30

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV024223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	49	54	60	rVB2	6558	5790	1.87%	0.231%
2	1.307	74	83	95	rVB	44981	47403	15.34%	1.893%
3	1.568	157	164	176	rBV	44025	49444	16.01%	1.974%
4	2.108	322	332	347	rBV	83463	117592	38.06%	4.695%
5	2.510	446	457	465	rBV2	4095	6887	2.23%	0.275%
6	3.905	881	891	914	rBV	16317	62683	20.29%	2.503%
7	4.349	1014	1029	1051	rBV2	60742	147317	47.69%	5.882%
8	5.047	1231	1246	1269	rBV2	122489	308927	100.00%	12.334%
9	5.619	1411	1424	1448	rBV	89444	183966	59.55%	7.345%
10	5.915	1504	1516	1529	rBV6	3224	7603	2.46%	0.304%
11	6.069	1546	1564	1589	rBV	70394	146842	47.53%	5.863%
12	6.989	1840	1850	1868	rBV	31546	58361	18.89%	2.330%
13	7.317	1940	1952	1967	rBV	145332	252809	81.83%	10.094%
14	7.397	1971	1977	1988	rVB3	6758	11167	3.61%	0.446%
15	7.625	2039	2048	2063	rBV2	18429	33555	10.86%	1.340%
16	8.092	2183	2193	2225	rBV	108391	252527	81.74%	10.082%
17	8.854	2414	2430	2447	rBV	149243	245951	79.61%	9.820%
18	10.217	2839	2854	2870	rVB2	49587	78622	25.45%	3.139%
19	11.249	3164	3175	3197	rBV	153732	234701	75.97%	9.371%
20	11.532	3254	3263	3275	rBV3	8735	17685	5.72%	0.706%
21	11.622	3281	3291	3311	rVB	151523	234776	76.00%	9.374%




Sum of corrected areas: 2504608

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024223.D
Acq On : 28 Dec 2021 17:11
Operator : SY/MD
Sample : M5193-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

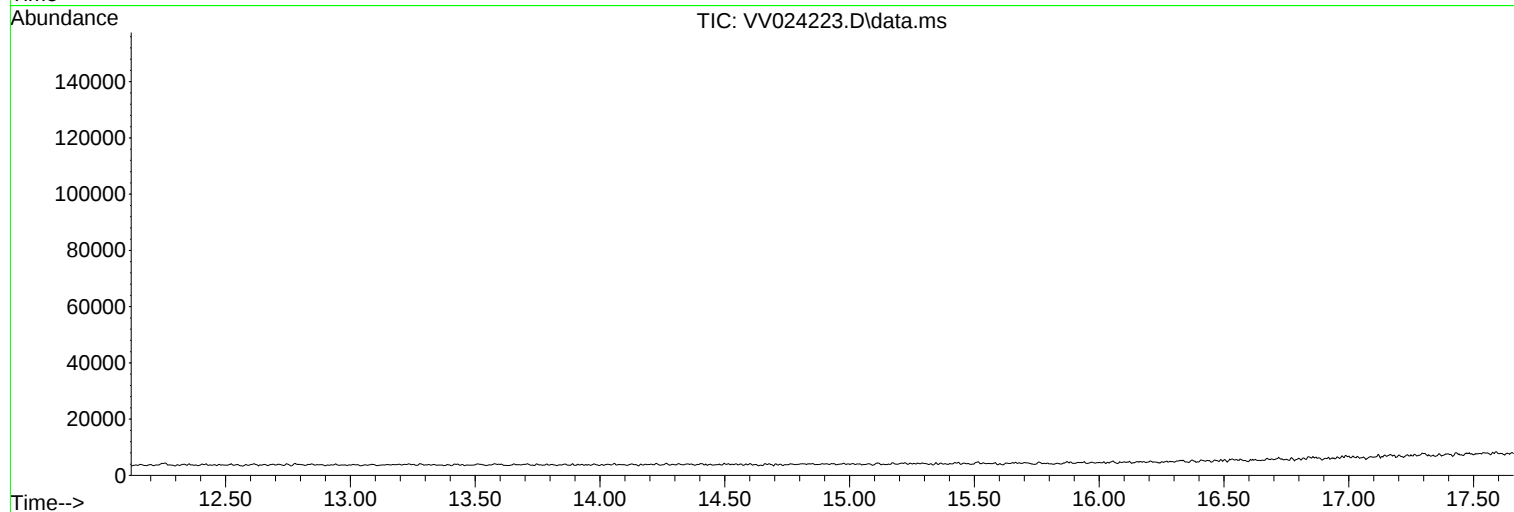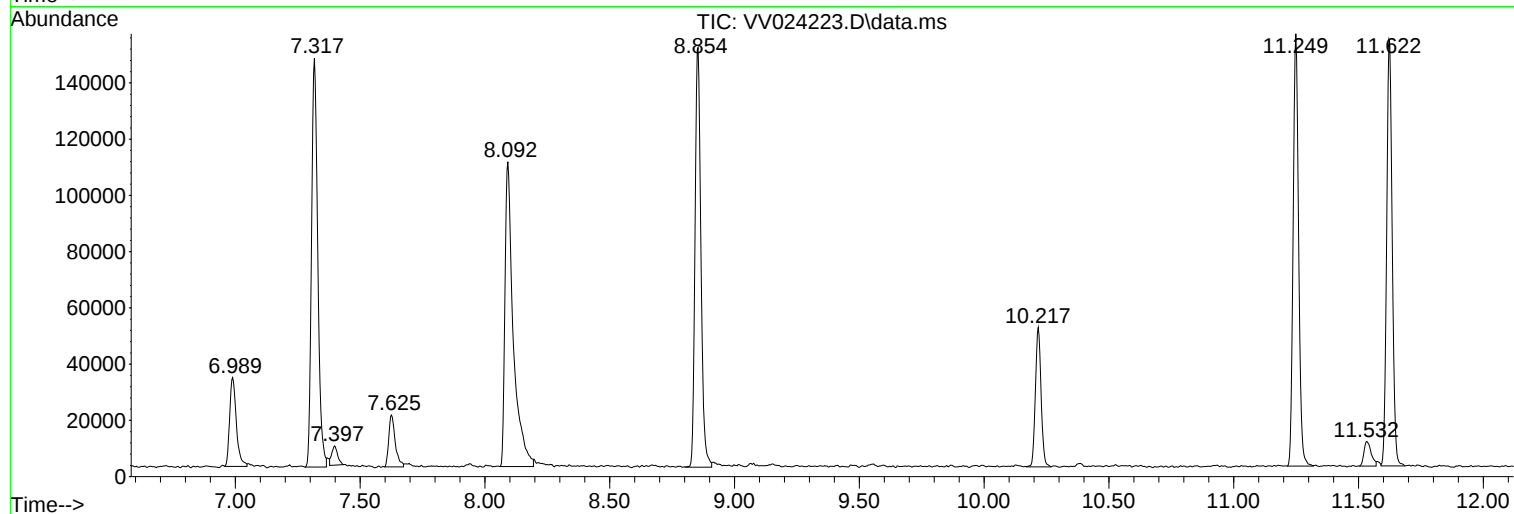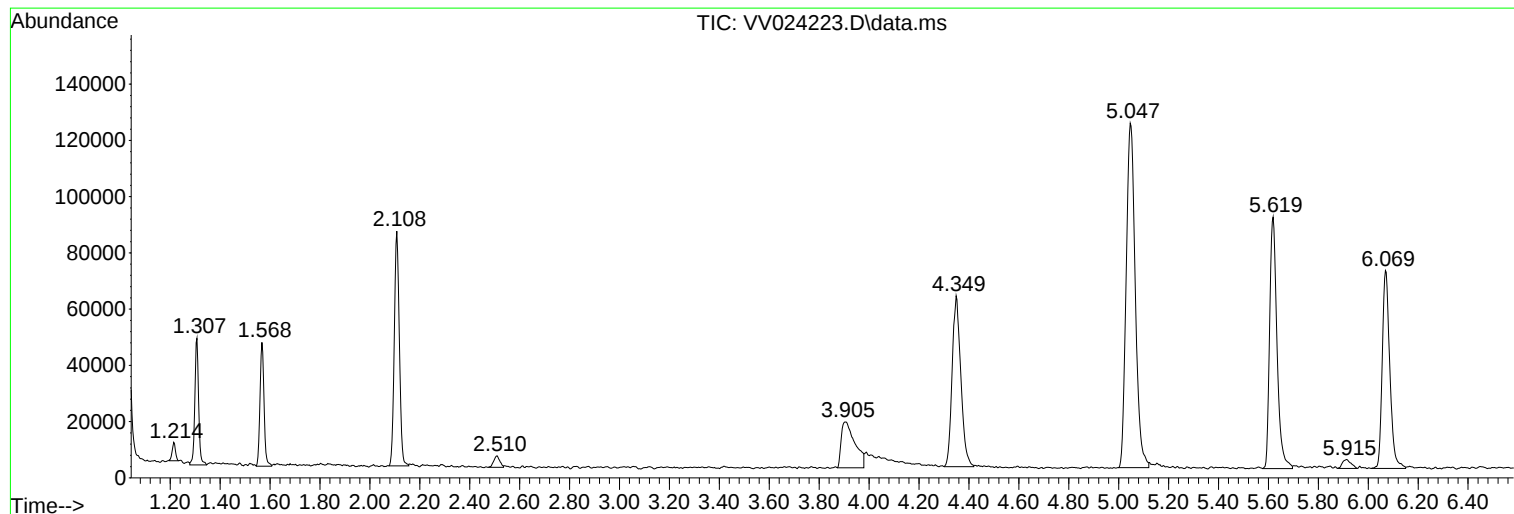

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024223.D
Acq On : 28 Dec 2021 17:11
Operator : SY/MD
Sample : M5193-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024223.D
Acq On : 28 Dec 2021 17:11
Operator : SY/MD
Sample : M5193-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc