

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
 Data File : VV024224.D
 Acq On : 28 Dec 2021 17:35
 Operator : SY/MD
 Sample : M5193-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J07

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	96	rVB3	64803	82594	4.96%	1.350%
2	1.571	157	165	176	rBV	49820	62234	3.73%	1.017%
3	2.117	322	335	352	rVB2	602108	945780	56.76%	15.453%
4	3.191	653	669	689	rBV	125491	263934	15.84%	4.312%
5	3.908	878	892	922	rBV3	43436	156512	9.39%	2.557%
6	4.349	1013	1029	1054	rBV2	72590	177256	10.64%	2.896%
7	4.609	1091	1110	1134	rBV2	162915	407031	24.43%	6.651%
8	5.046	1230	1246	1268	rBV2	148317	371889	22.32%	6.076%
9	5.619	1411	1424	1441	rBV	86751	177258	10.64%	2.896%
10	5.911	1501	1515	1547	rBV	862176	1666308	100.00%	27.226%
11	6.069	1552	1564	1588	rVB2	87990	182345	10.94%	2.979%
12	6.989	1836	1850	1866	rBV2	40244	74703	4.48%	1.221%
13	7.316	1941	1952	1970	rBV	176968	301865	18.12%	4.932%
14	7.625	2038	2048	2068	rVB2	23943	43882	2.63%	0.717%
15	8.088	2183	2192	2229	rBV	163508	315144	18.91%	5.149%
16	8.853	2419	2430	2456	rBV	145521	240202	14.42%	3.925%
17	10.217	2839	2854	2870	rBV	65123	102932	6.18%	1.682%
18	11.249	3165	3175	3194	rBV	155170	237892	14.28%	3.887%
19	11.532	3253	3263	3275	rBV2	13032	23555	1.41%	0.385%
20	11.625	3281	3292	3306	rBV	181139	286917	17.22%	4.688%




Sum of corrected areas: 6120233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024224.D
Acq On : 28 Dec 2021 17:35
Operator : SY/MD
Sample : M5193-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

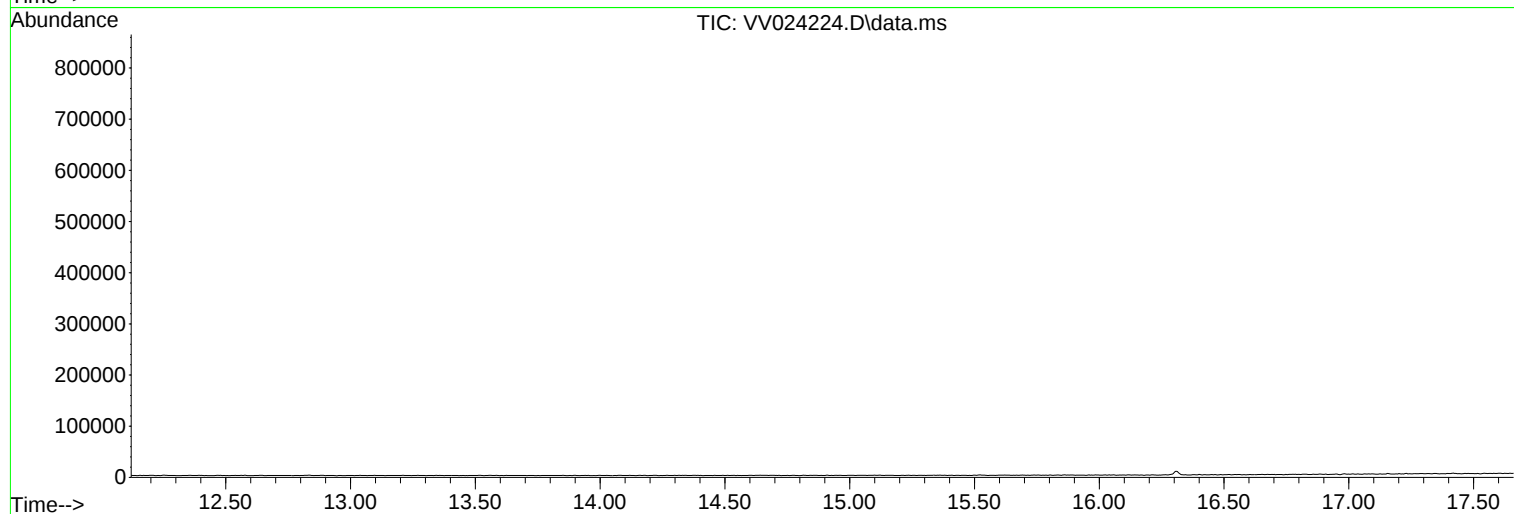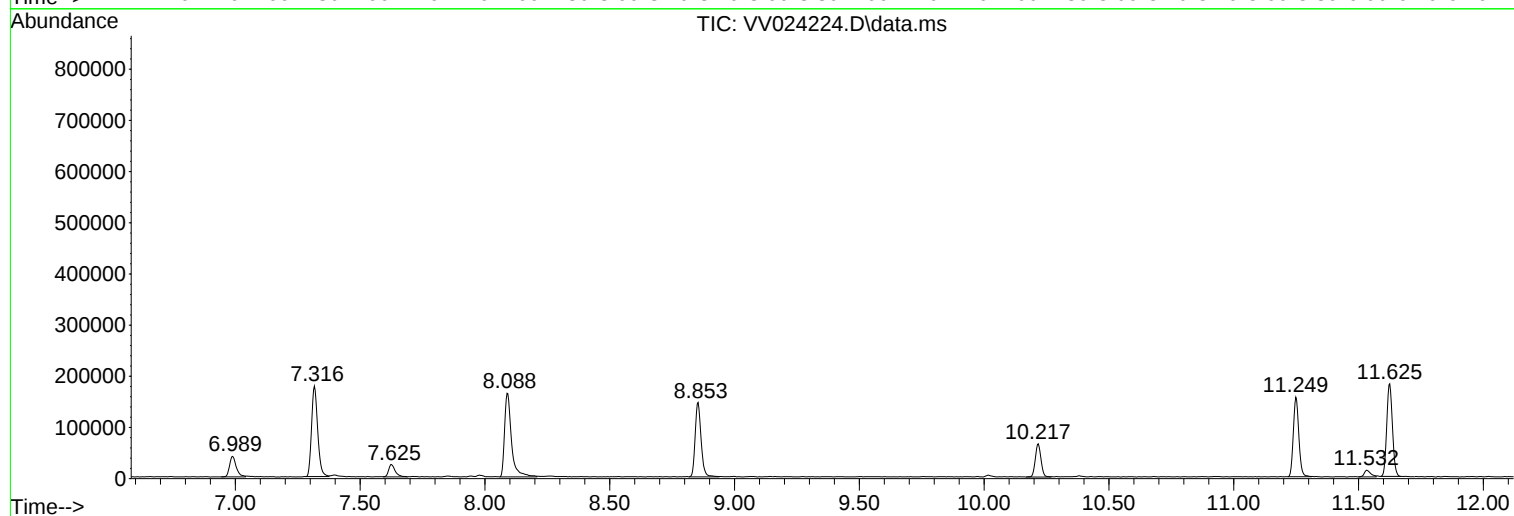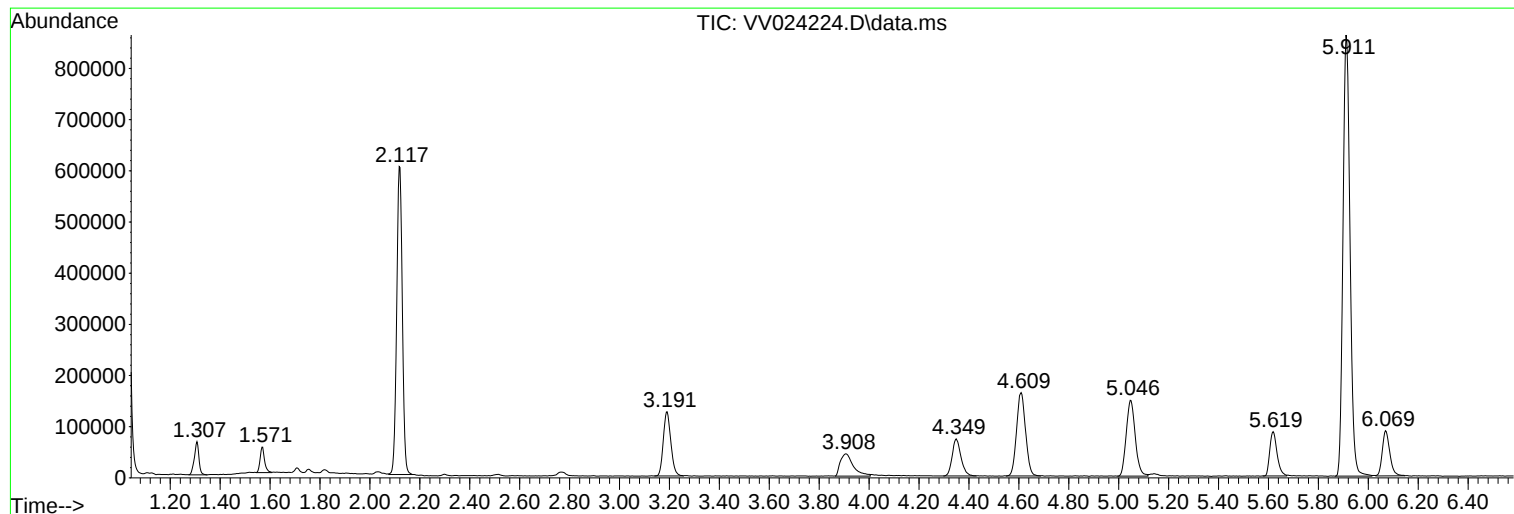

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024224.D
Acq On : 28 Dec 2021 17:35
Operator : SY/MD
Sample : M5193-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024224.D
Acq On : 28 Dec 2021 17:35
Operator : SY/MD
Sample : M5193-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
