

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
 Data File : VV024227.D
 Acq On : 28 Dec 2021 18:46
 Operator : SY/MD
 Sample : M5193-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0J33

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	42	50	73	rBV	365980	696585	100.00%	20.704%
2	1.307	76	83	87	rBV	75490	100277	14.40%	2.980%
3	1.568	159	164	174	rVB	45100	49374	7.09%	1.467%
4	2.108	324	332	346	rVB	91684	140080	20.11%	4.163%
5	2.510	448	457	470	rVB2	11650	20323	2.92%	0.604%
6	3.896	877	888	917	rBV	28516	107405	15.42%	3.192%
7	4.349	1011	1029	1051	rBV	64251	155729	22.36%	4.629%
8	5.050	1231	1247	1275	rBV3	126943	320780	46.05%	9.534%
9	5.619	1410	1424	1450	rBV2	86693	181159	26.01%	5.384%
10	6.069	1550	1564	1583	rBV2	73970	153717	22.07%	4.569%
11	6.986	1838	1849	1868	rBV2	27018	53102	7.62%	1.578%
12	7.317	1935	1952	1970	rBV	146830	261390	37.52%	7.769%
13	7.400	1970	1978	1989	rVB4	5692	10461	1.50%	0.311%
14	7.625	2040	2048	2061	rBV	16698	27857	4.00%	0.828%
15	8.088	2179	2192	2210	rBV	144782	267576	38.41%	7.953%
16	8.854	2414	2430	2456	rBV	143668	238620	34.26%	7.092%
17	10.217	2843	2854	2869	rBV	55106	87365	12.54%	2.597%
18	11.249	3164	3175	3193	rBV	152546	234192	33.62%	6.961%
19	11.535	3254	3264	3277	rBV3	6738	13349	1.92%	0.397%
20	11.625	3281	3292	3306	rVV	157901	245194	35.20%	7.288%




Sum of corrected areas: 3364535

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024227.D
Acq On : 28 Dec 2021 18:46
Operator : SY/MD
Sample : M5193-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

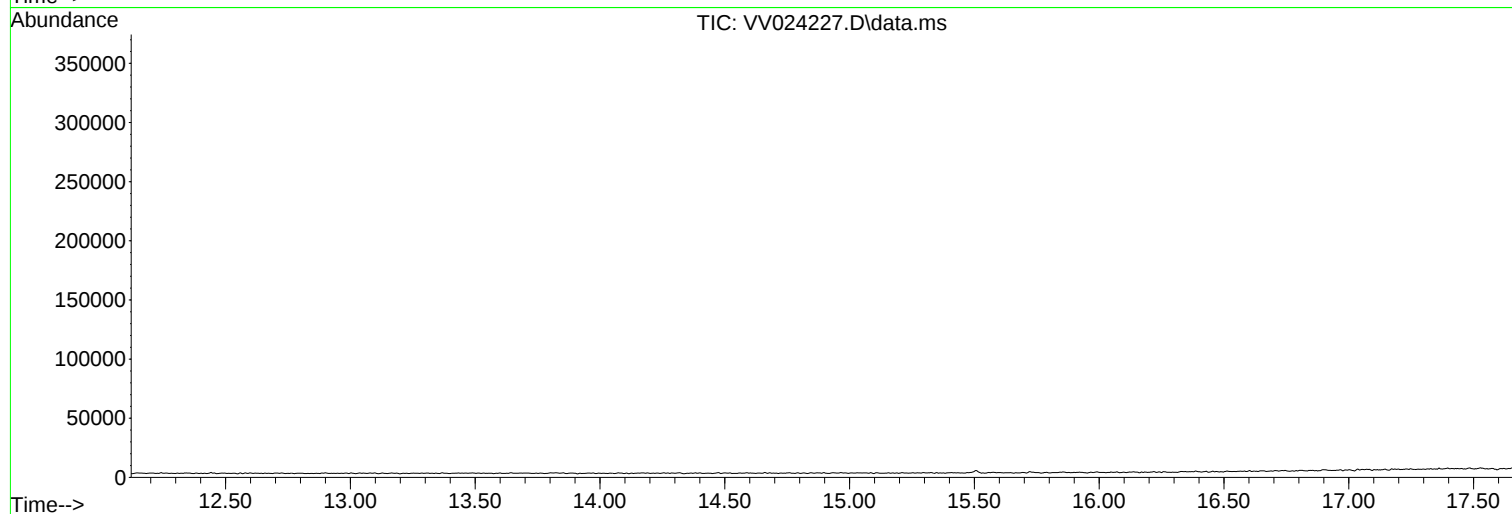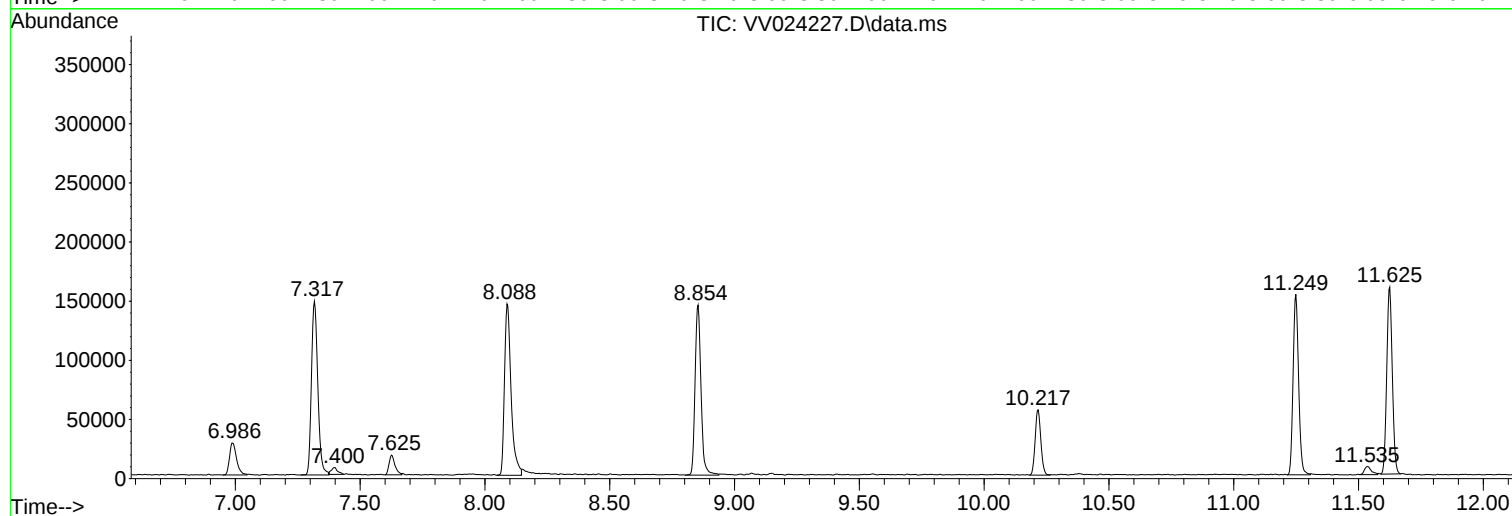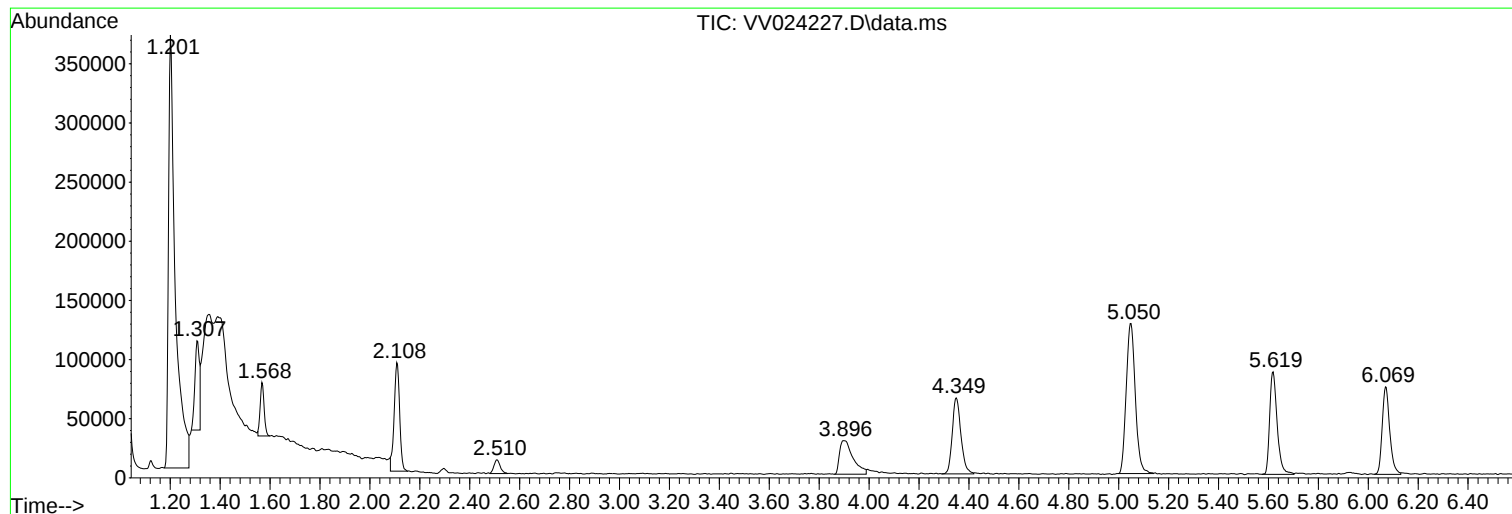

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024227.D
Acq On : 28 Dec 2021 18:46
Operator : SY/MD
Sample : M5193-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV122821\
Data File : VV024227.D
Acq On : 28 Dec 2021 18:46
Operator : SY/MD
Sample : M5193-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0J33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR122721WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc